

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 21:34
 Operator : HP/AJ
 Sample : K5076-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-02-20190926-A

Manual Integrations
 APPROVED

Ankita
 9/30/2019 1:53:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:59:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.369	3.530	1259874	914499	34.244	32.752
2) SA Decachlor...	10.029	8.397	837290	581231	18.223	16.582m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092719\
Data File : PO061445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 21:34
Operator : HP/AJ
Sample : K5076-05
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
SIMW-02-20190926-A


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:59:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

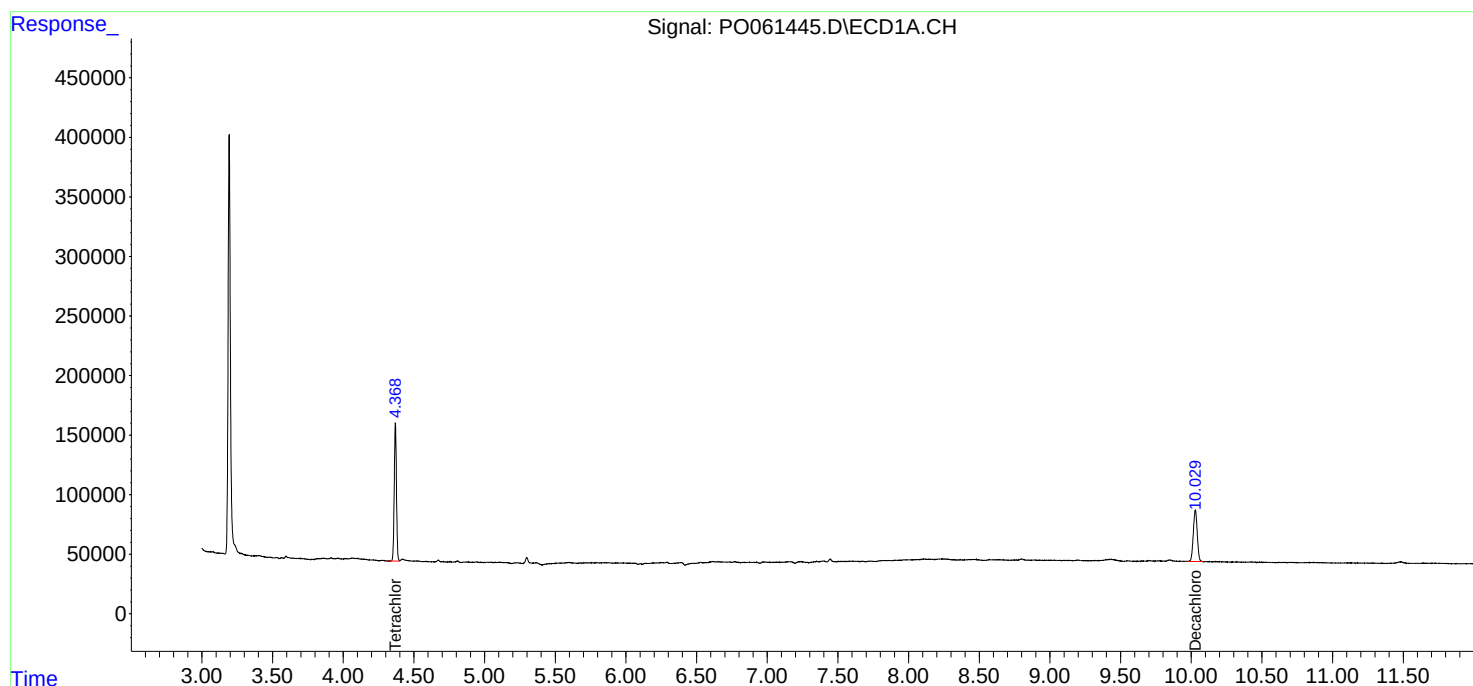

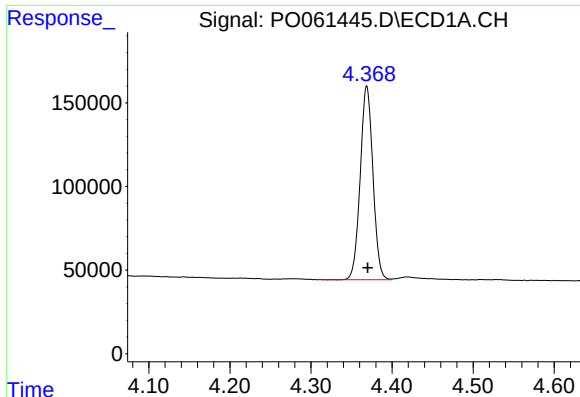


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: -0.001 min
Response: 1259874
Conc: 34.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-02-20190926-A


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:50 PM

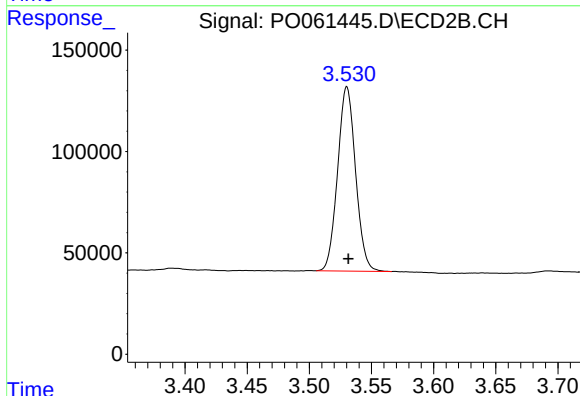


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 914499
Conc: 32.75 ng/ml

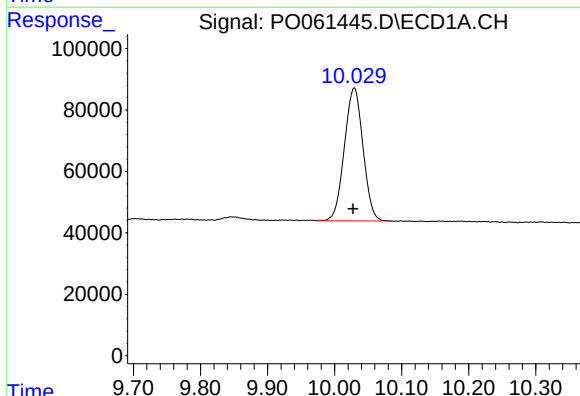

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.002 min
Response: 837290
Conc: 18.22 ng/ml

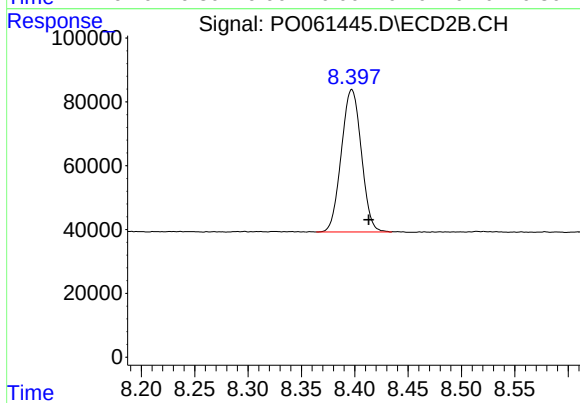

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.016 min
Response: 581231
Conc: 16.58 ng/ml m