

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 21:50
 Operator : HP/AJ
 Sample : K5076-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SIMW-04-20190926

Manual Integrations
 APPROVED

Ankita
 9/30/2019 1:53:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 00:00:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.369	3.530	1382664	972261	37.582	34.820m
2) SA Decachlor...	10.029	8.397	856086	585320	18.632	16.699m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 21:50
Operator : HP/AJ
Sample : K5076-06
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SIMW-04-20190926


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 00:00:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

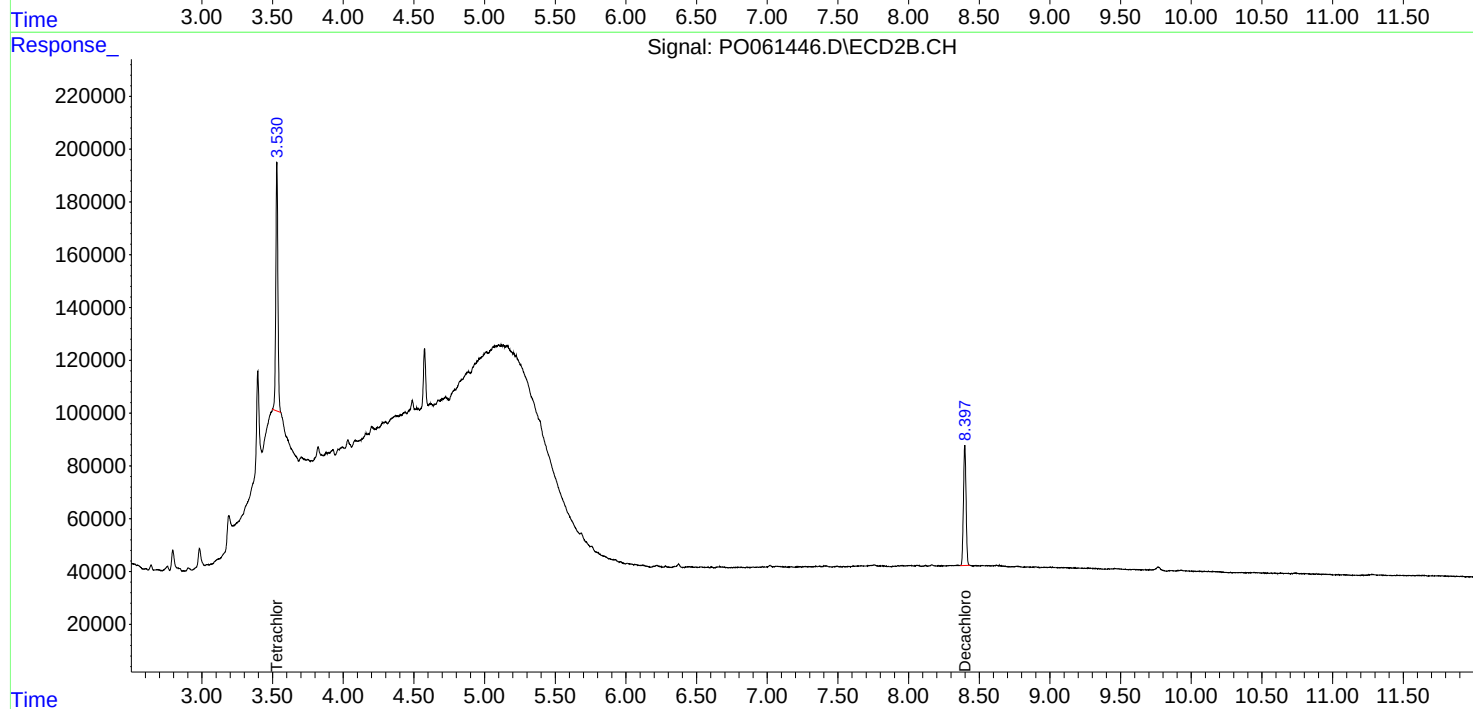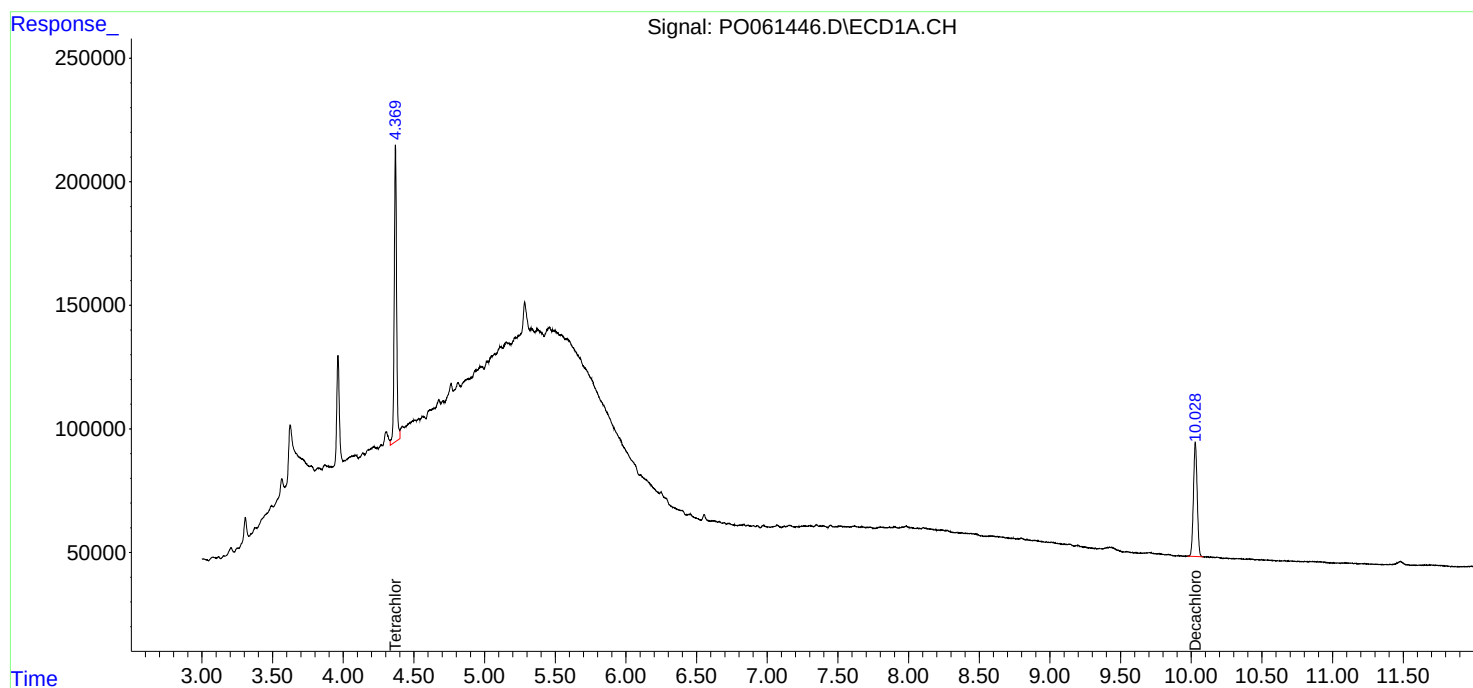

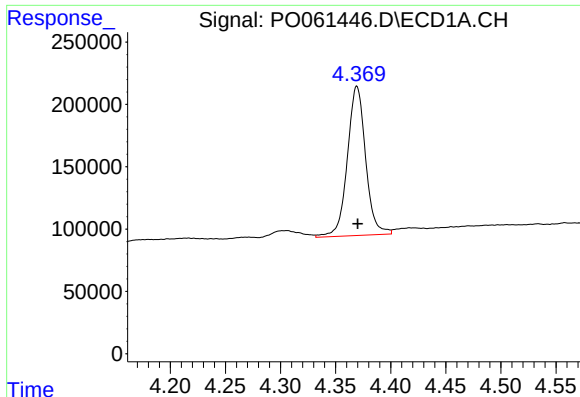


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 1382664
Conc: 37.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
SIMW-04-20190926


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:52 PM

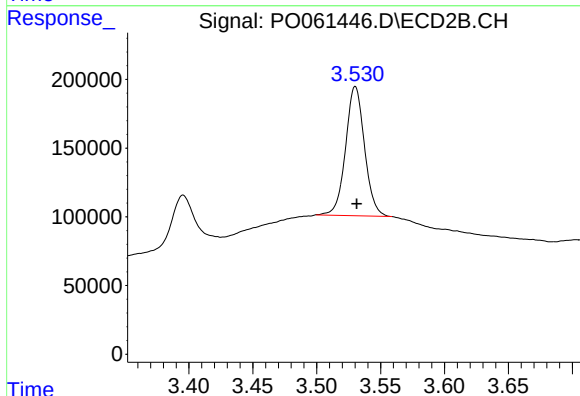


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.001 min
Response: 972261
Conc: 34.82 ng/ml m

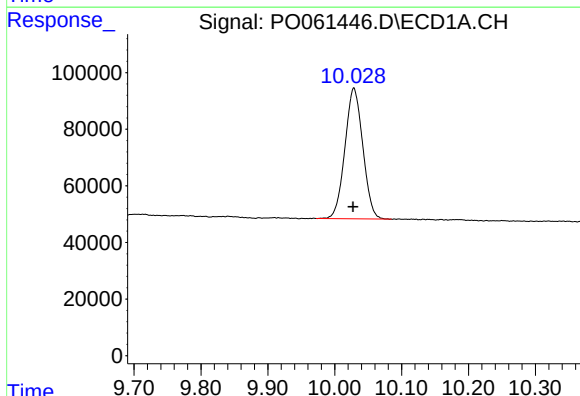

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.001 min
Response: 856086
Conc: 18.63 ng/ml

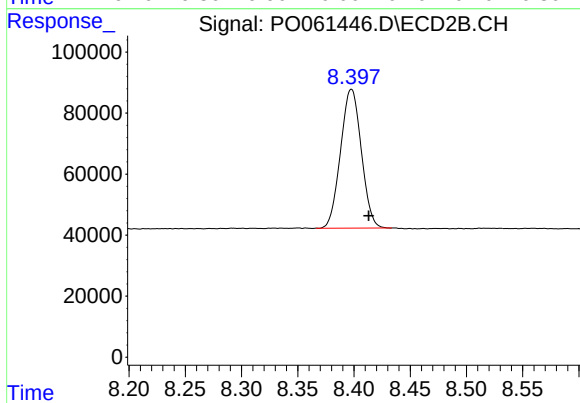

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.016 min
Response: 585320
Conc: 16.70 ng/ml m