

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061453.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2019 1:22
 Operator : HP/AJ
 Sample : K5055-01 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1-STAIRWELL-INNER-WINDOW-CA

Manual Integrations
 APPROVED

Ankita
 9/30/2019 1:54:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:46:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.526	207014	163270	5.627m	5.847
2) SA Decachlor...	10.028	8.397	222972	174238	4.853	4.971m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092719\
Data File : PO061453.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2019 1:22
Operator : HP/AJ
Sample : K5055-01 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1-STAIRWELL-INNER-WINDOW-CA


Manual Integrations
APPROVED

Ankita
9/30/2019 1:54:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:46:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

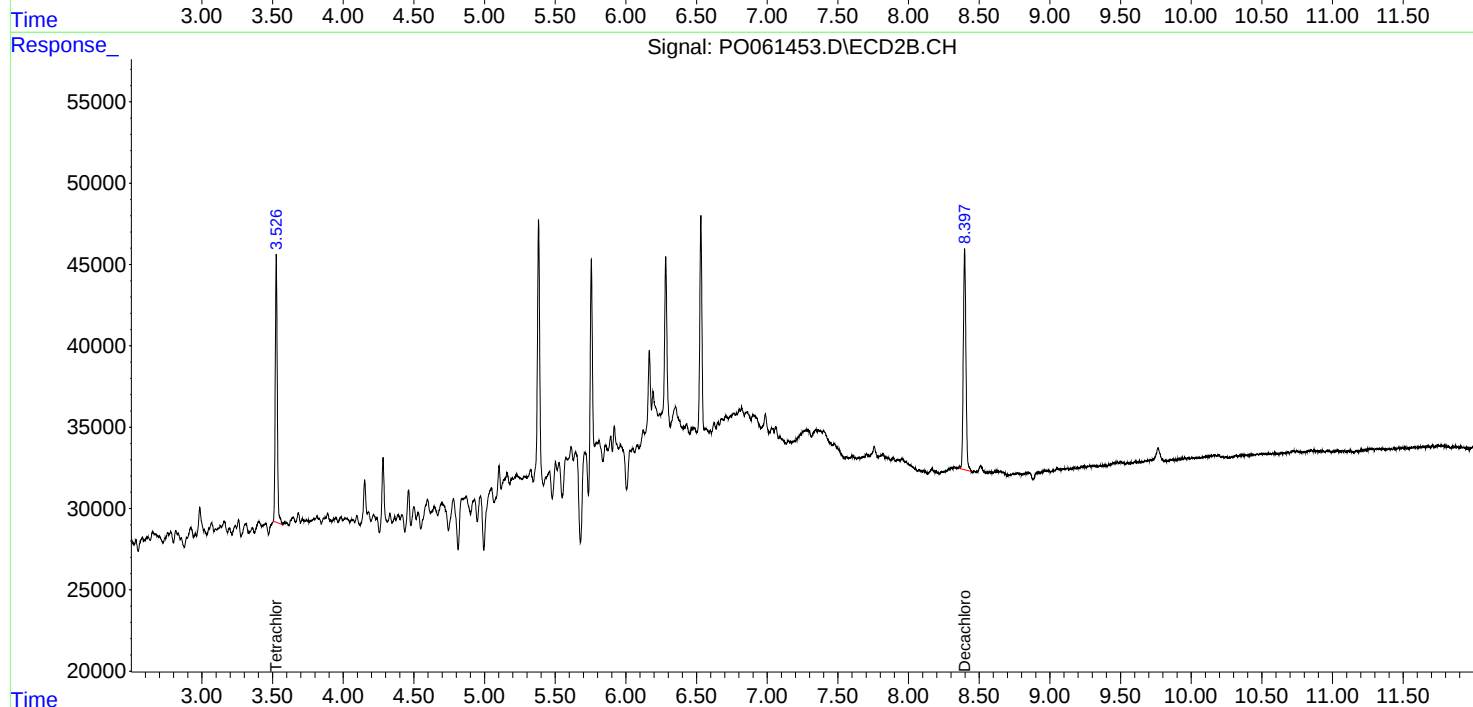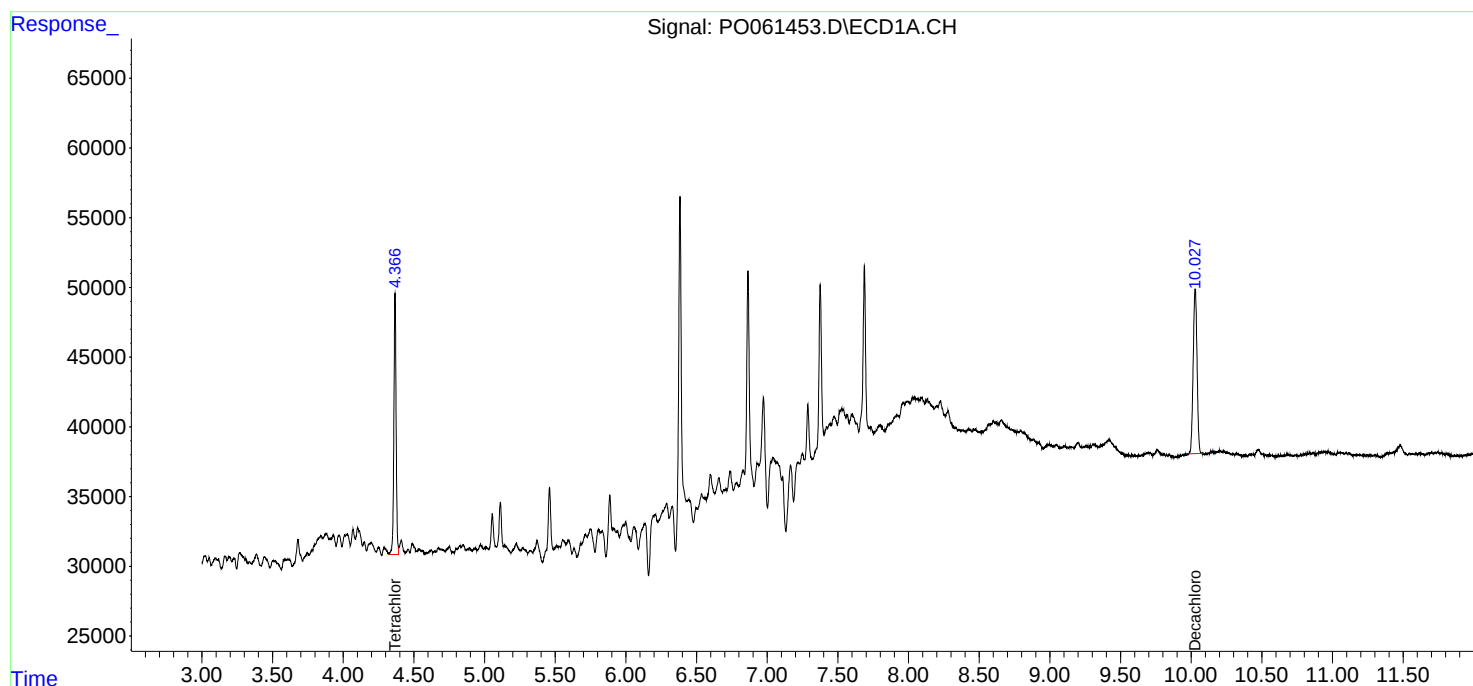

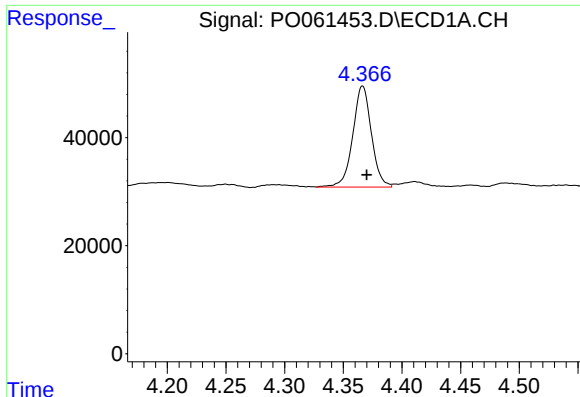


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 207014
Conc: 5.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1-STAIRWELL-INNER-WINDOW-CA


Manual Integrations
APPROVED

Ankita
9/30/2019 1:54:10 PM

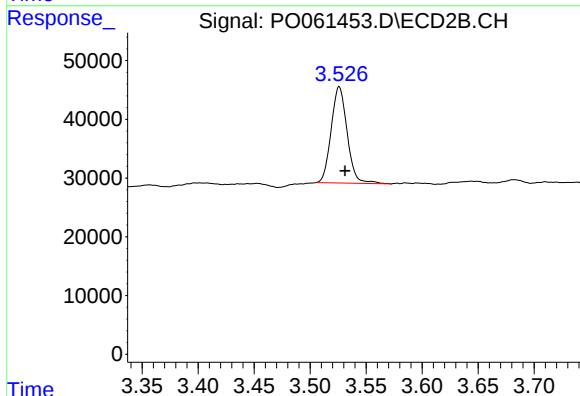


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.005 min
Response: 163270
Conc: 5.85 ng/ml

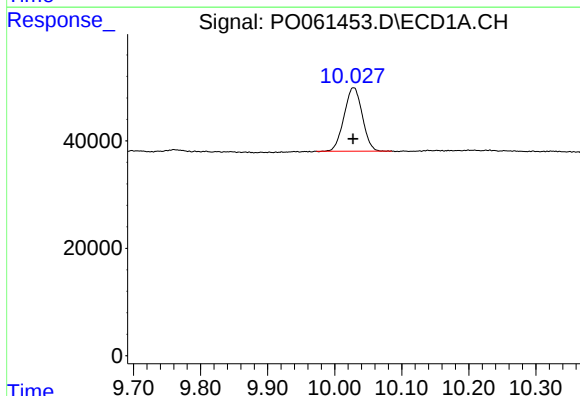

#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 222972
Conc: 4.85 ng/ml

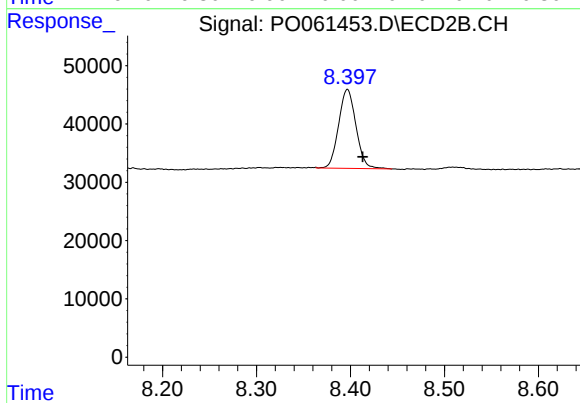

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.017 min
Response: 174238
Conc: 4.97 ng/ml m