

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092721\
 Data File : P0081570.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2021 12:39
 Operator : AJ\MA
 Sample : M3917-19RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1RE

Manual Integrations
 APPROVED

mohammad
 9/28/2021 9:31:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 03:02:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	3.984	2062635	588199	23.130m	22.078m
2) SA Decachlor...	10.879	9.331	2287709	821069	30.713	35.356

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092721\
Data File : P0081570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2021 12:39
Operator : AJ\MA
Sample : M3917-19RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1RE


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 03:02:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

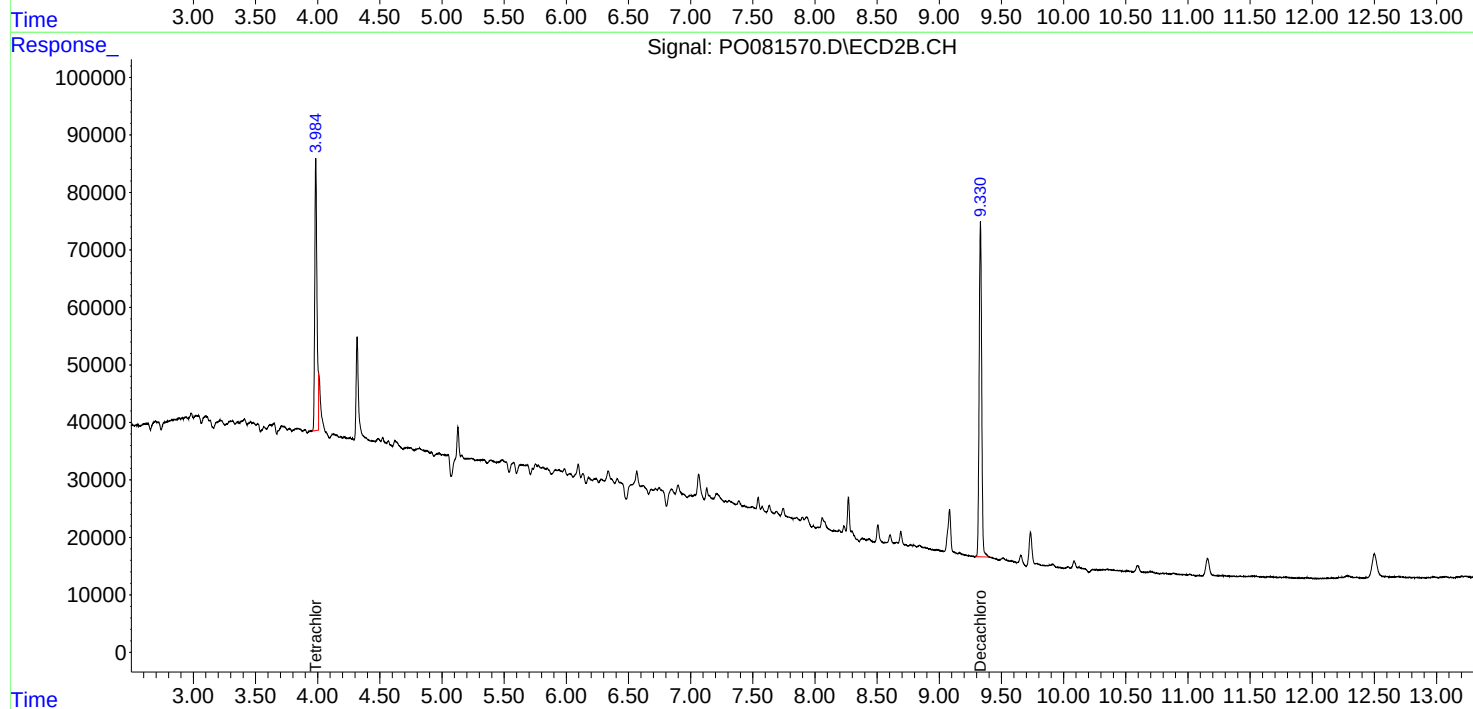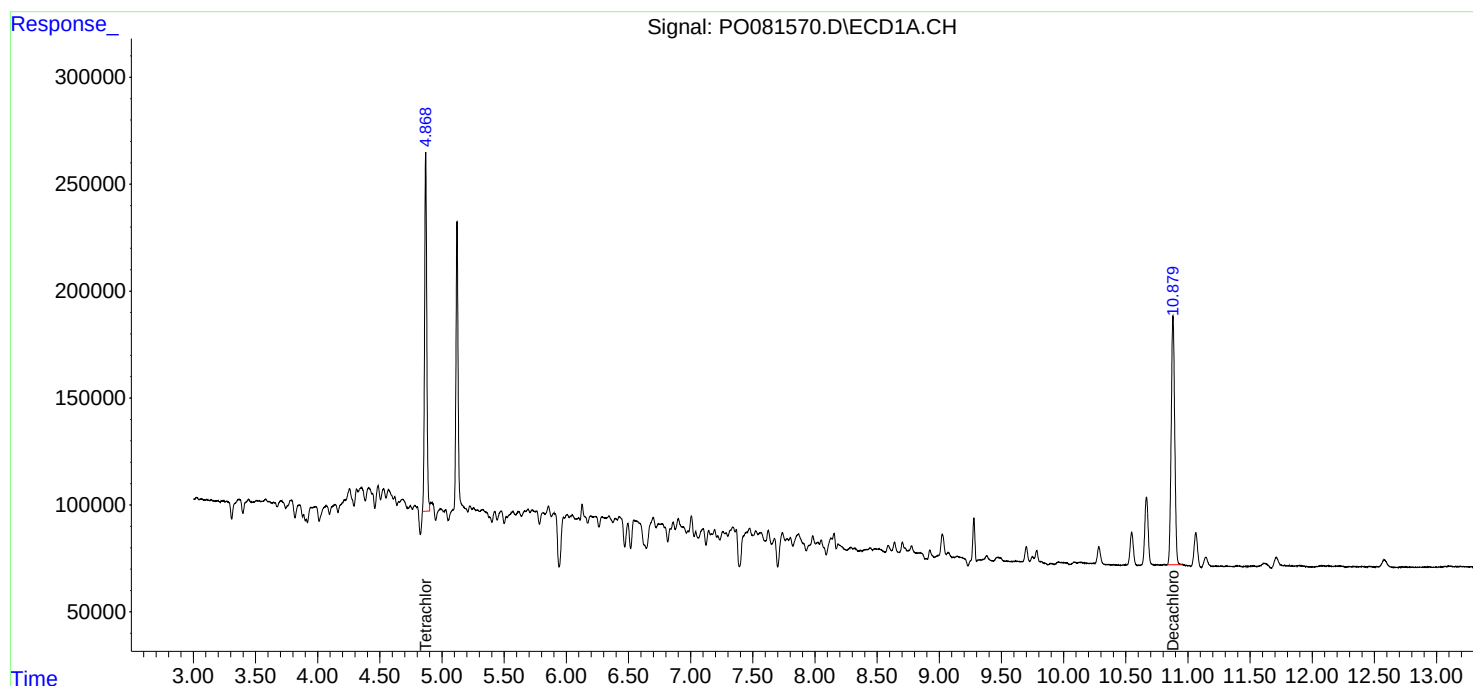

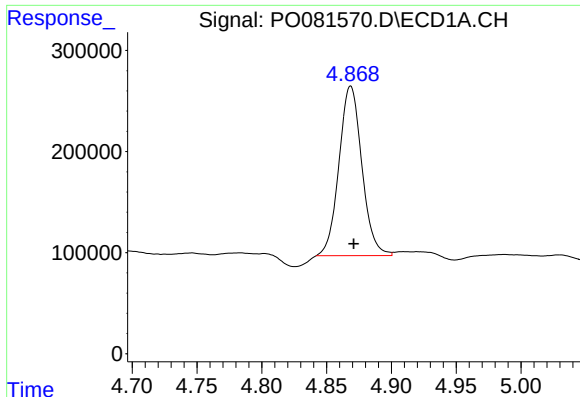


#1 Tetrachloro-m-xylene

R.T.: 4.868 min
Delta R.T.: -0.003 min
Response: 2062635
Conc: 23.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1RE


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:27 AM

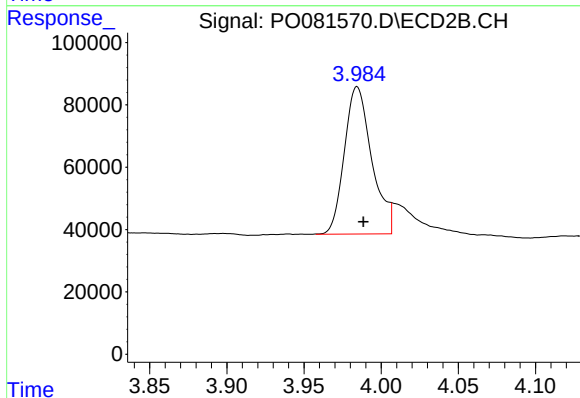


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.004 min
Response: 588199
Conc: 22.08 ng/ml m

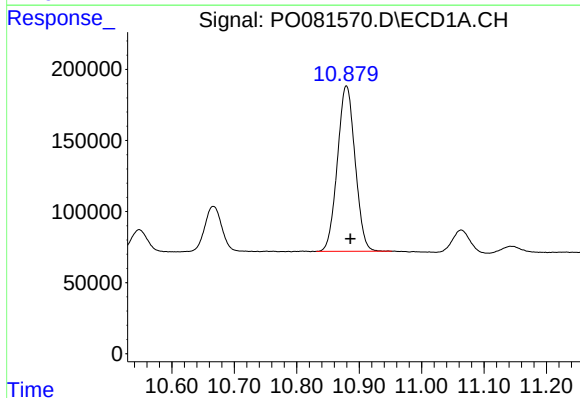

#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: -0.007 min
Response: 2287709
Conc: 30.71 ng/ml

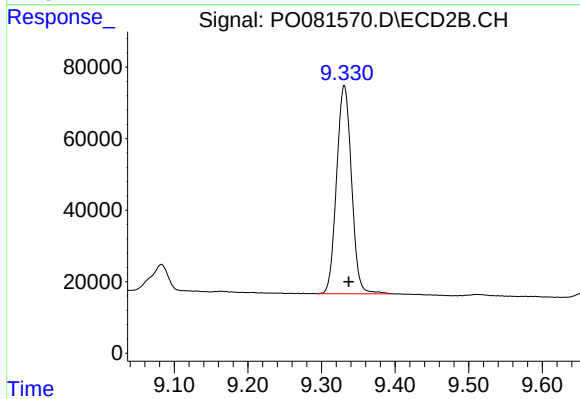

#2 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: -0.006 min
Response: 821069
Conc: 35.36 ng/ml