

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092721\
 Data File : P0081574.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2021 13:48
 Operator : AJ\MA
 Sample : M3935-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-S

Manual Integrations
 APPROVED

mohammad
 9/28/2021 9:31:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 03:11:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	3.985	2266040	668418	25.411	25.089
2)	SA Decachlor...	10.880	9.332	1619862	506724	21.747	21.820
Target Compounds							
26)	L6 AR-1254-1	7.116	6.135	605189	164484	168.789	107.418 #
27)	L6 AR-1254-2	7.342	6.292	621591	103438	112.732	76.027 #
28)	L6 AR-1254-3	7.722	6.718	472840	130875	83.799	65.794
29)	L6 AR-1254-4	8.019	6.959	325307	98292	79.110m	78.720
30)	L6 AR-1254-5	8.448	7.391	450850	159728	97.811m	85.443

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092721\
Data File : PO081574.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2021 13:48
Operator : AJ\MA
Sample : M3935-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1-S


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 03:11:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

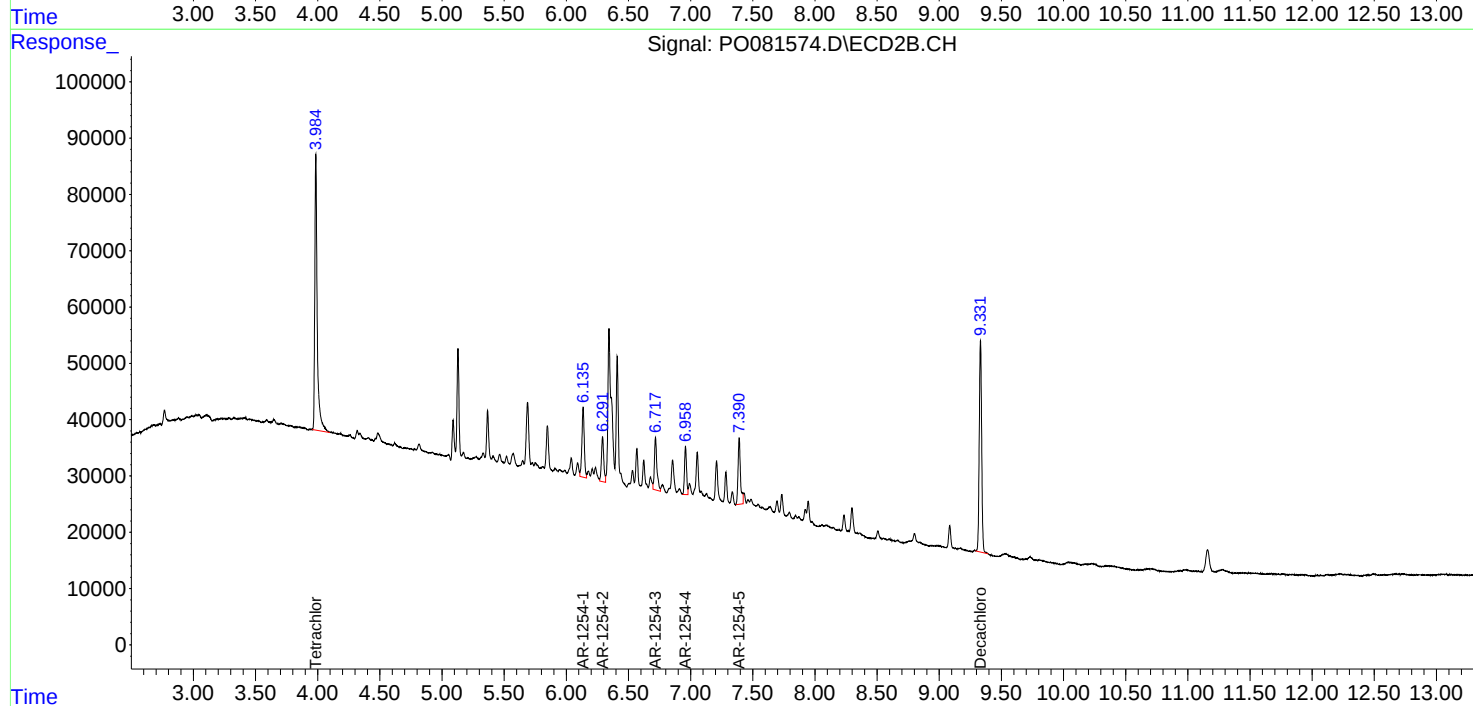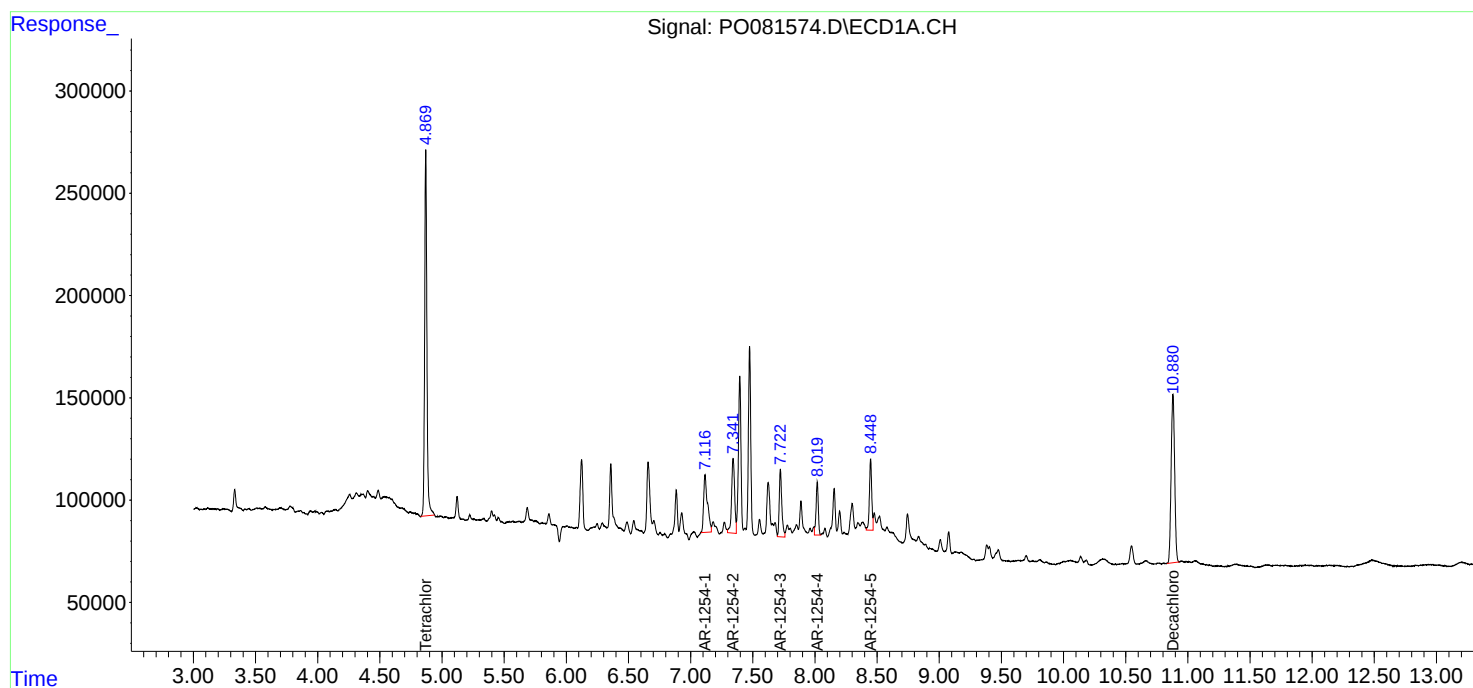

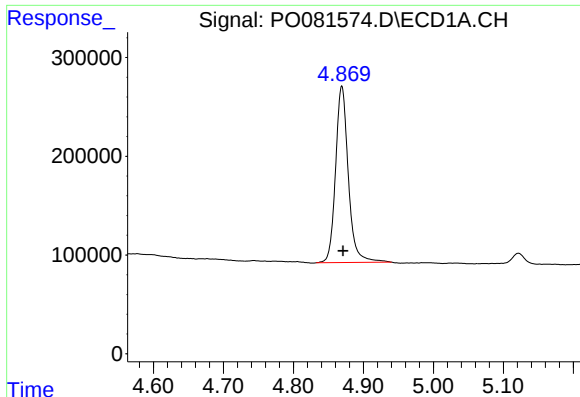


#1 Tetrachloro-m-xylene

R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 2266040
Conc: 25.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:40 AM

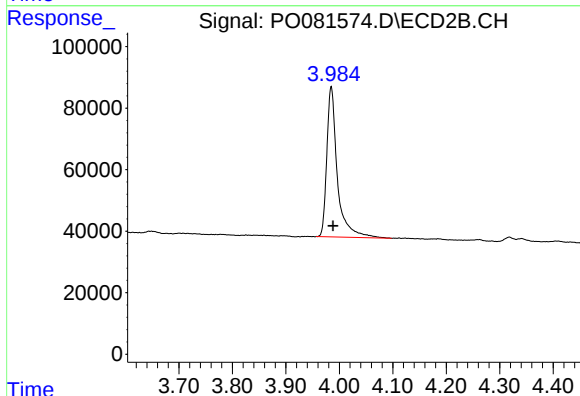


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: -0.004 min
Response: 668418
Conc: 25.09 ng/ml

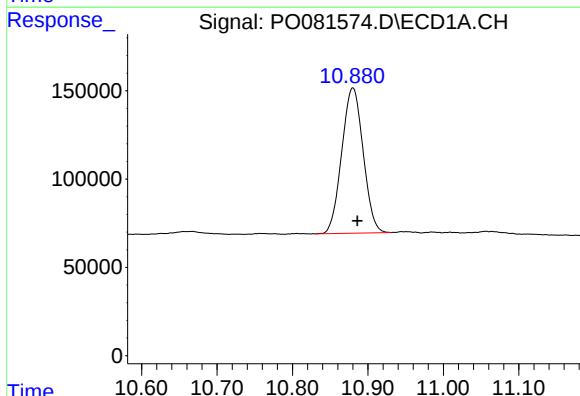


#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 1619862
Conc: 21.75 ng/ml

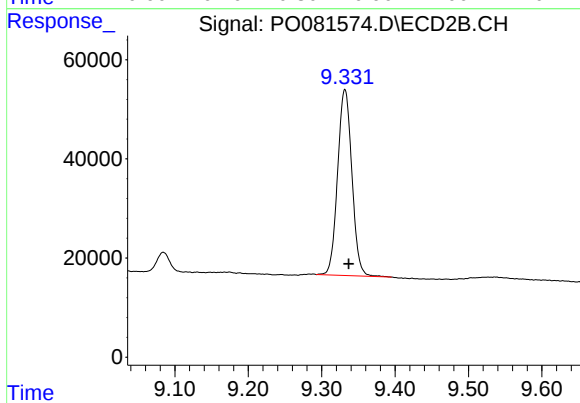

#2 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: -0.005 min
Response: 506724
Conc: 21.82 ng/ml

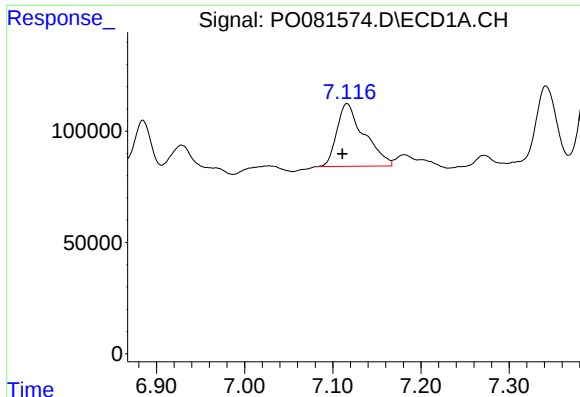


#26 AR-1254-1

R.T.: 7.116 min
Delta R.T.: 0.005 min
Response: 605189
Conc: 168.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:40 AM

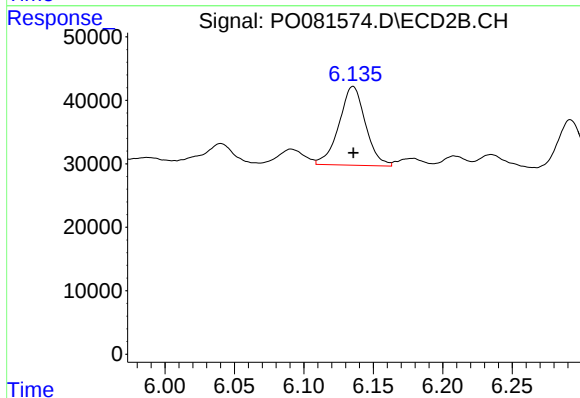


#26 AR-1254-1

R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 164484
Conc: 107.42 ng/ml

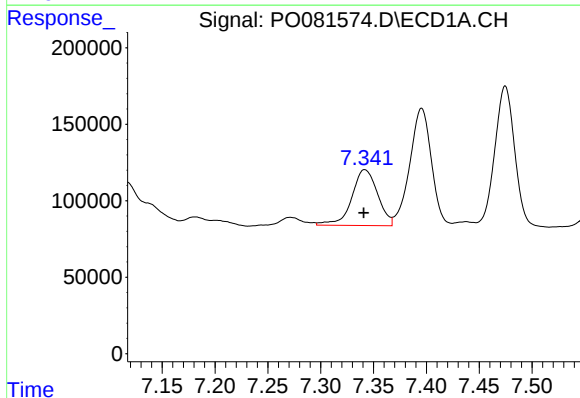


#27 AR-1254-2

R.T.: 7.342 min
Delta R.T.: 0.000 min
Response: 621591
Conc: 112.73 ng/ml

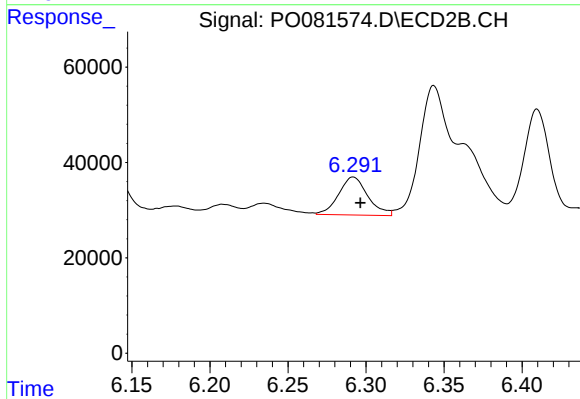

#27 AR-1254-2

R.T.: 6.292 min
Delta R.T.: -0.004 min
Response: 103438
Conc: 76.03 ng/ml

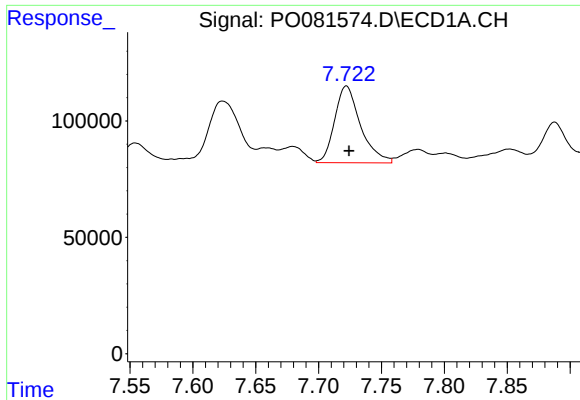


#28 AR-1254-3

R.T.: 7.722 min
Delta R.T.: -0.002 min
Response: 472840
Conc: 83.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S


Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:40 AM

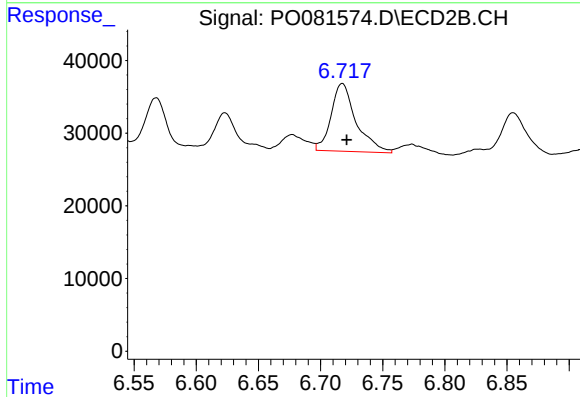


#28 AR-1254-3

R.T.: 6.718 min
Delta R.T.: -0.004 min
Response: 130875
Conc: 65.79 ng/ml

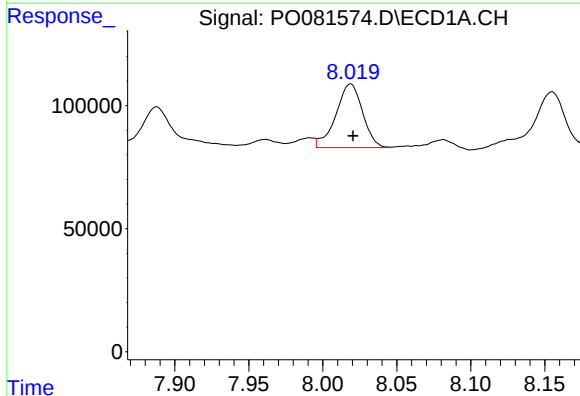


#29 AR-1254-4

R.T.: 8.019 min
Delta R.T.: -0.002 min
Response: 325307
Conc: 79.11 ng/ml m

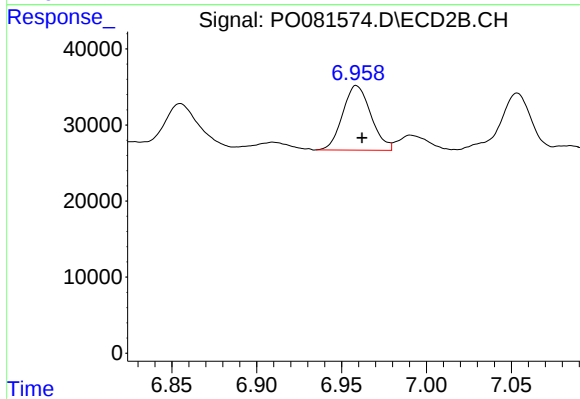

#29 AR-1254-4

R.T.: 6.959 min
Delta R.T.: -0.003 min
Response: 98292
Conc: 78.72 ng/ml

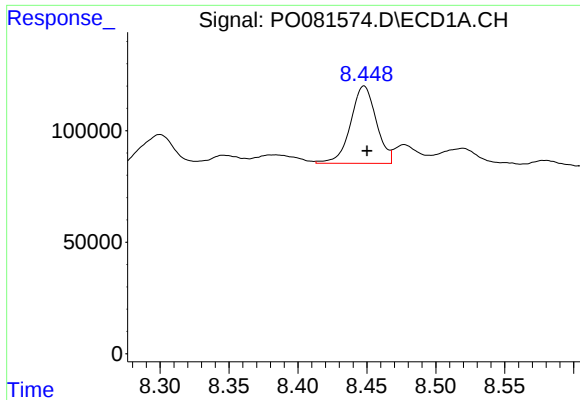


#30 AR-1254-5

R.T.: 8.448 min
Delta R.T.: -0.002 min
Response: 450850
Conc: 97.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1-S

Manual Integrations
APPROVED

mohammad
9/28/2021 9:31:40 AM

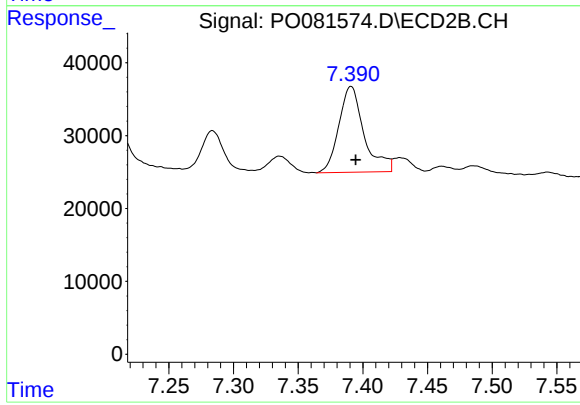

#30 AR-1254-5

R.T.: 7.391 min
Delta R.T.: -0.004 min
Response: 159728
Conc: 85.44 ng/ml