

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092818\
 Data File : P0049448.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2018 3:45
 Operator : SM/SJ
 Sample : J5133-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 092618-SIDI-F-D-S

Manual Integrations
 APPROVED

Sohil
 10/1/2018 4:04:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:26:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 29 00:05:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.520	3992852	3252744	19.028	19.015m
2) SA Decachlor...	10.098	8.451	4557552	2924628	12.692m	12.127

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092818\
Data File : PO049448.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2018 3:45
Operator : SM/SJ
Sample : J5133-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
092618-SIDI-F-D-S


Manual Integrations
APPROVED

Sohil
10/1/2018 4:04:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:26:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092818.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 29 00:05:46 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

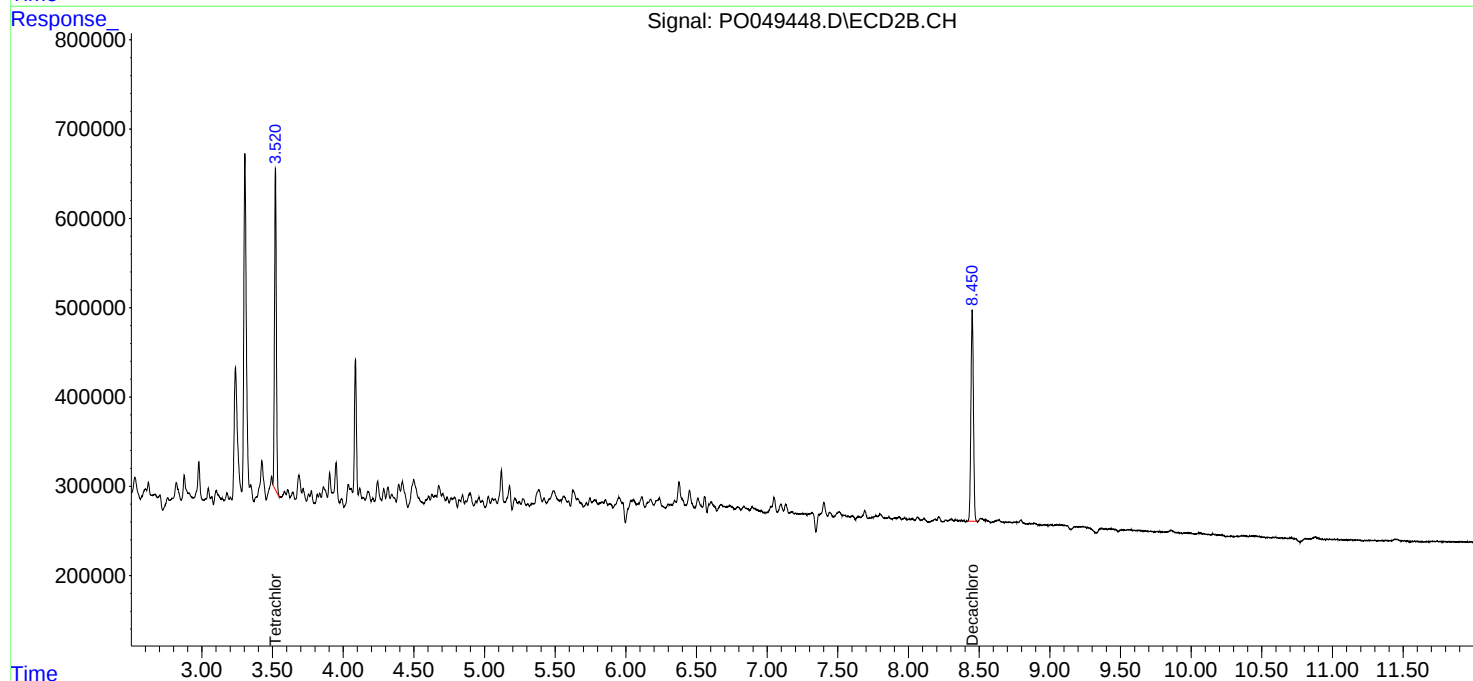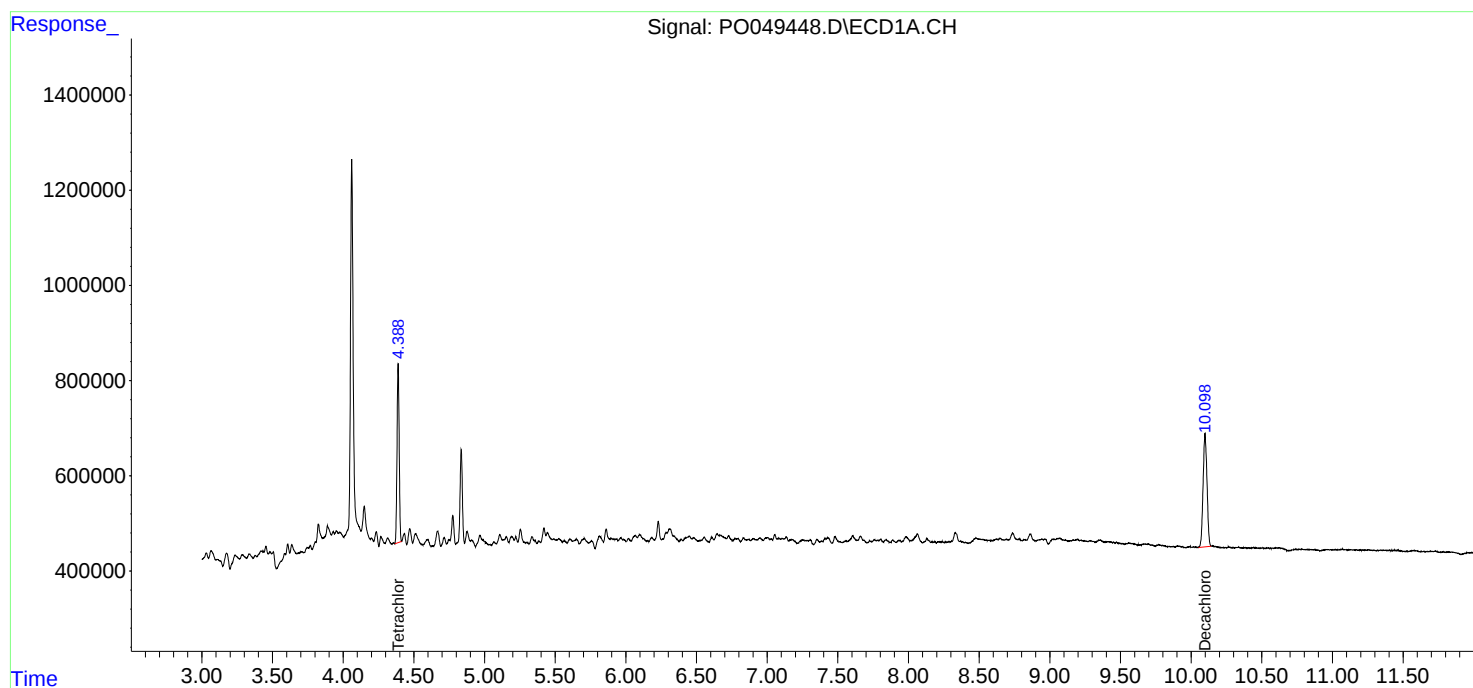

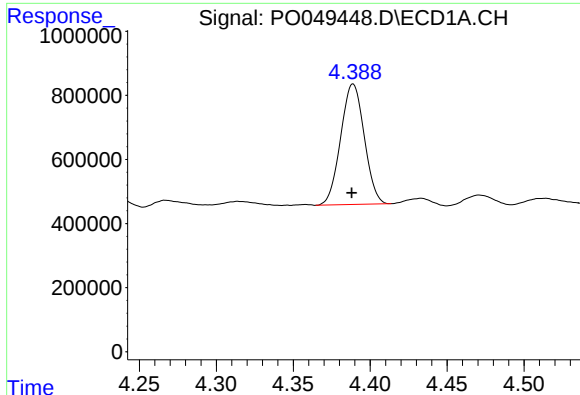


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 3992852
Conc: 19.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
092618-SIDI-F-D-S


Manual Integrations
APPROVED

Sohil
10/1/2018 4:04:02 PM

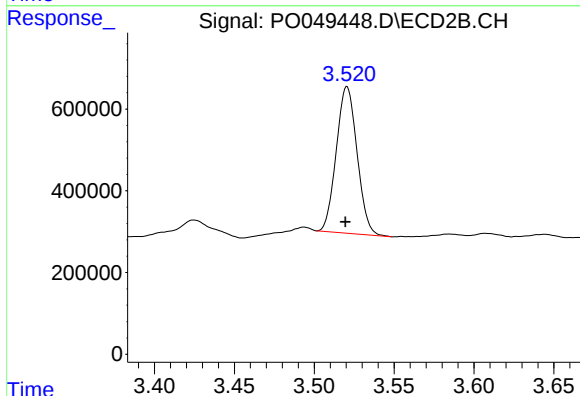


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: 0.000 min
Response: 3252744
Conc: 19.02 ng/ml m

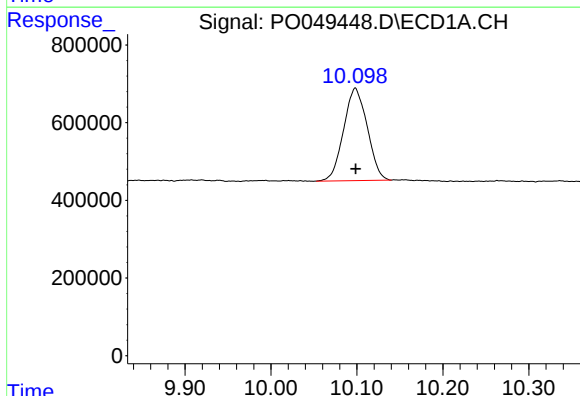

#2 Decachlorobiphenyl

R.T.: 10.098 min
Delta R.T.: 0.000 min
Response: 4557552
Conc: 12.69 ng/ml m

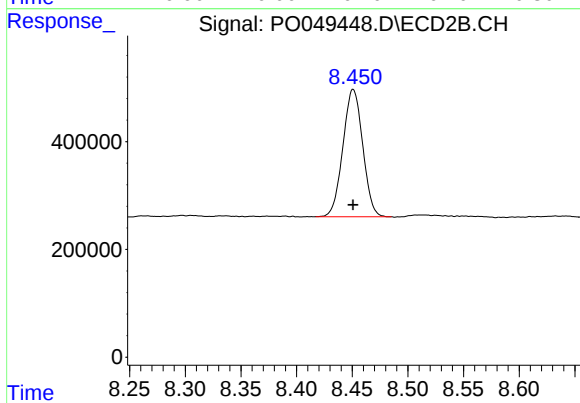

#2 Decachlorobiphenyl

R.T.: 8.451 min
Delta R.T.: 0.000 min
Response: 2924628
Conc: 12.13 ng/ml