

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092818\
 Data File : P0049476.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2018 11:27
 Operator : SM/SJ
 Sample : J4775-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-091418-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:48:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 29 00:05:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.520	5648355	5173039	26.918	30.241
2) SA Decachlor...	10.097	8.450	6071448	3544084	16.908	14.696

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092818\
Data File : PO049476.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2018 11:27
Operator : SM/SJ
Sample : J4775-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OR-03-091418-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:48:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092818.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 29 00:05:46 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

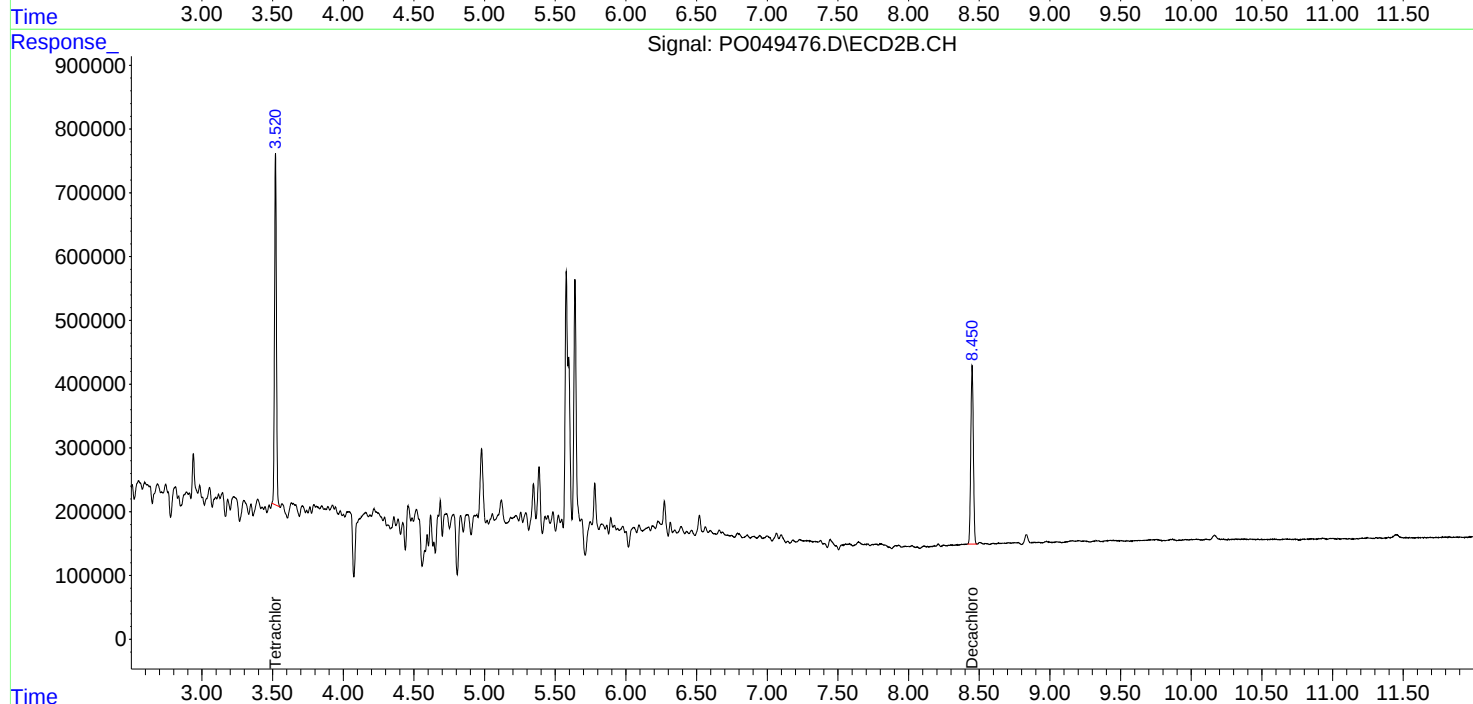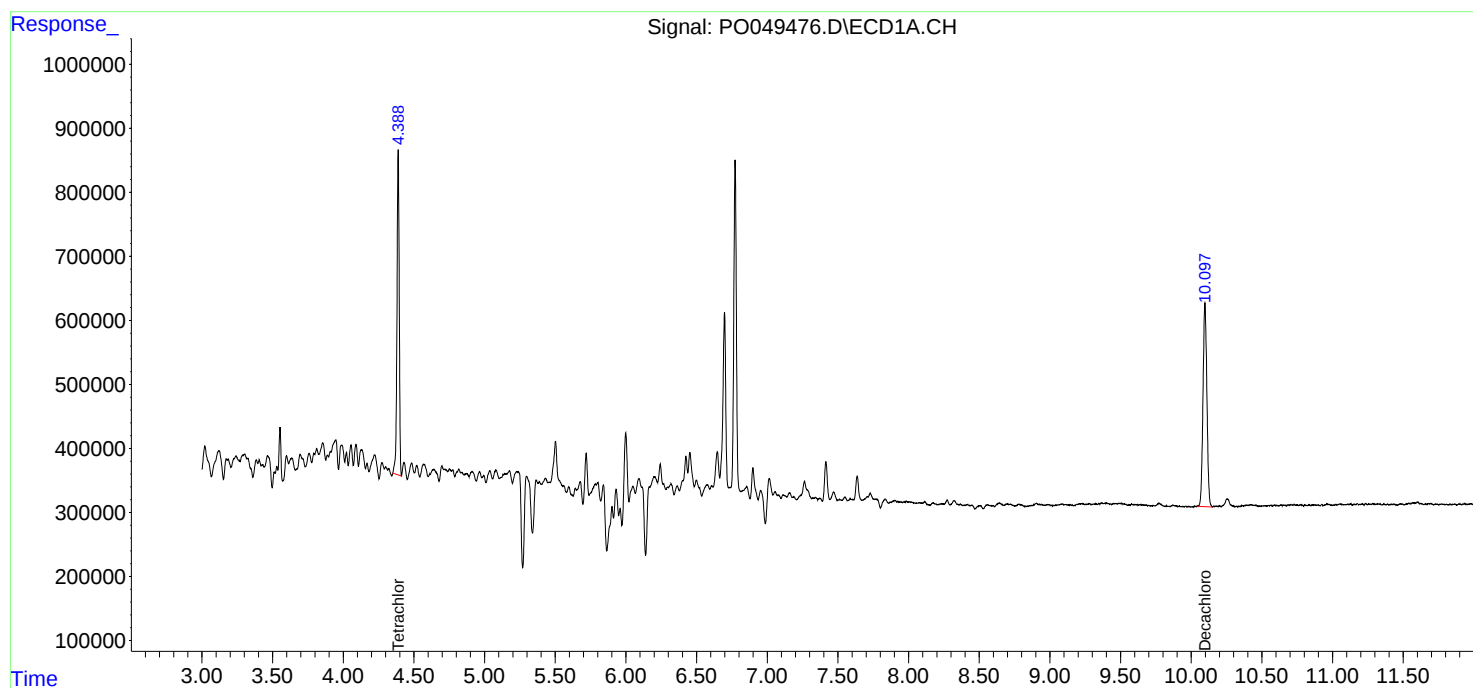


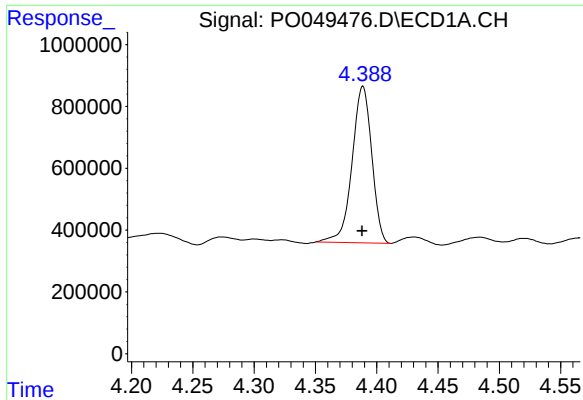

#1 Tetrachloro-m-xylene


R.T.: 4.389 min
Delta R.T.: 0.000 min
Response: 5648355
Conc: 26.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-03-091418-A

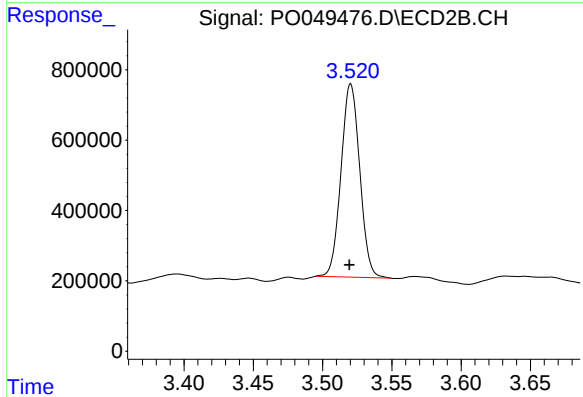


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: 0.001 min
Response: 5173039
Conc: 30.24 ng/ml

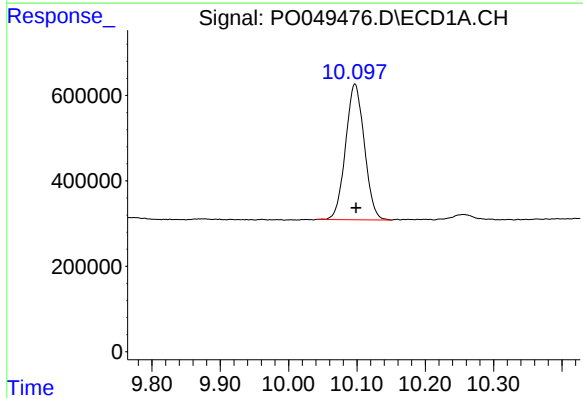

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: -0.002 min
Response: 6071448
Conc: 16.91 ng/ml

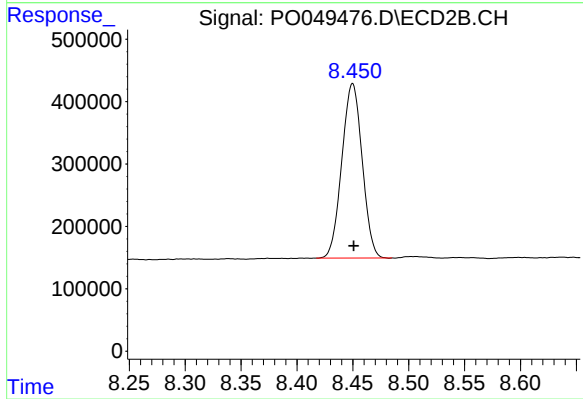

#2 Decachlorobiphenyl

R.T.: 8.450 min
Delta R.T.: 0.000 min
Response: 3544084
Conc: 14.70 ng/ml