

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092820\
 Data File : P0071715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2020 23:15
 Operator : DD\AJ
 Sample : L4160-02
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11976

Manual Integrations
 APPROVED

Ankita
 9/29/2020 11:23:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 02:44:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.524	2308124	1033308	26.897m	25.089
2) SA Decachlor...	9.953	8.700	2667519	1291378	23.218	21.245

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092820\
Data File : P0071715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2020 23:15
Operator : DD\AJ
Sample : L4160-02
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
11976


Manual Integrations
APPROVED

Ankita
9/29/2020 11:23:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 02:44:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

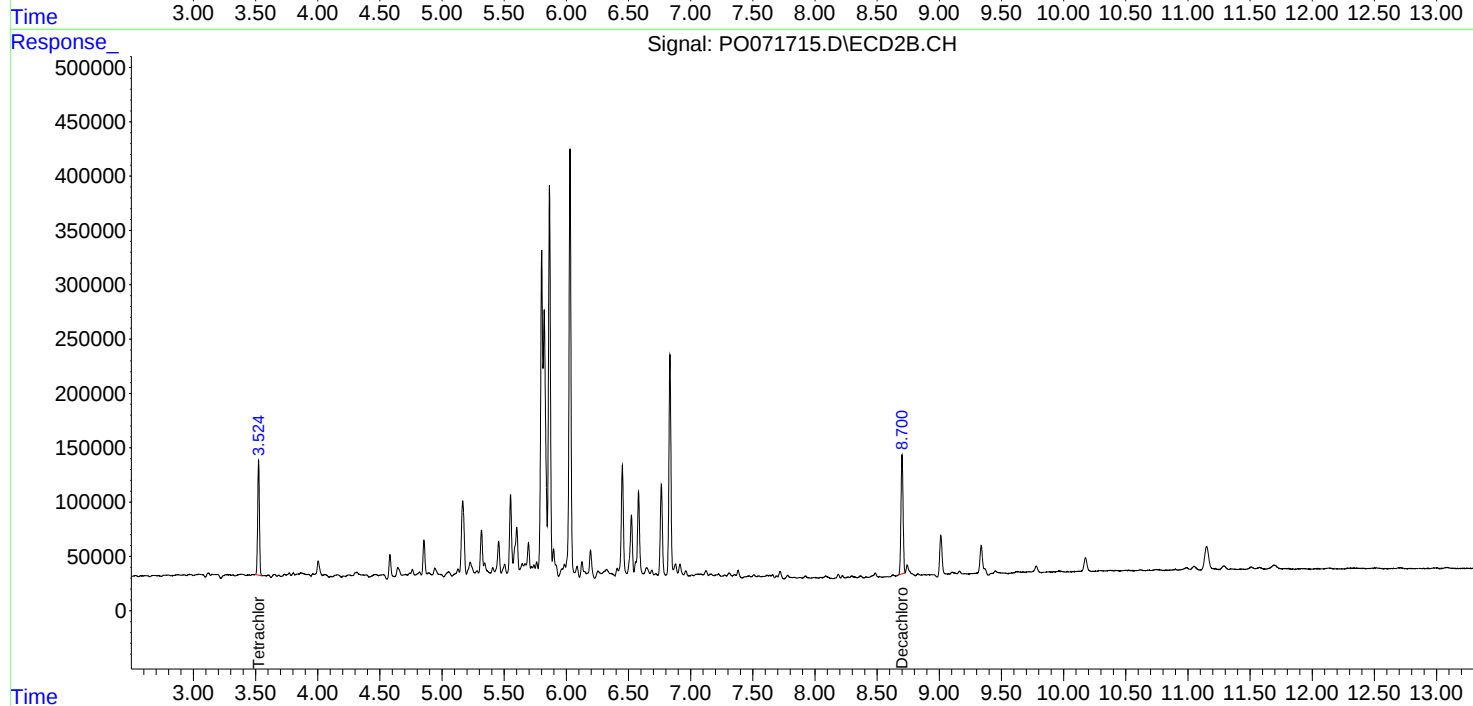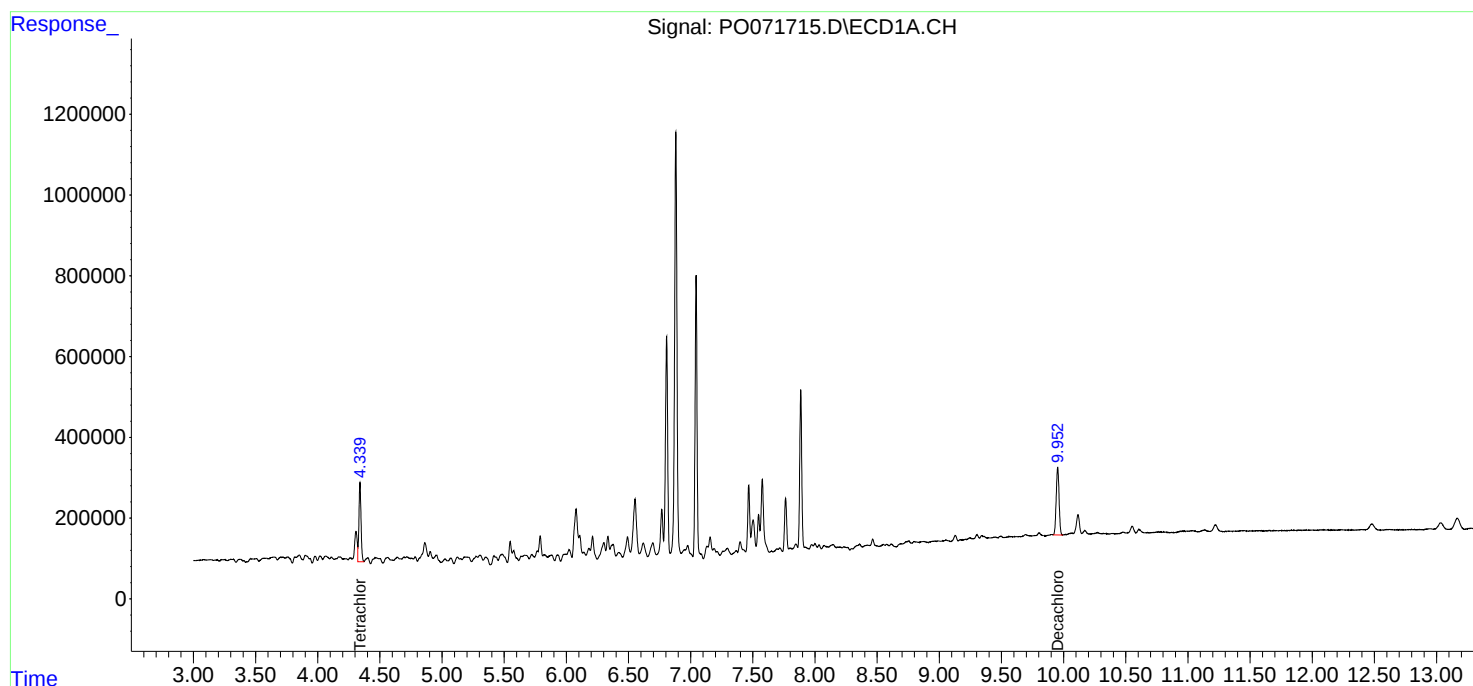

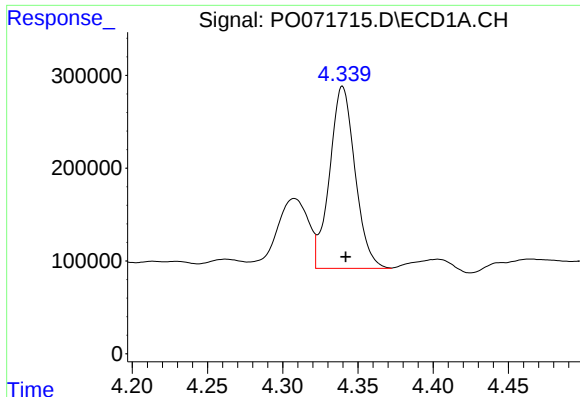


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.003 min
Response: 2308124
Conc: 26.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
11976


Manual Integrations
APPROVED

Ankita
9/29/2020 11:23:48 AM

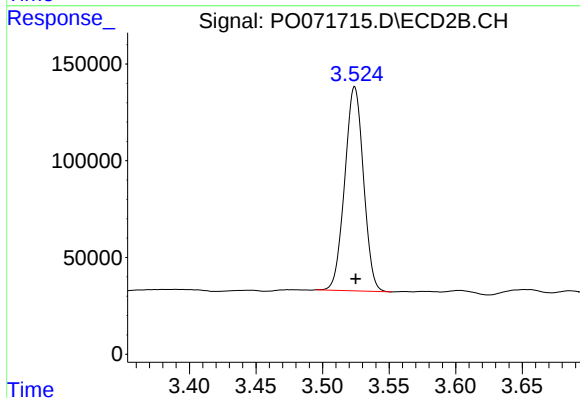


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 1033308
Conc: 25.09 ng/ml

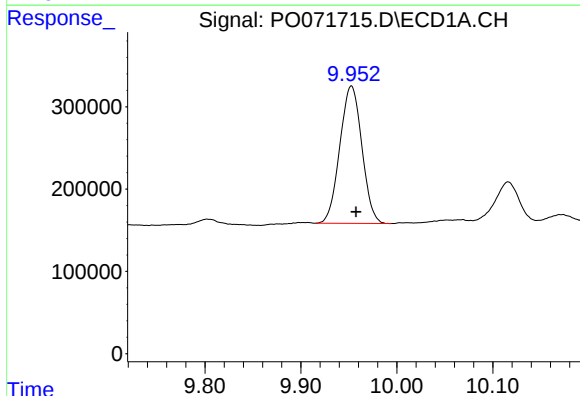

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.005 min
Response: 2667519
Conc: 23.22 ng/ml

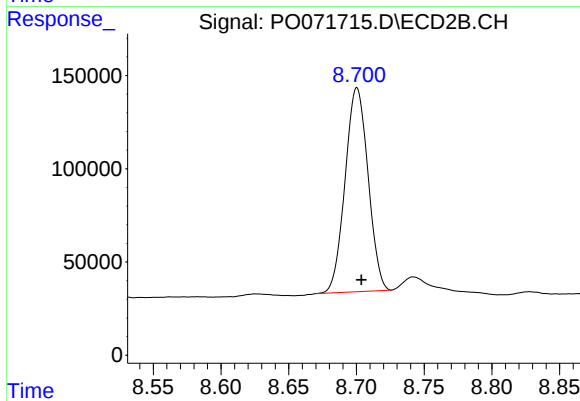

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.003 min
Response: 1291378
Conc: 21.24 ng/ml