

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
 Data File : P0081610.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2021 10:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 15:15:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.870	3.984	2584161	704597	28.978	26.447
2)	SA Decachlor...	10.883	9.332	2109792	656553	28.324	28.272
Target Compounds							
8)	L2 AR-1221-1	5.122	0.000	56840	0	51.942	N.D. #
9)	L2 AR-1221-2	5.224	0.000	34162	0	43.328	N.D. #
24)	L5 AR-1248-4	7.138	0.000	8446	0	2.452	N.D. #
26)	L6 AR-1254-1	7.117	0.000	42684	0	11.905	N.D. #
28)	L6 AR-1254-3	7.741f	0.000	46746	0	8.284	N.D. #
32)	L7 AR-1260-2	8.133f	0.000	18854	0	3.633	N.D. #
33)	L7 AR-1260-3	0.000	7.206	0	20301	N.D.	12.208 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
Data File : P0081610.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2021 10:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 15:15:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

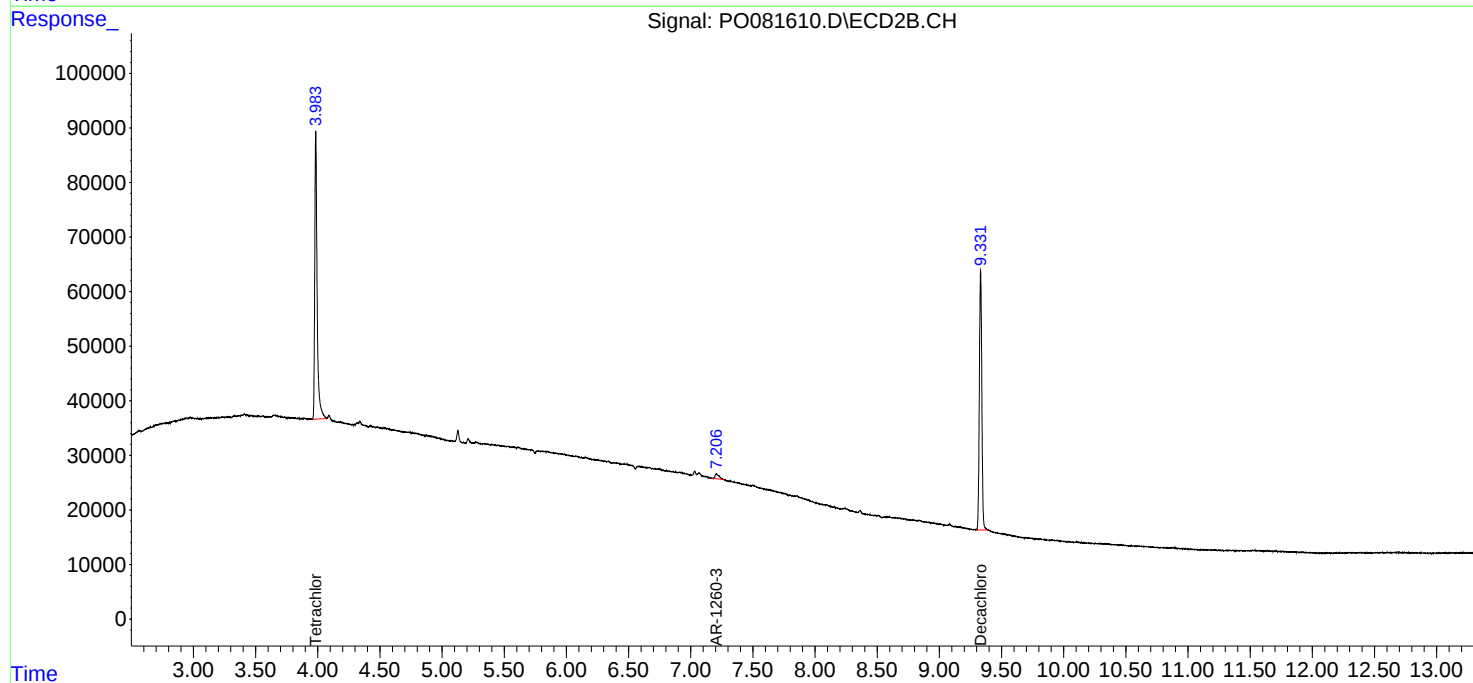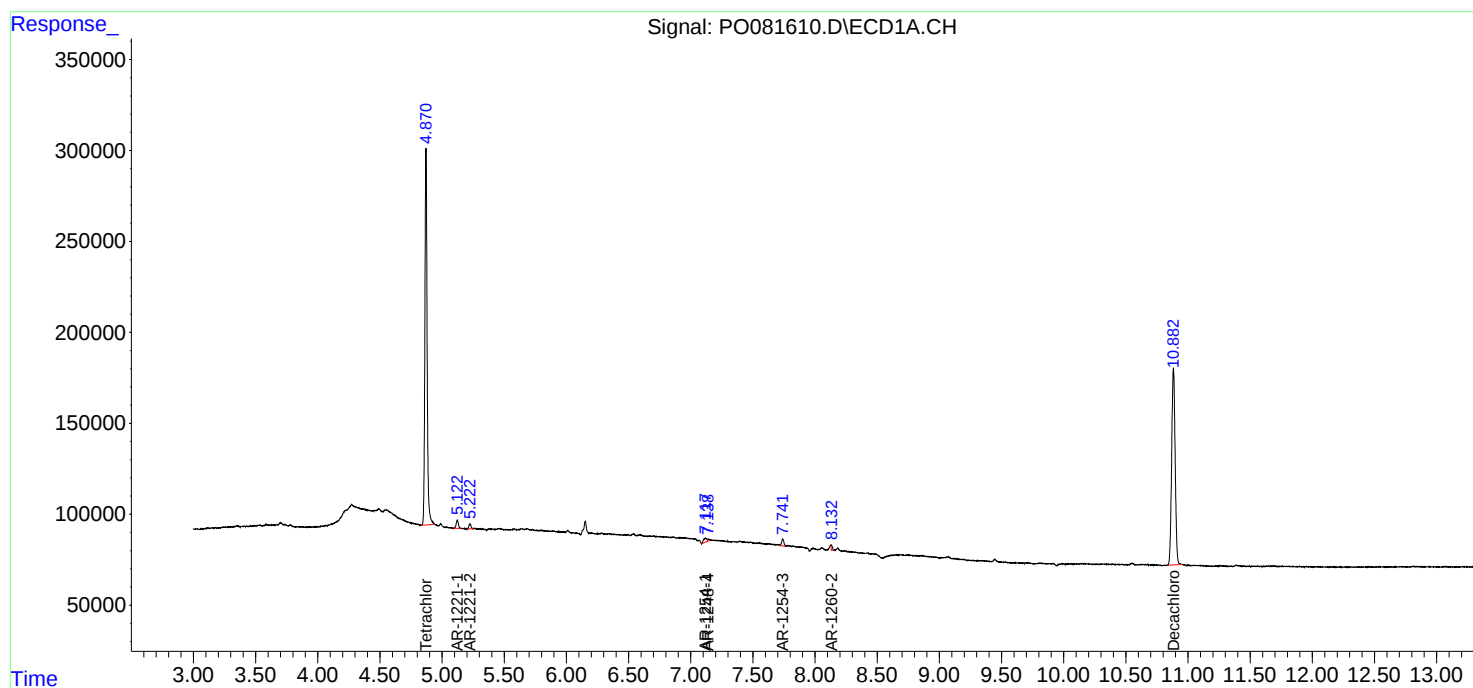


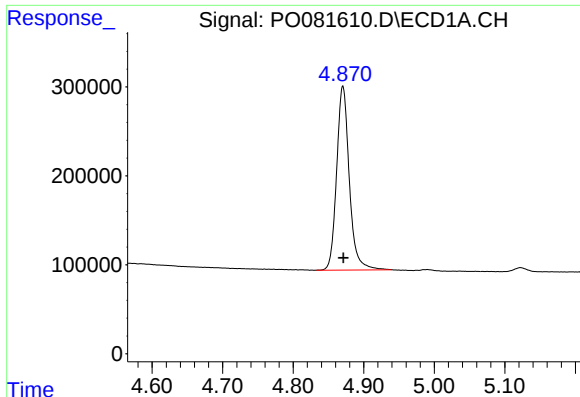

#1 Tetrachloro-m-xylene


R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 2584161
Conc: 28.98 ng/ml

Instrument :
ECD_O
ClientSampleId :

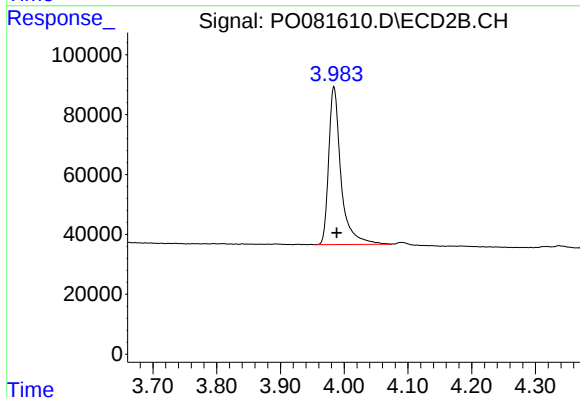


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.004 min
Response: 704597
Conc: 26.45 ng/ml

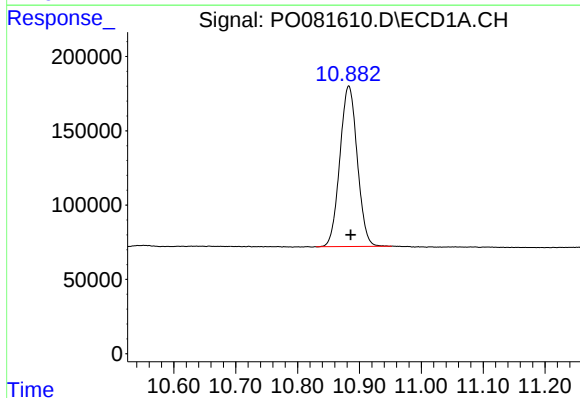


#2 Decachlorobiphenyl

R.T.: 10.883 min
Delta R.T.: -0.003 min
Response: 2109792
Conc: 28.32 ng/ml

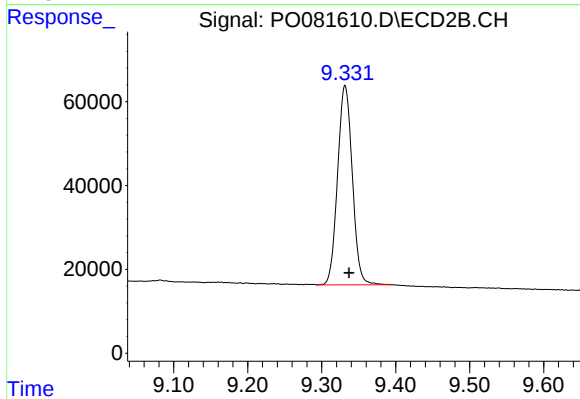

#2 Decachlorobiphenyl


R.T.: 9.332 min
Delta R.T.: -0.005 min
Response: 656553
Conc: 28.27 ng/ml

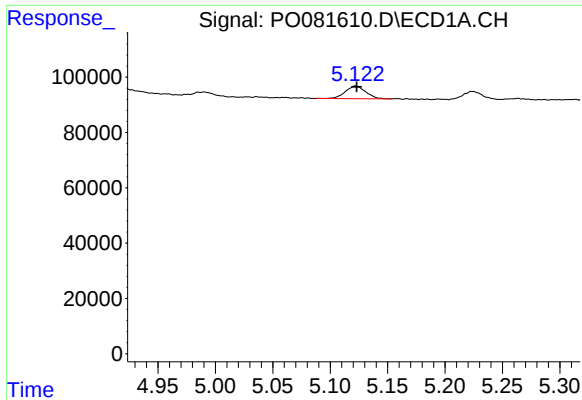

#8 AR-1221-1


R.T.: 5.122 min
Delta R.T.: -0.001 min
Response: 56840
Conc: 51.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

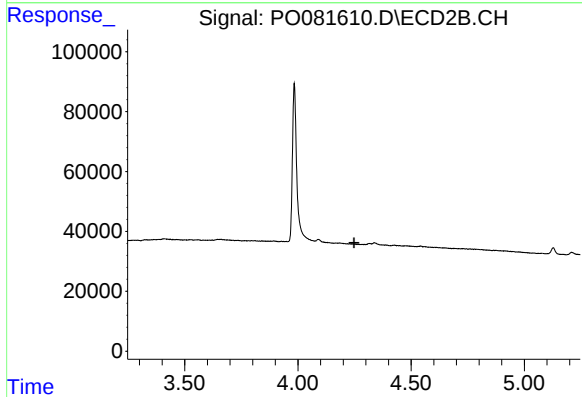


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.248 min
Response: 0
Conc: N.D.

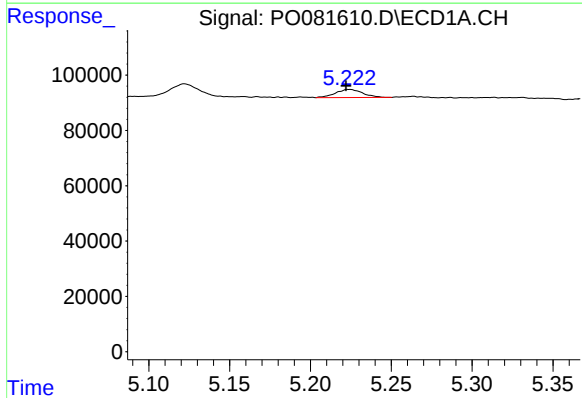


#9 AR-1221-2

R.T.: 5.224 min
Delta R.T.: 0.002 min
Response: 34162
Conc: 43.33 ng/ml

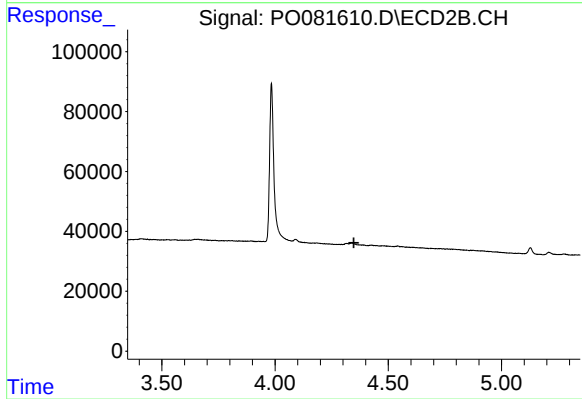

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.348 min
Response: 0
Conc: N.D.

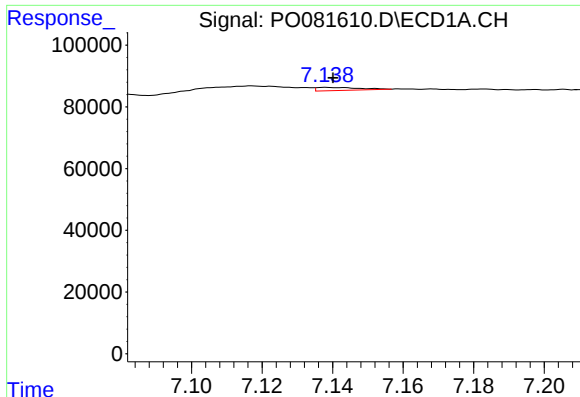

#24 AR-1248-4


R.T.: 7.138 min
Delta R.T.: -0.002 min
Response: 8446
Conc: 2.45 ng/ml

Instrument :
ECD_O
ClientSampleId :

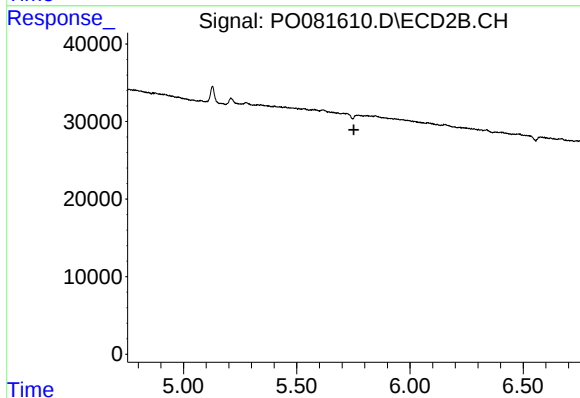


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

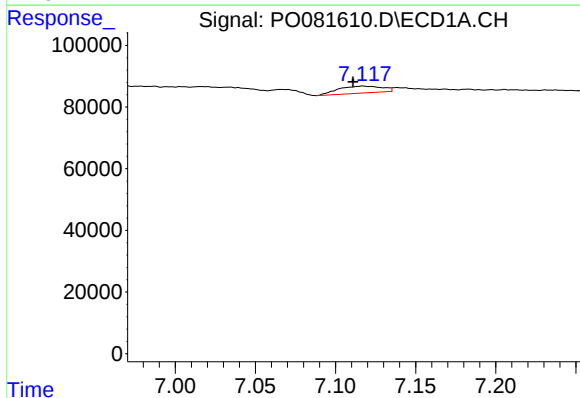


#26 AR-1254-1

R.T.: 7.117 min
Delta R.T.: 0.006 min
Response: 42684
Conc: 11.90 ng/ml

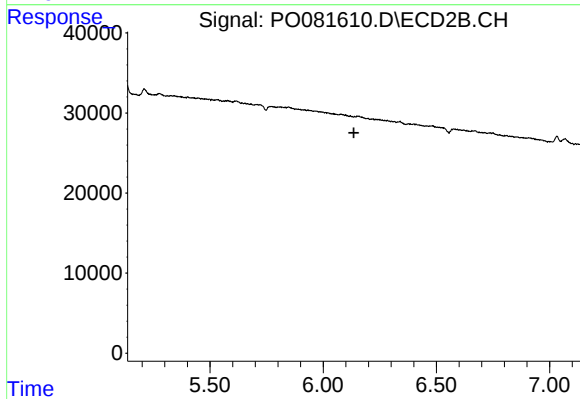

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

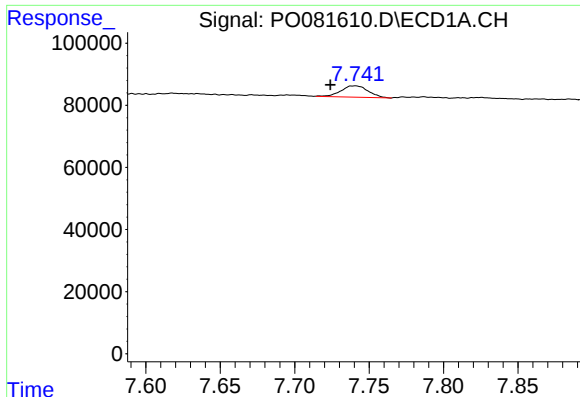

#28 AR-1254-3


R.T.: 7.741 min
Delta R.T.: 0.017 min
Response: 46746
Conc: 8.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

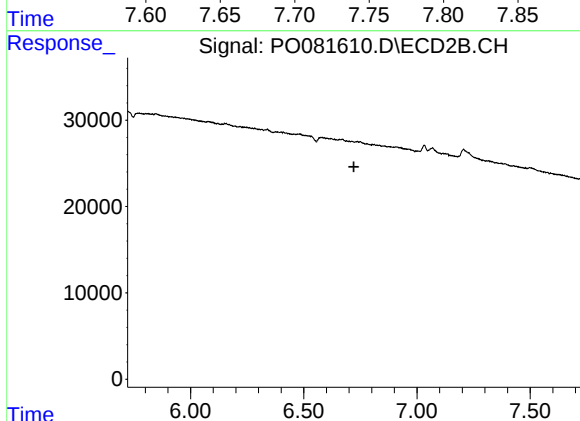


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.721 min
Response: 0
Conc: N.D.

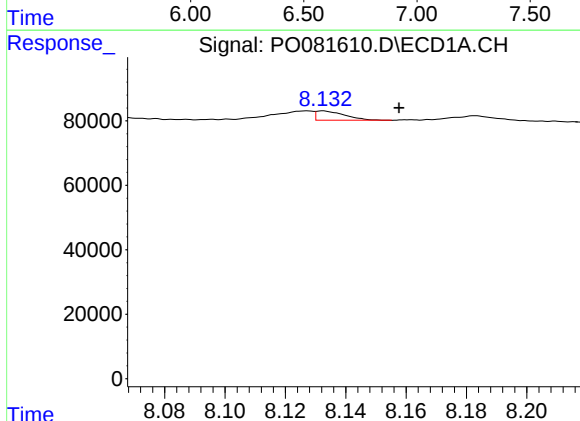


#32 AR-1260-2

R.T.: 8.133 min
Delta R.T.: -0.025 min
Response: 18854
Conc: 3.63 ng/ml

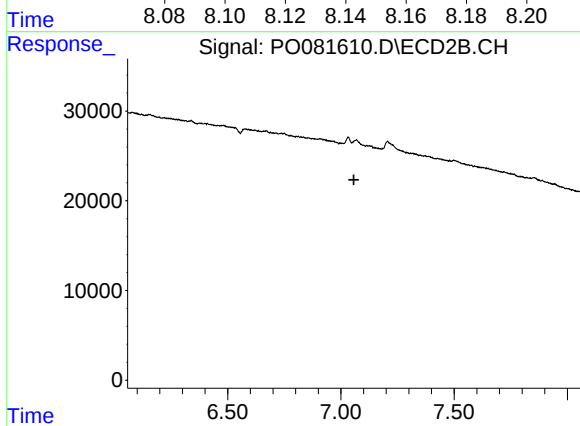

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

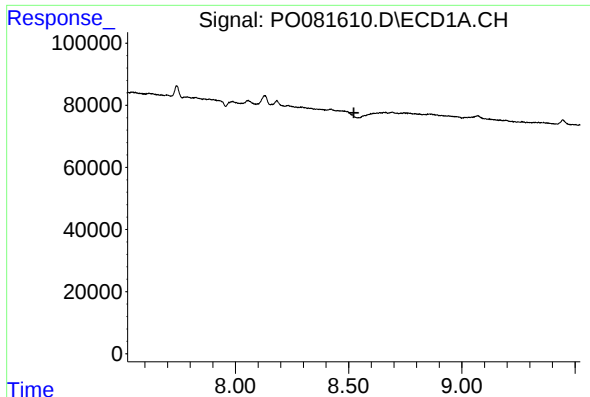

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

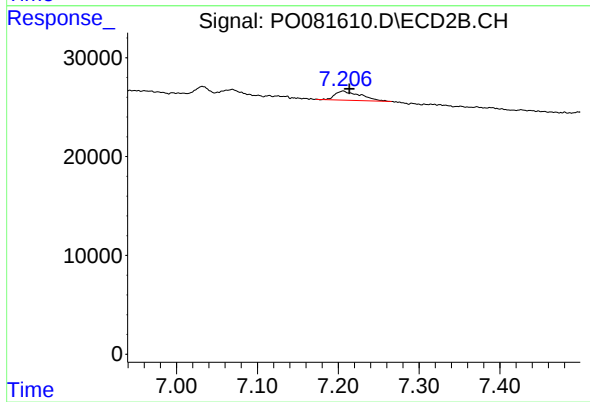

#33 AR-1260-3

R.T.: 7.206 min
Delta R.T.: -0.008 min
Response: 20301
Conc: 12.21 ng/ml