

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
 Data File : P0081616.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2021 12:17
 Operator : AJ\MA
 Sample : M3920-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EB-02-092321

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 15:17:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.869	3.985	2161709	594718	24.241	22.323
2) SA Decachlor...	10.880	9.331	1586267	500261	21.296	21.542

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
Data File : P0081616.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2021 12:17
Operator : AJ\MA
Sample : M3920-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EB-02-092321

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 15:17:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

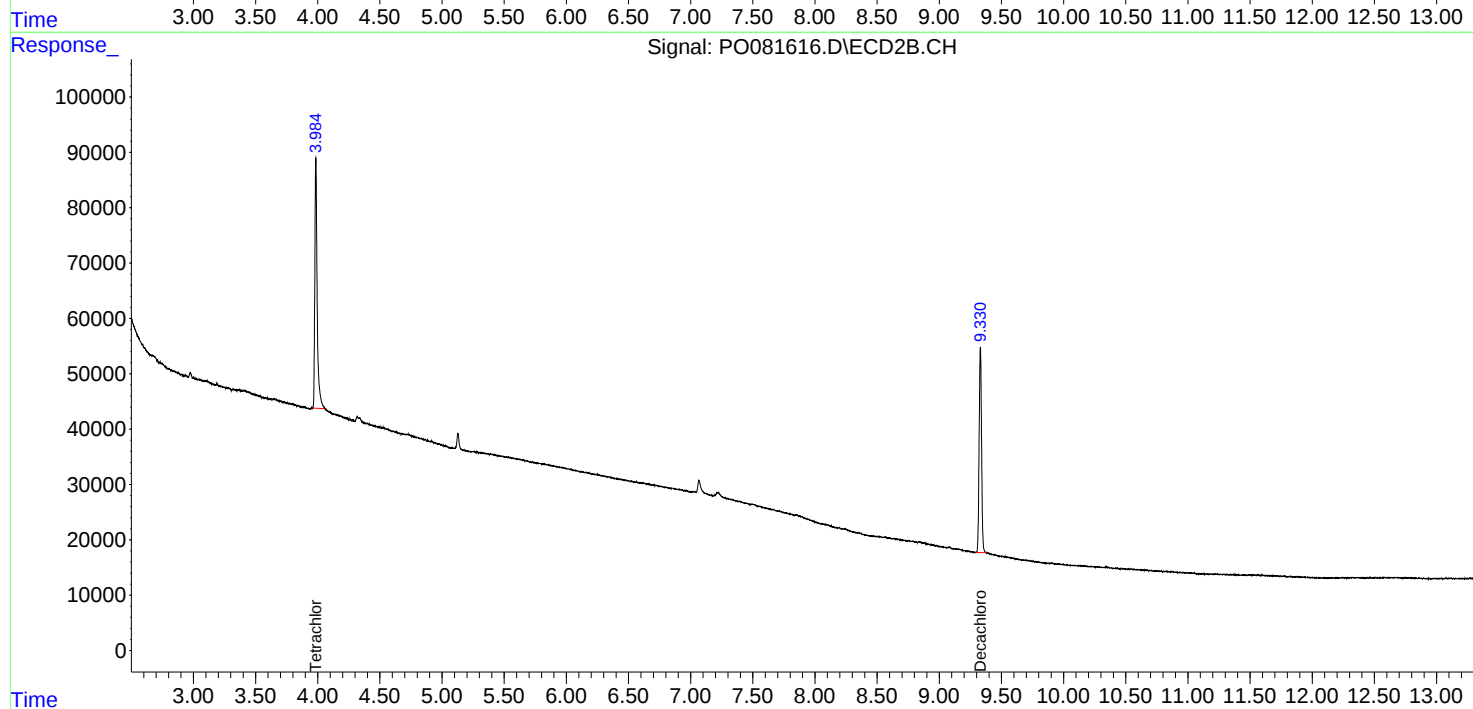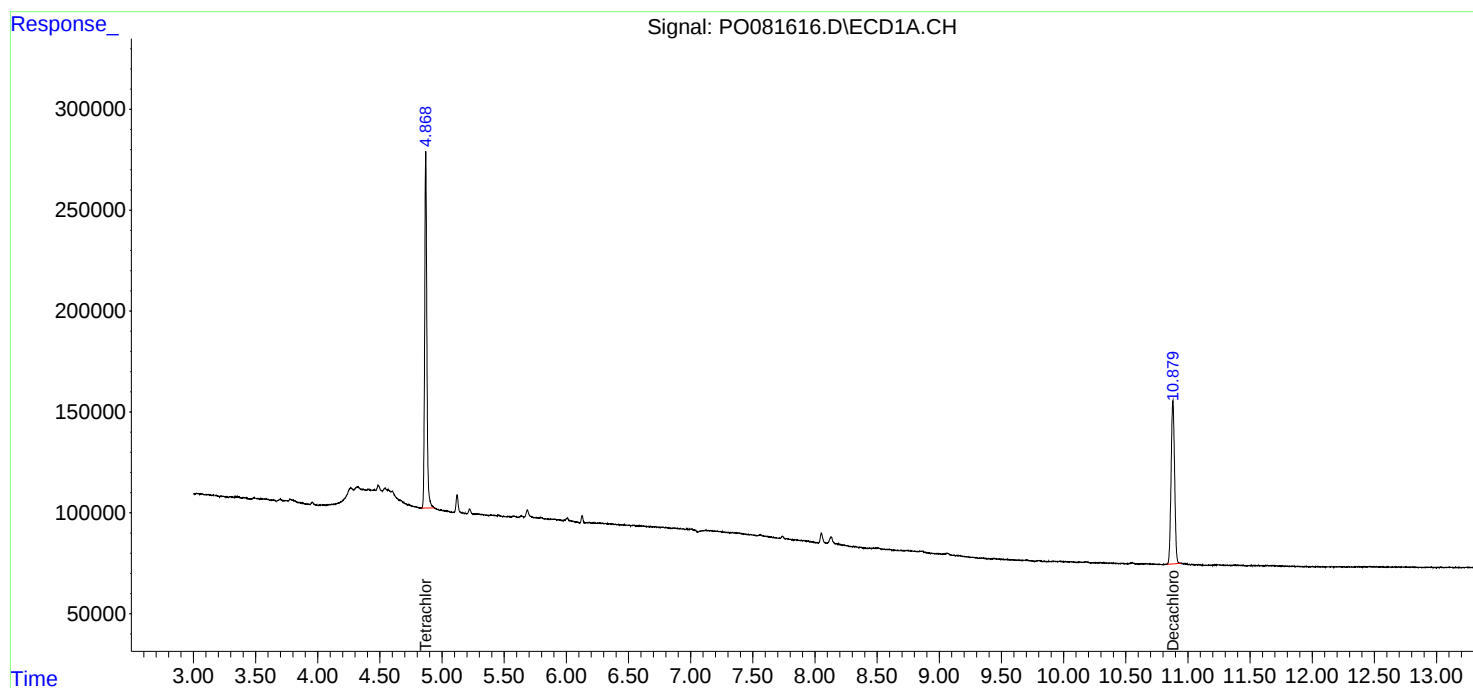


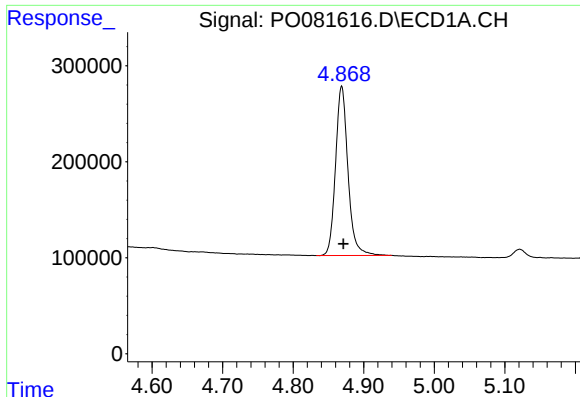

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 2161709
Conc: 24.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
EB-02-092321

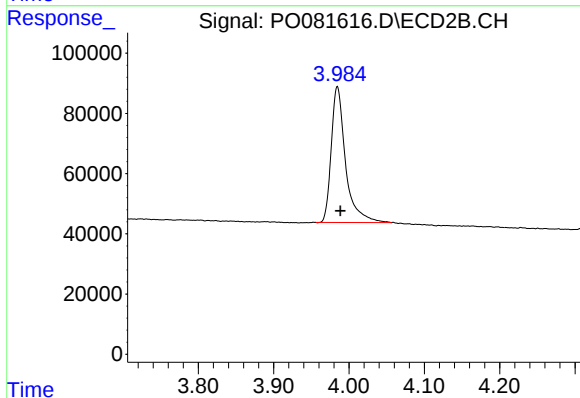


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: -0.004 min
Response: 594718
Conc: 22.32 ng/ml

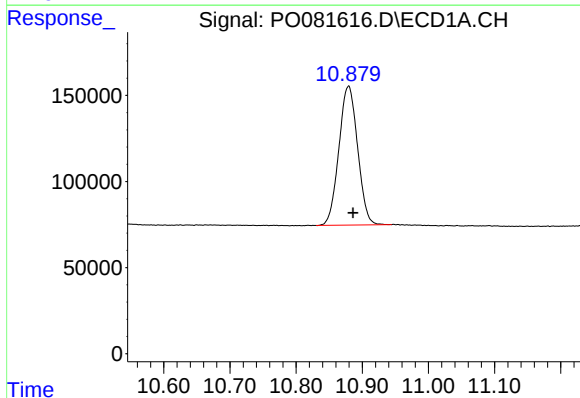

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 1586267
Conc: 21.30 ng/ml

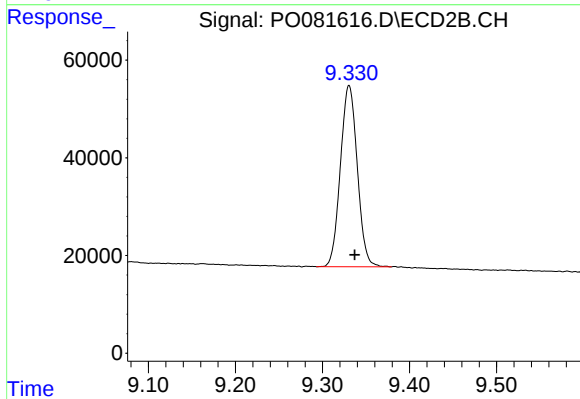

#2 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: -0.006 min
Response: 500261
Conc: 21.54 ng/ml