

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
 Data File : P0081618.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2021 14:04
 Operator : AJ\MA
 Sample : M3962-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 UNDERPASS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 15:17:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	3.983	1542617	454171	17.299	17.047m
2) SA Decachlor...	10.880	9.330	1170397	392504	15.713	16.902

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092821\
Data File : P0081618.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2021 14:04
Operator : AJ\MA
Sample : M3962-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
UNDERPASS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 15:17:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

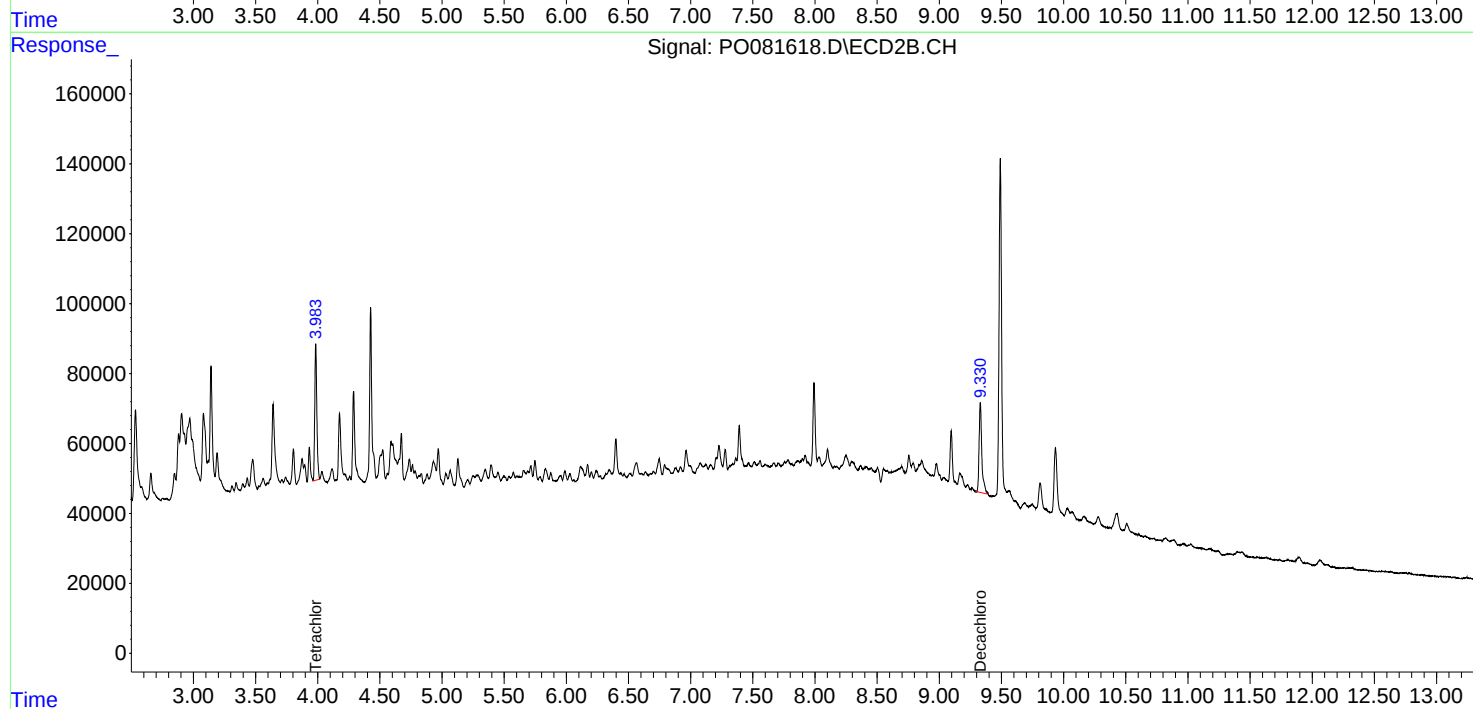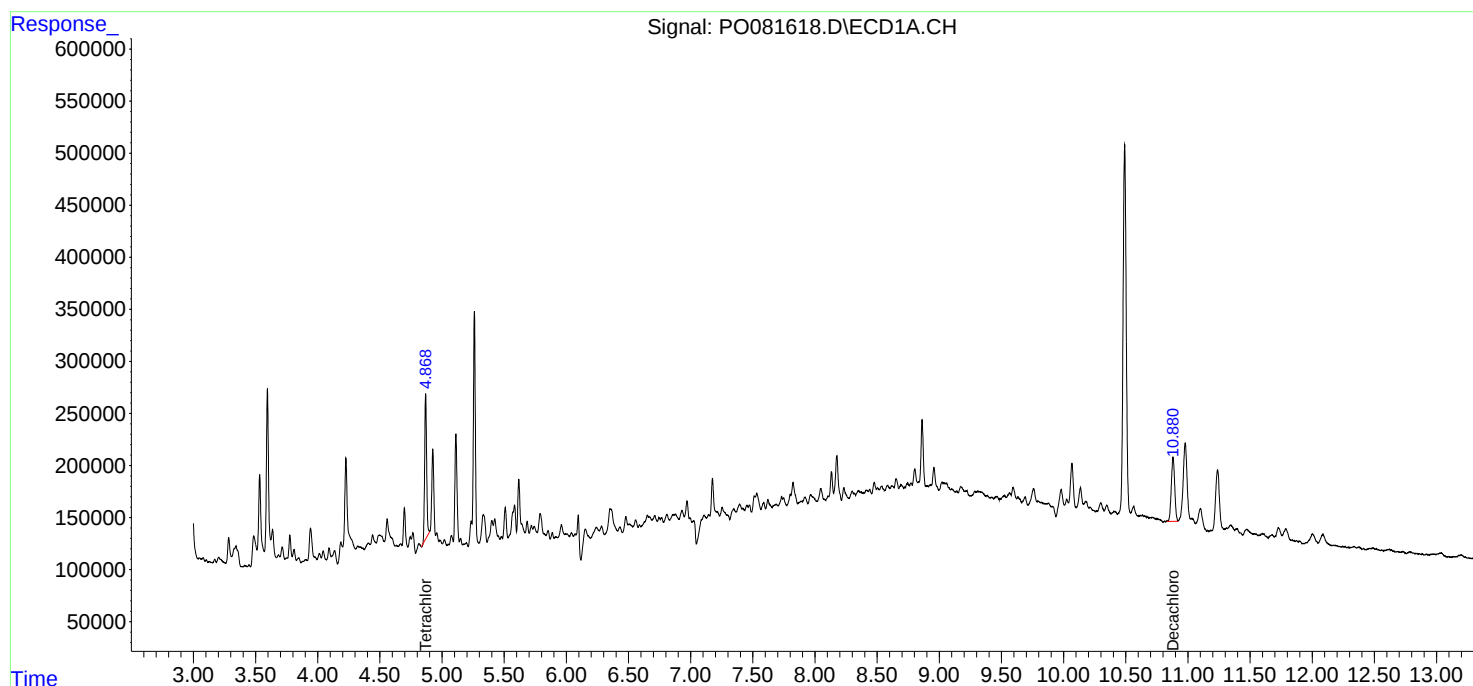


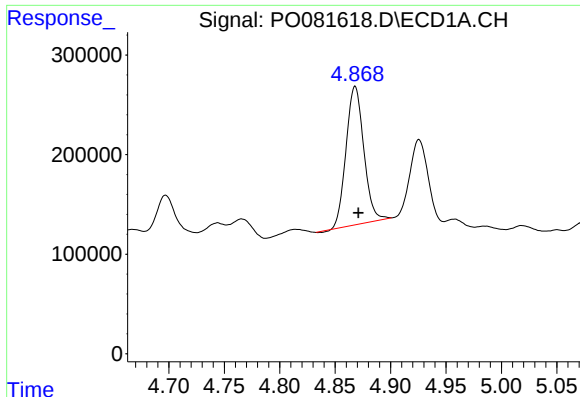

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.003 min
Response: 1542617
Conc: 17.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
UNDERPASS

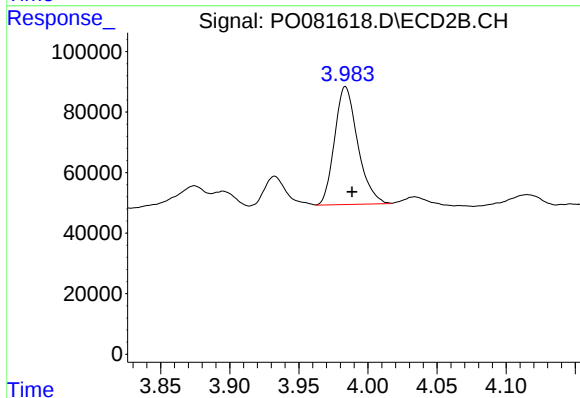


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.005 min
Response: 454171
Conc: 17.05 ng/ml m

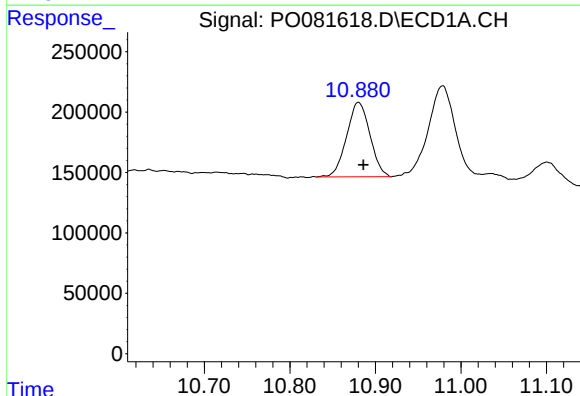

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 1170397
Conc: 15.71 ng/ml

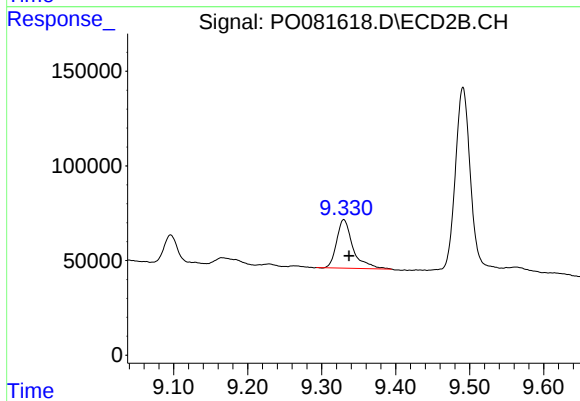

#2 Decachlorobiphenyl

R.T.: 9.330 min
Delta R.T.: -0.007 min
Response: 392504
Conc: 16.90 ng/ml