

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092823\
 Data File : P0098372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 17:48
 Operator : YP/AJ
 Sample : 04628-09RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-092023-103-22RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 00:40:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.638	68335802	17800919	35.588m	22.855m#
2) SA Decachlor...	10.301	8.648	33160111	30558821	27.318	57.038m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO092823\
Data File : PO098372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 17:48
Operator : YP/AJ
Sample : 04628-09RE
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-092023-103-22RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 00:40:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

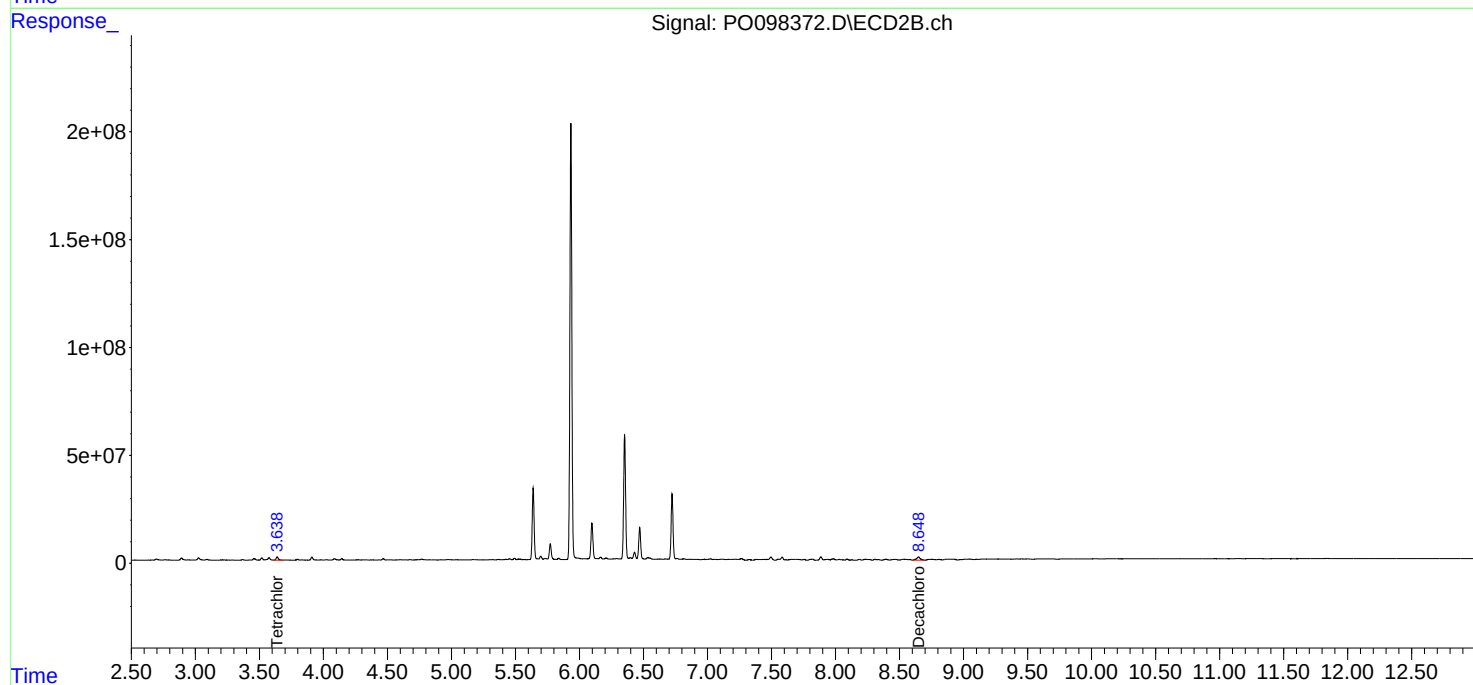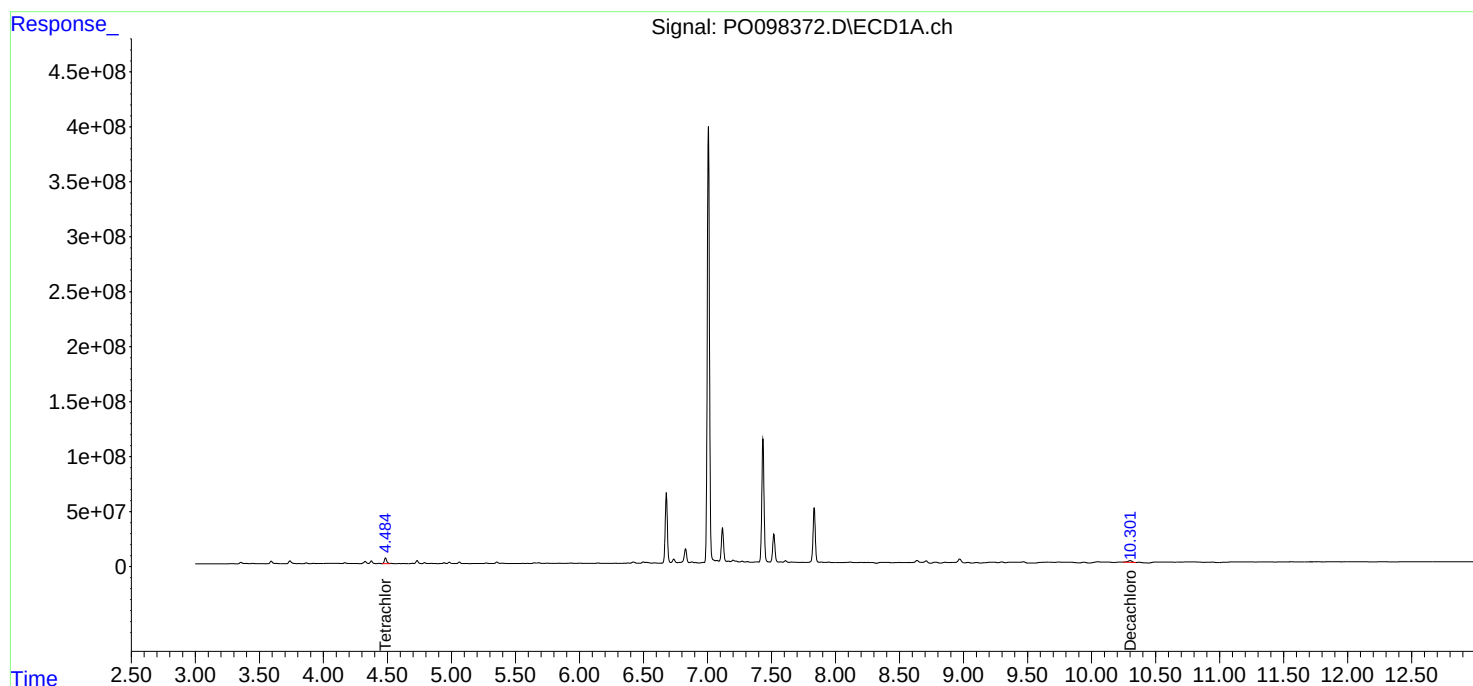

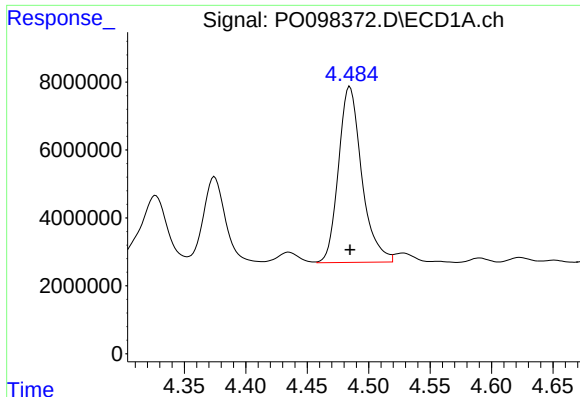


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.000 min
Response: 68335802
Conc: 35.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-092023-103-22RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

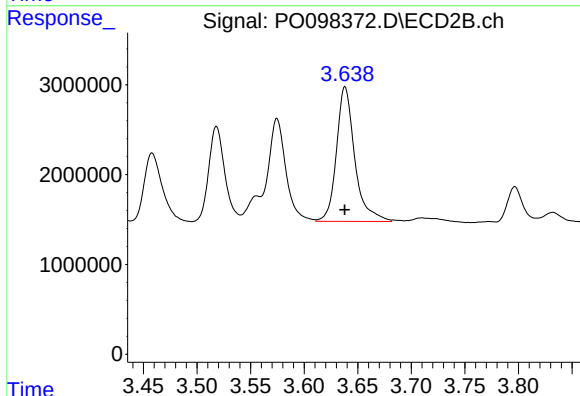


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 17800919
Conc: 22.86 ng/ml m

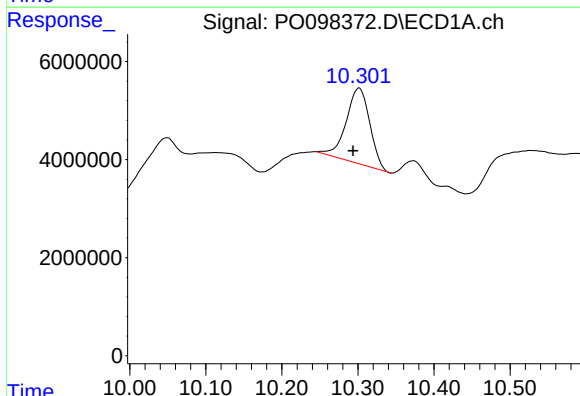

#2 Decachlorobiphenyl

R.T.: 10.301 min
Delta R.T.: 0.008 min
Response: 33160111
Conc: 27.32 ng/ml

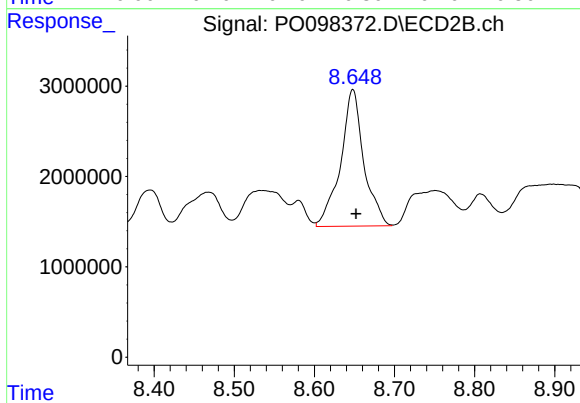

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.004 min
Response: 30558821
Conc: 57.04 ng/ml m