

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092920\
 Data File : P0071728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2020 14:33
 Operator : DD\AJ
 Sample : L4158-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BLUE-FRAC-TANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 16:04:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.524	1476665	746729	17.208	18.131
2) SA Decachlor...	9.950	8.700	2033514	1032304	17.700	16.983

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092920\
Data File : P0071728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2020 14:33
Operator : DD\AJ
Sample : L4158-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BLUE-FRAC-TANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 16:04:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

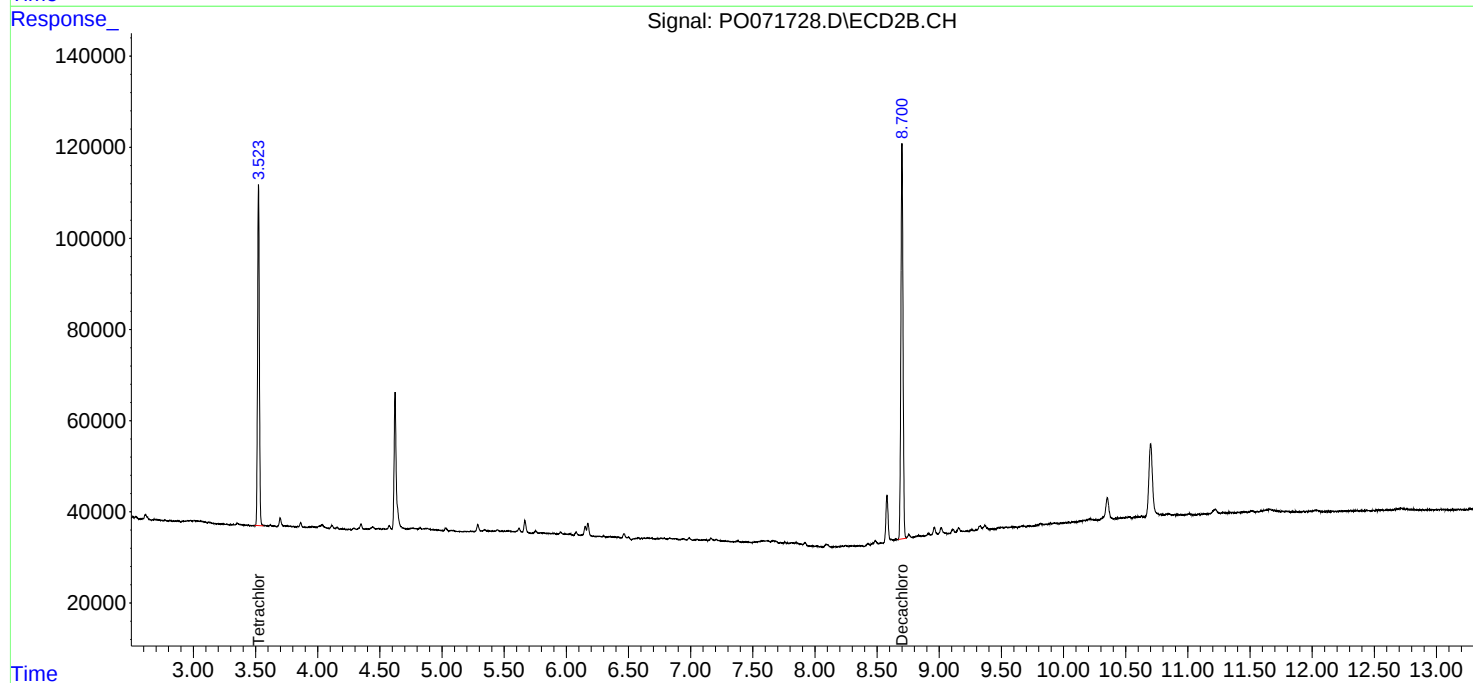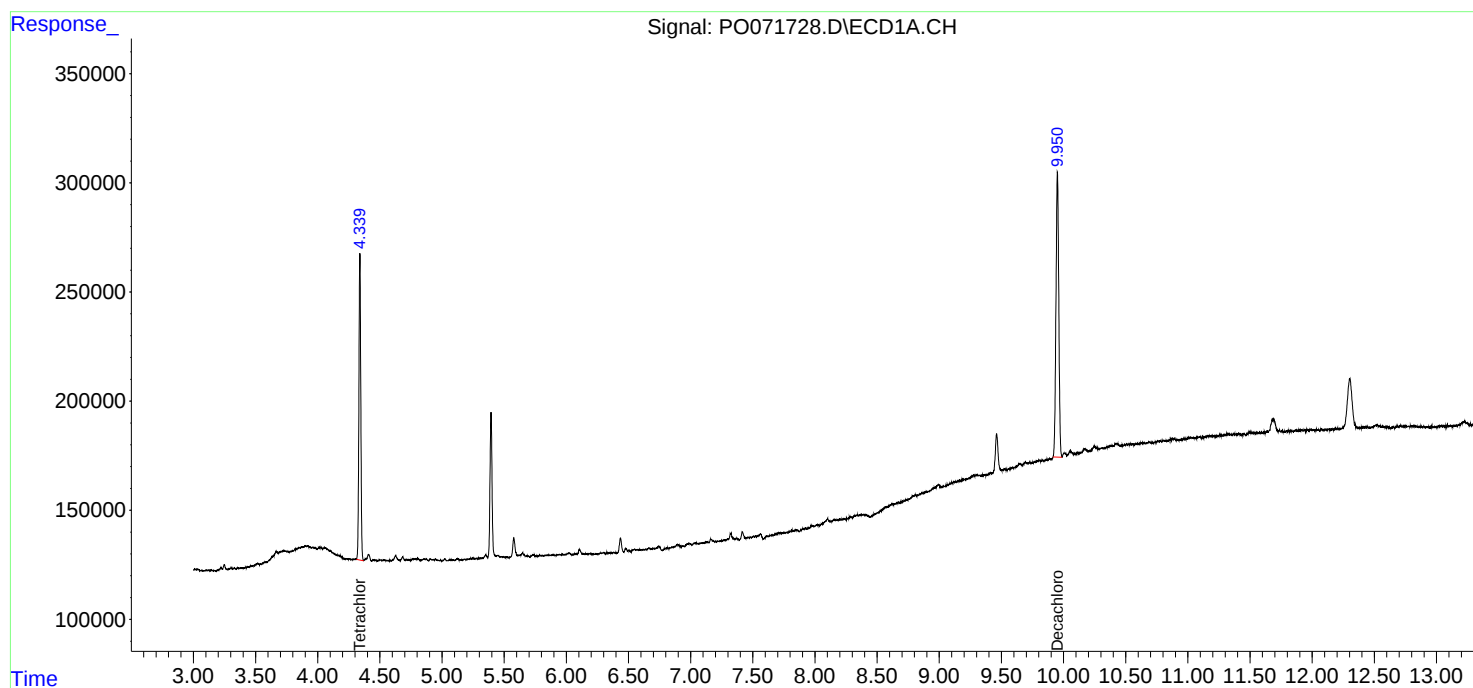


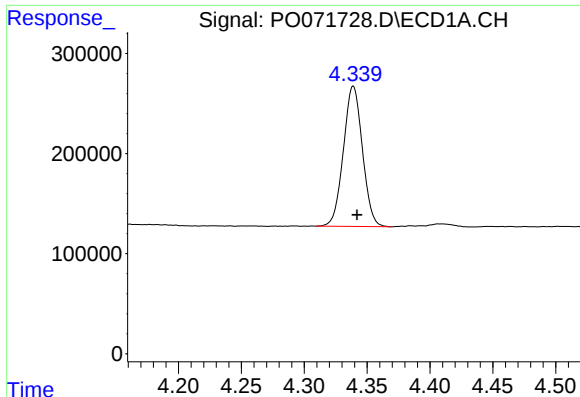

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.003 min
Response: 1476665
Conc: 17.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
BLUE-FRAC-TANK

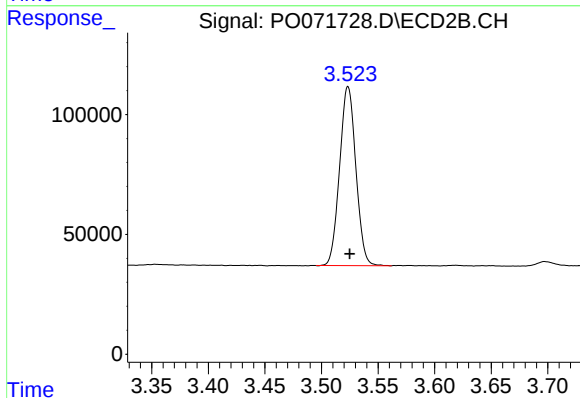


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.001 min
Response: 746729
Conc: 18.13 ng/ml

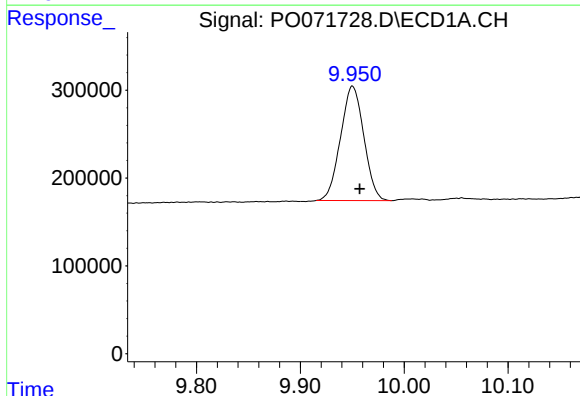

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.007 min
Response: 2033514
Conc: 17.70 ng/ml

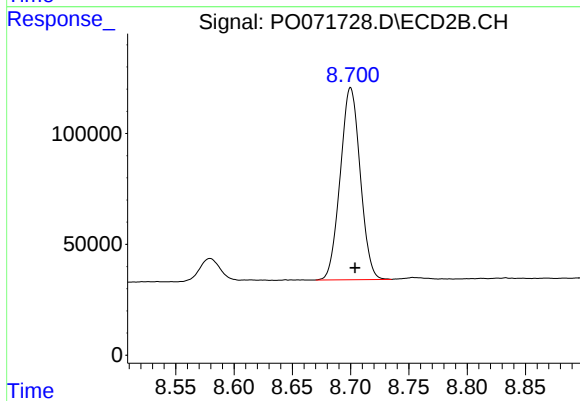

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.004 min
Response: 1032304
Conc: 16.98 ng/ml