

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092920\
 Data File : P0071733.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2020 16:02
 Operator : DD\AJ
 Sample : L3867-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-092820

Manual Integrations
 APPROVED

Ankita
 9/30/2020 2:29:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 04:04:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.526	2123024	1061932	24.740m	25.784
2) SA Decachlor...	9.955	8.703	2398455	1132254	20.877	18.627

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092920\
Data File : P0071733.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2020 16:02
Operator : DD\AJ
Sample : L3867-07
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-01-092820


Manual Integrations
APPROVED

Ankita
9/30/2020 2:29:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 04:04:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

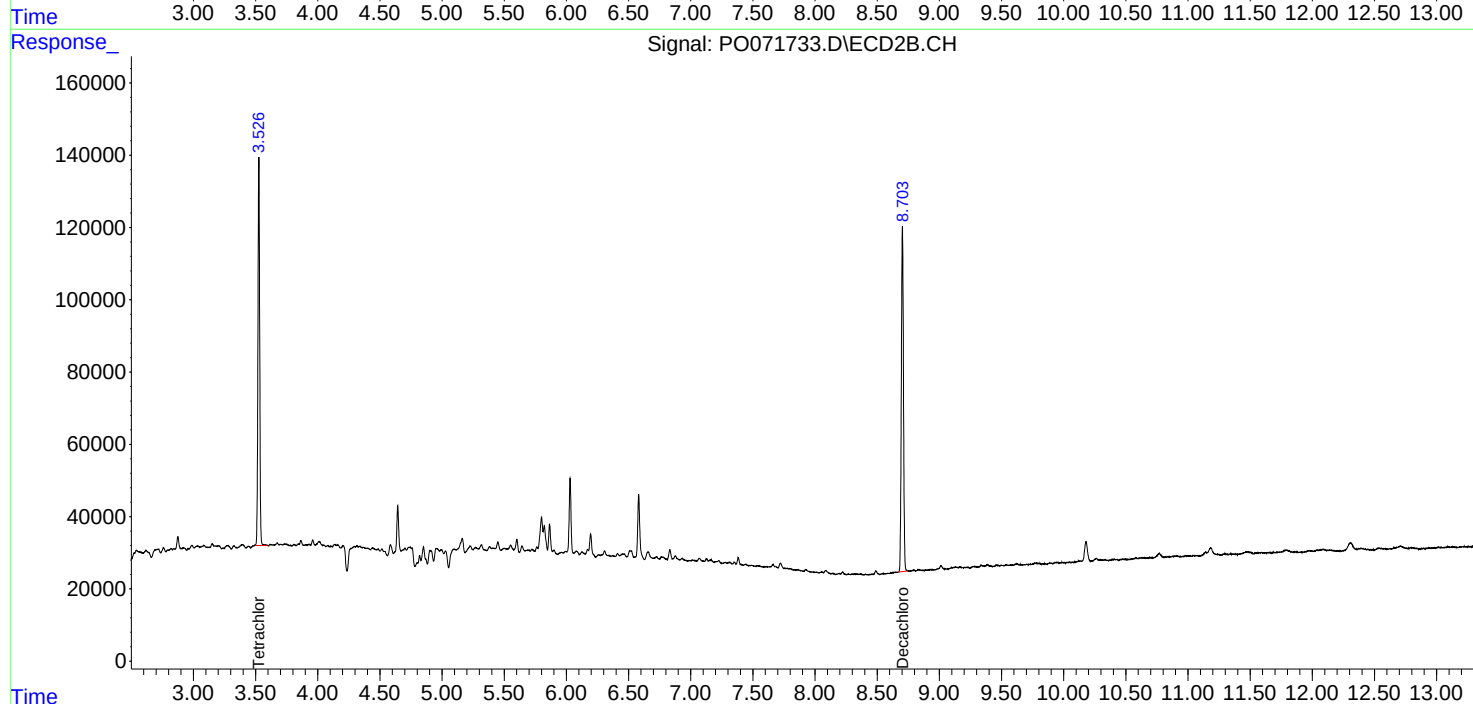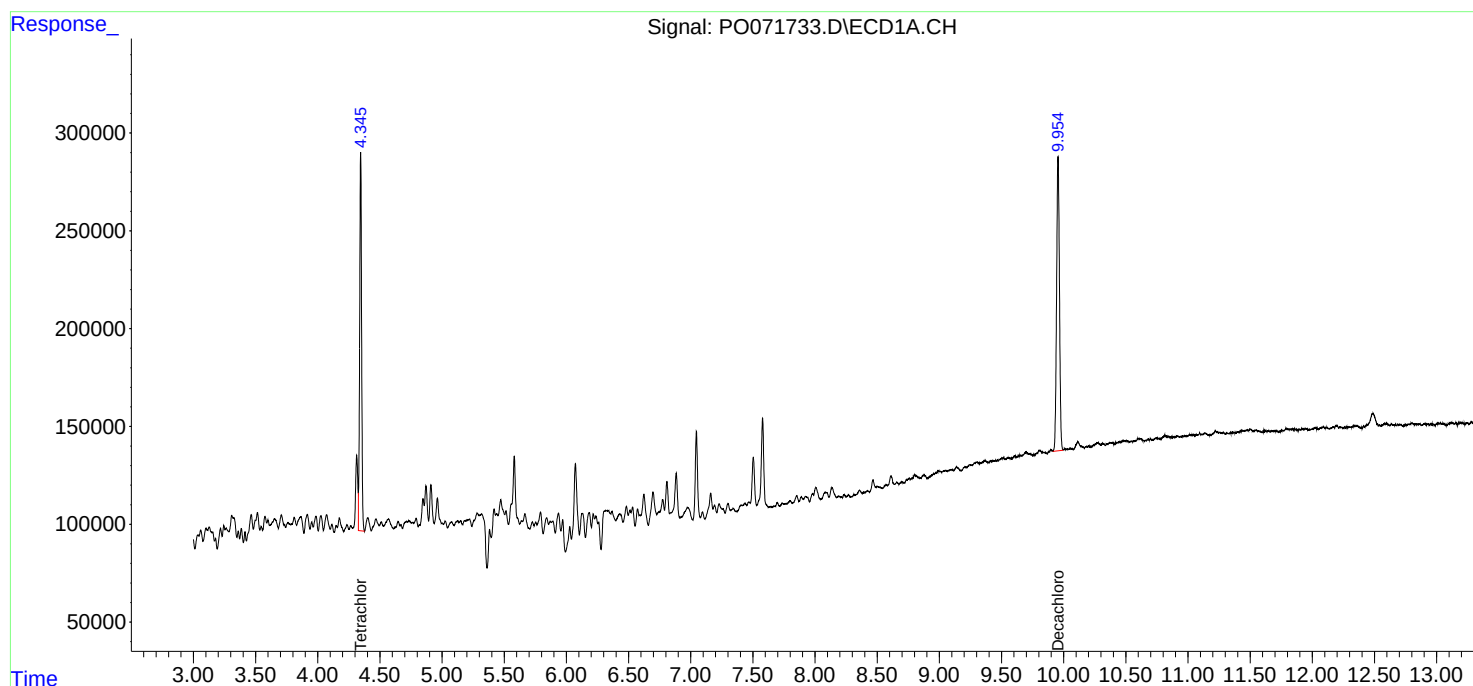

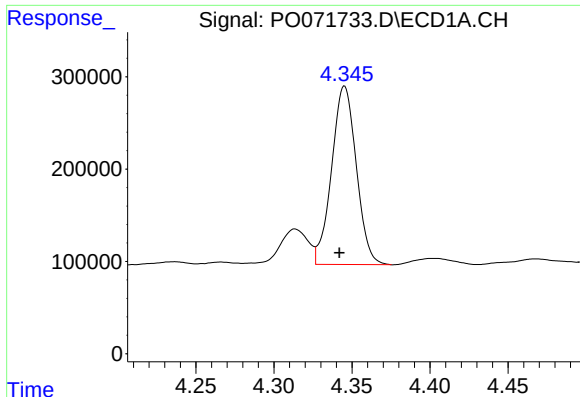


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.003 min
Response: 2123024
Conc: 24.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EO-01-092820


Manual Integrations
APPROVED

Ankita
9/30/2020 2:29:04 PM

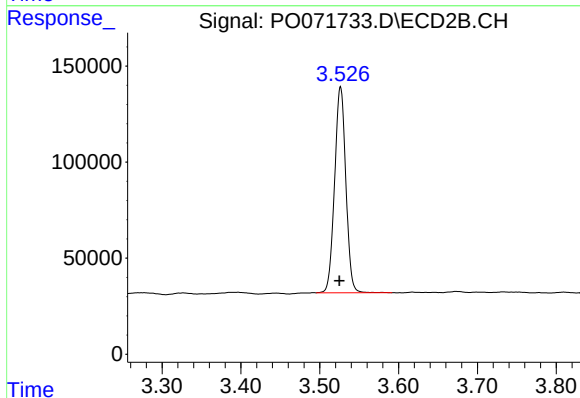


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: 0.001 min
Response: 1061932
Conc: 25.78 ng/ml

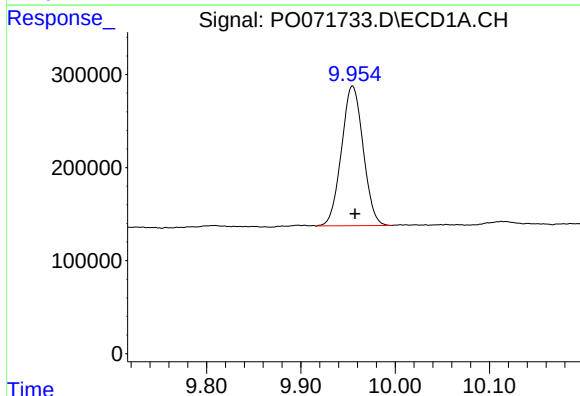

#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.003 min
Response: 2398455
Conc: 20.88 ng/ml

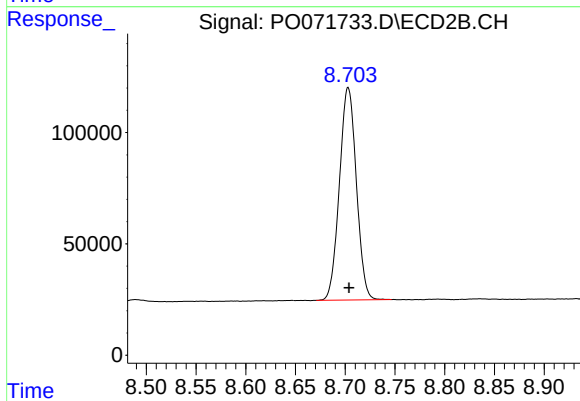

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.000 min
Response: 1132254
Conc: 18.63 ng/ml