

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092920\
 Data File : P0071736.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2020 16:54
 Operator : DD\AJ
 Sample : L4157-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA9581-END-2

Manual Integrations
 APPROVED

Ankita
 9/30/2020 2:29:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 04:32:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.534	1275234	991627	14.861	24.077 #
2) SA Decachlor...	9.979f	8.727f	1583823	804528	13.786m	13.236m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092920\
Data File : PO071736.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2020 16:54
Operator : DD\AJ
Sample : L4157-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
KMA9581-END-2


Manual Integrations
APPROVED

Ankita
9/30/2020 2:29:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 04:32:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

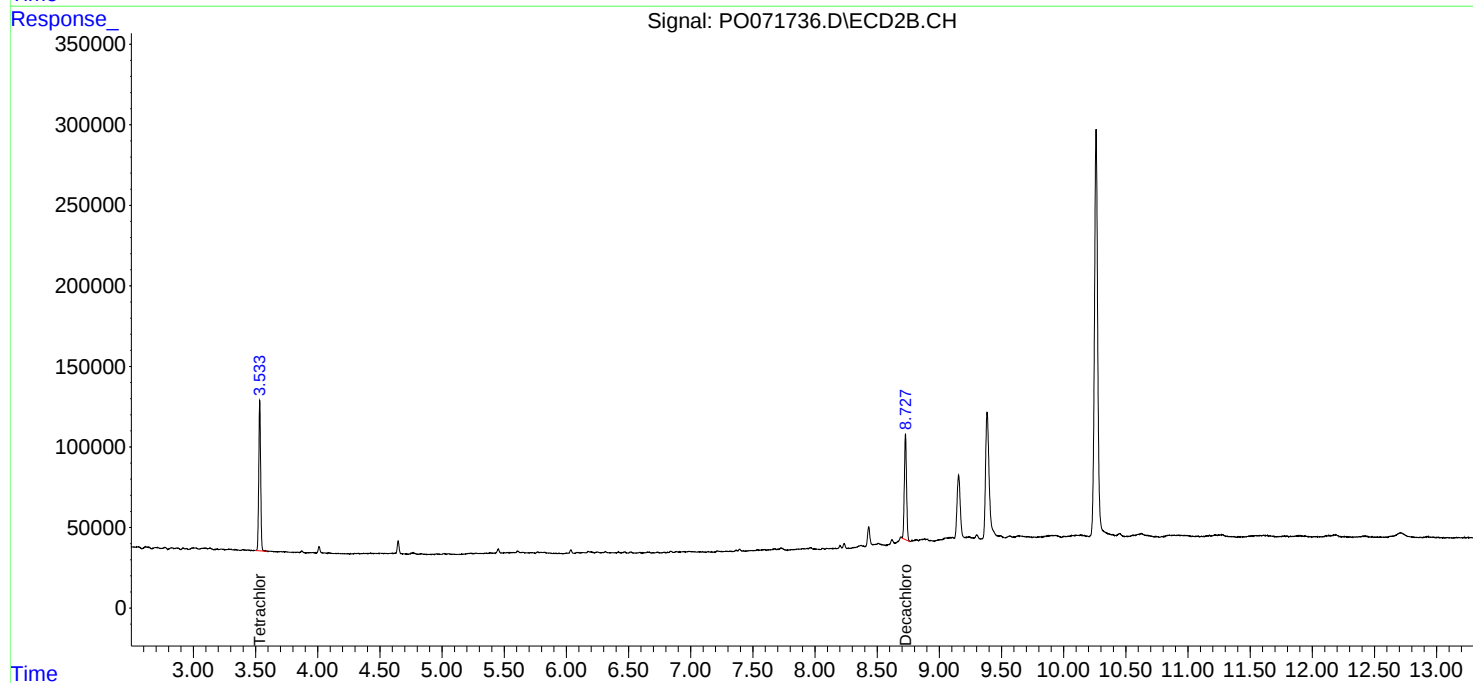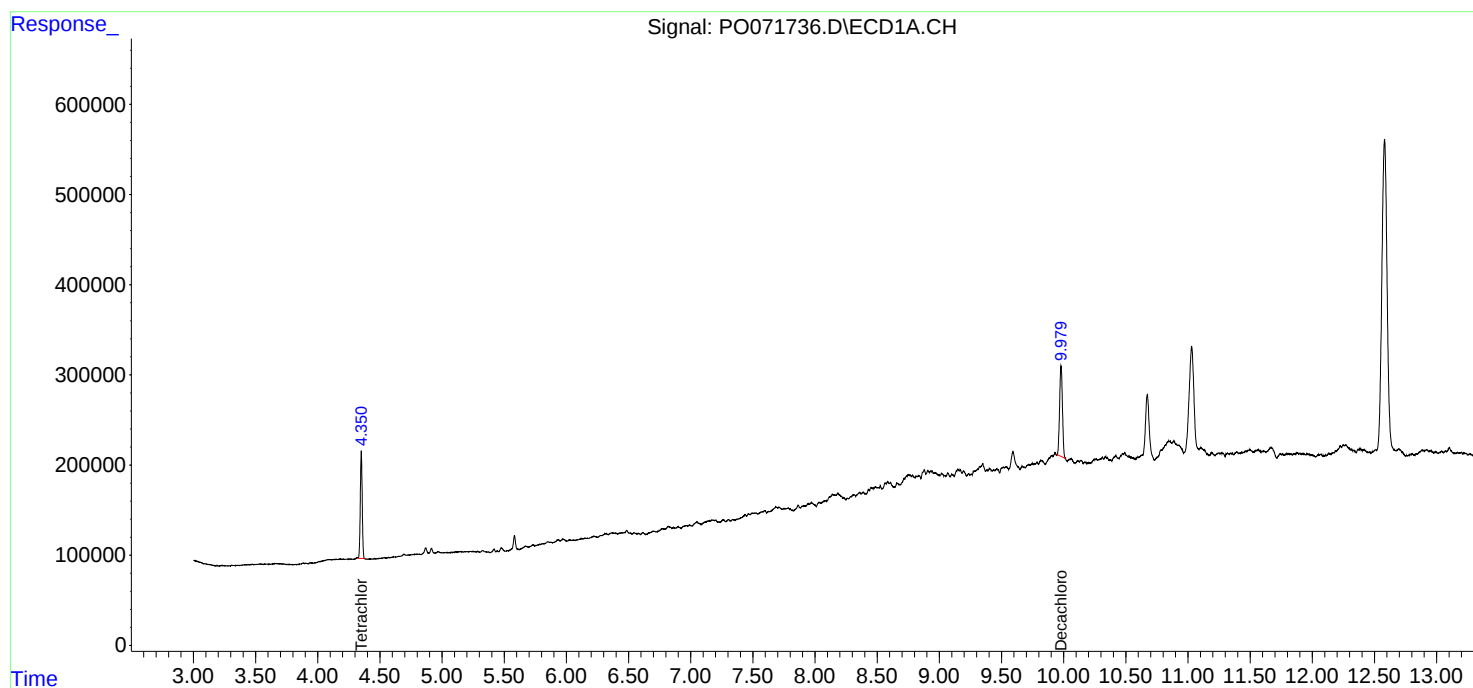

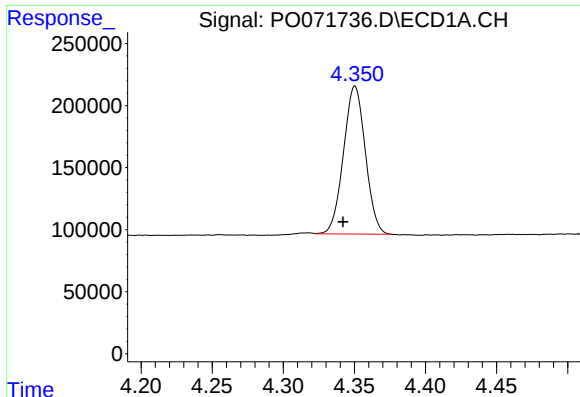


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: 0.008 min
Response: 1275234
Conc: 14.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA9581-END-2


Manual Integrations
APPROVED

Ankita
9/30/2020 2:29:09 PM

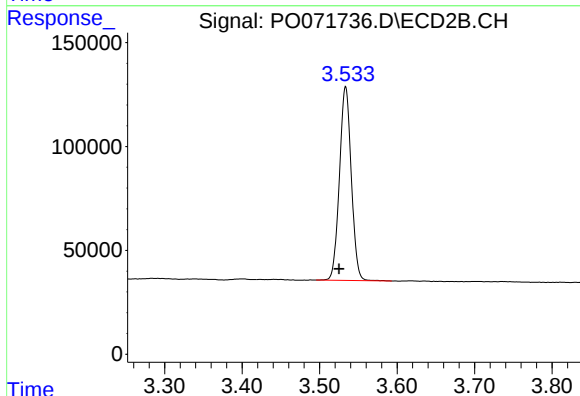


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.009 min
Response: 991627
Conc: 24.08 ng/ml

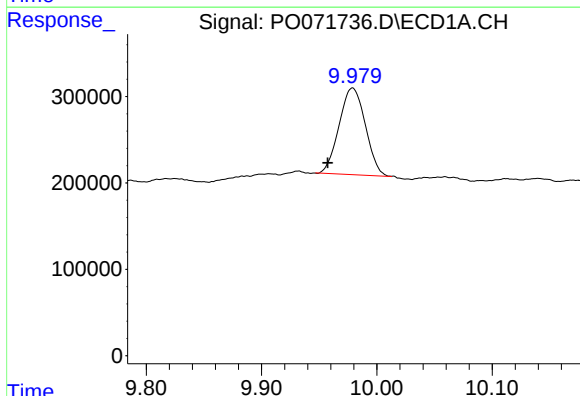

#2 Decachlorobiphenyl

R.T.: 9.979 min
Delta R.T.: 0.021 min
Response: 1583823
Conc: 13.79 ng/ml m

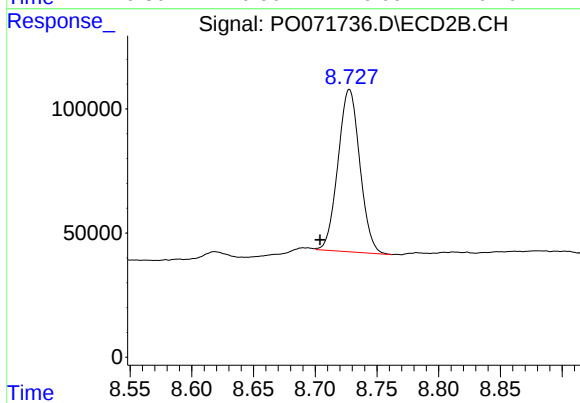

#2 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.024 min
Response: 804528
Conc: 13.24 ng/ml m