

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092921\
Data File : P0081634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2021 14:32
Operator : AJ\MA
Sample : M3965-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CC-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:33:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.870	3.985	2318607	643268	26.000	24.145
2) SA Decachlor...	10.882	9.333	1966461	613325	26.400	26.411

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092921\
Data File : P0081634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2021 14:32
Operator : AJ\MA
Sample : M3965-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CC-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 01:33:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

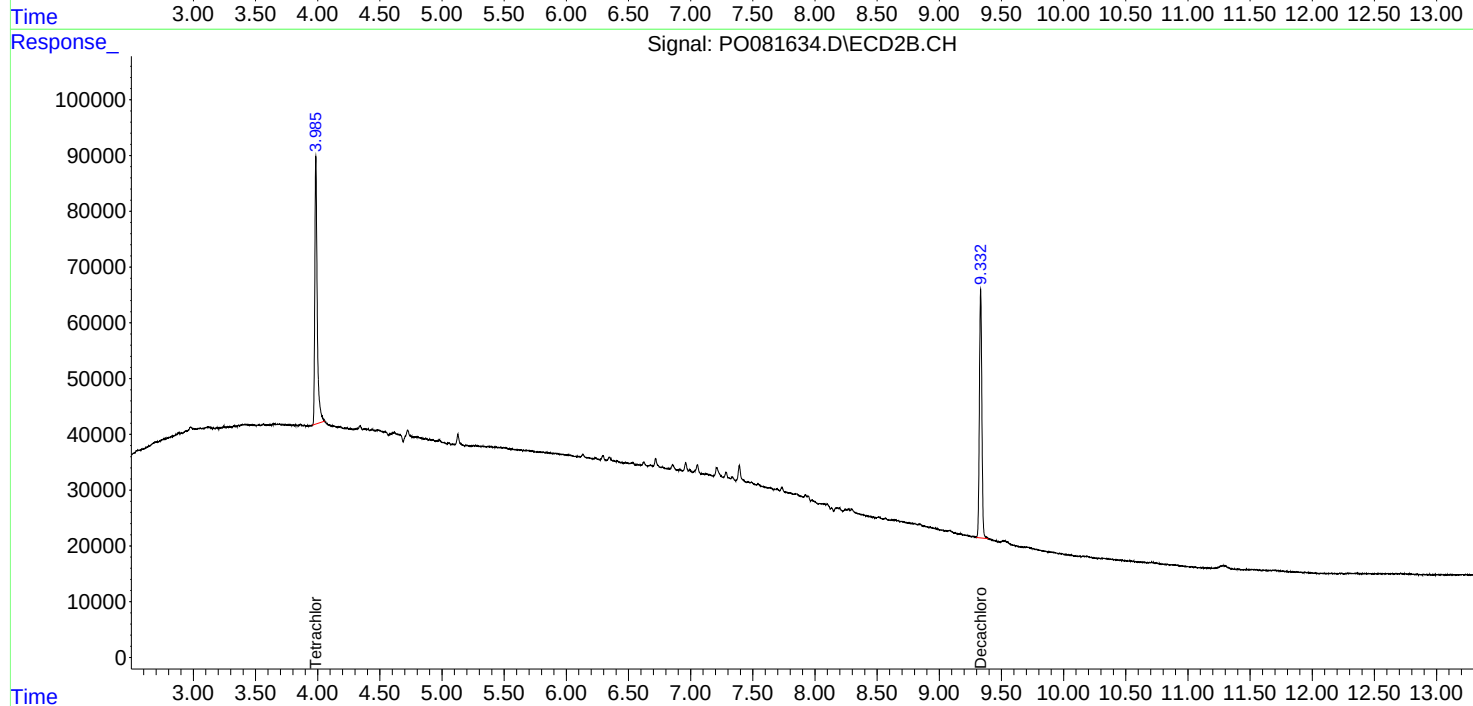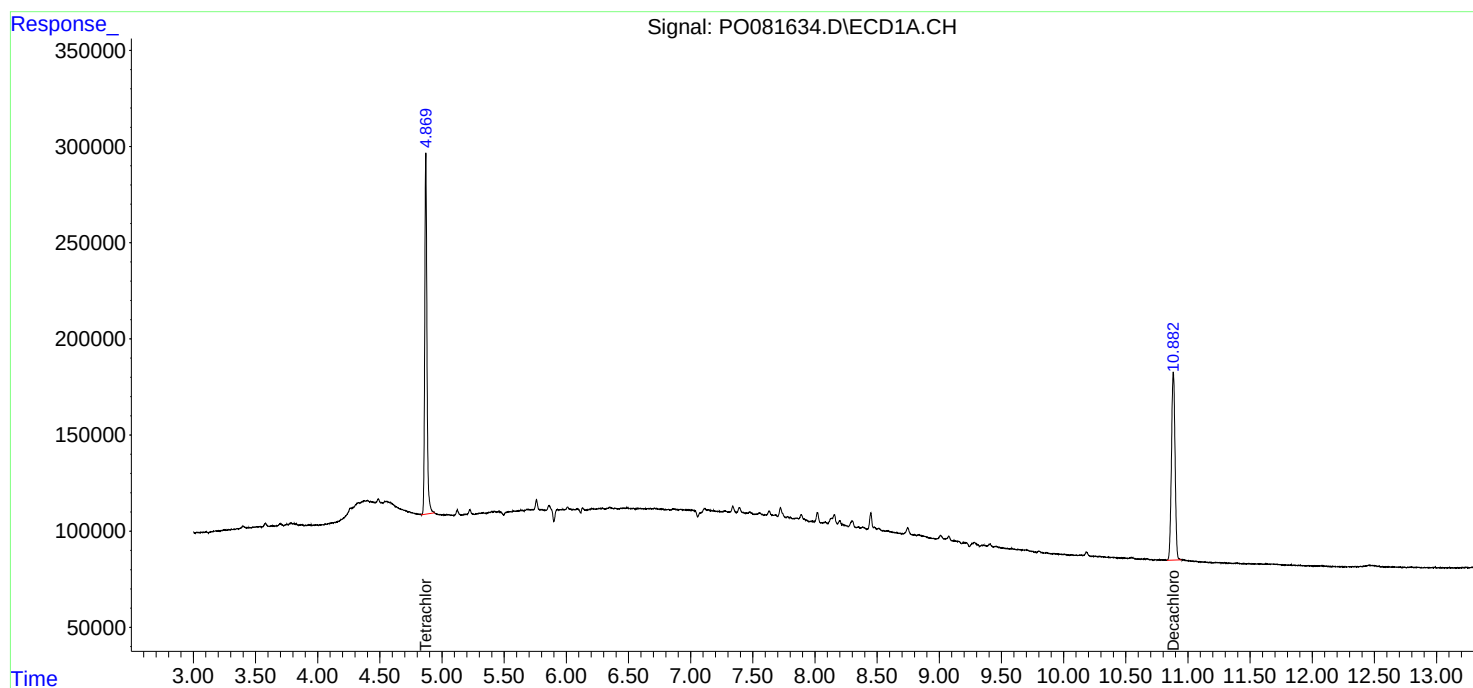


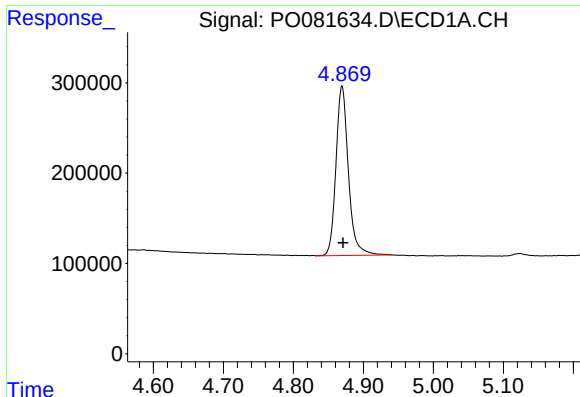

#1 Tetrachloro-m-xylene


R.T.: 4.870 min
Delta R.T.: -0.001 min
Response: 2318607
Conc: 26.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC-24

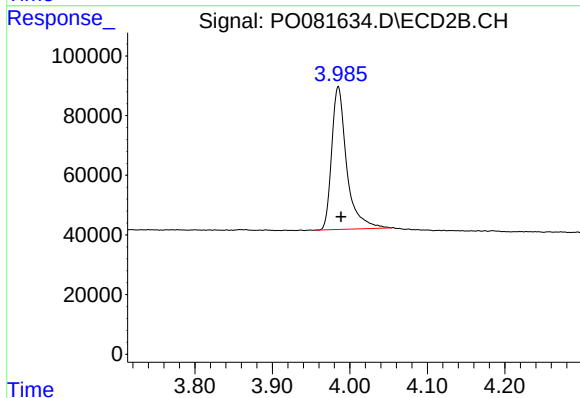


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 643268
Conc: 24.14 ng/ml

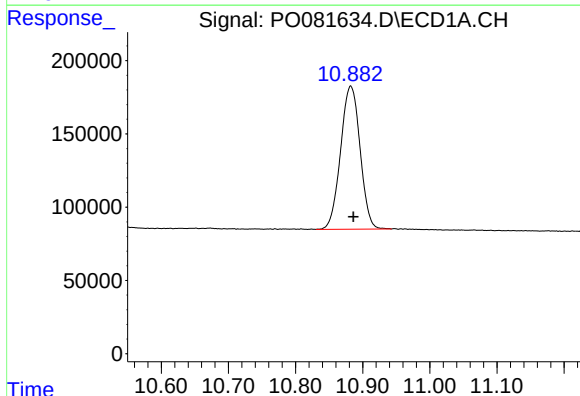

#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.004 min
Response: 1966461
Conc: 26.40 ng/ml

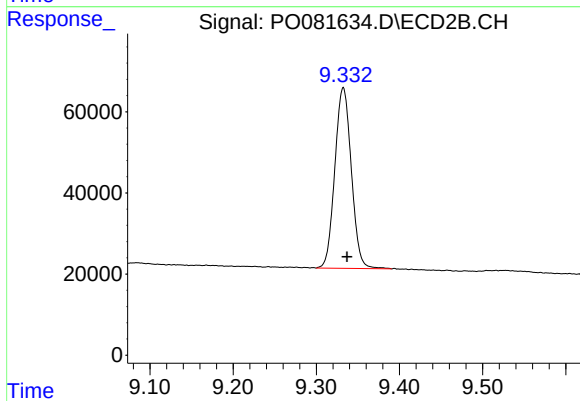

#2 Decachlorobiphenyl

R.T.: 9.333 min
Delta R.T.: -0.004 min
Response: 613325
Conc: 26.41 ng/ml