

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092925\
 Data File : P0114103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Sep 2025 17:02
 Operator : YP/AJ
 Sample : Q3221-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-01-092625

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/30/2025
 Supervised By :mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 02:36:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.648	141.0E6	78569064	15.992m	14.711m
2) SA Decachlor...	8.665	8.608	67959058	22973960	10.158	11.004

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092925\
Data File : PO114103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Sep 2025 17:02
Operator : YP/AJ
Sample : Q3221-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-01-092625


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 02:36:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

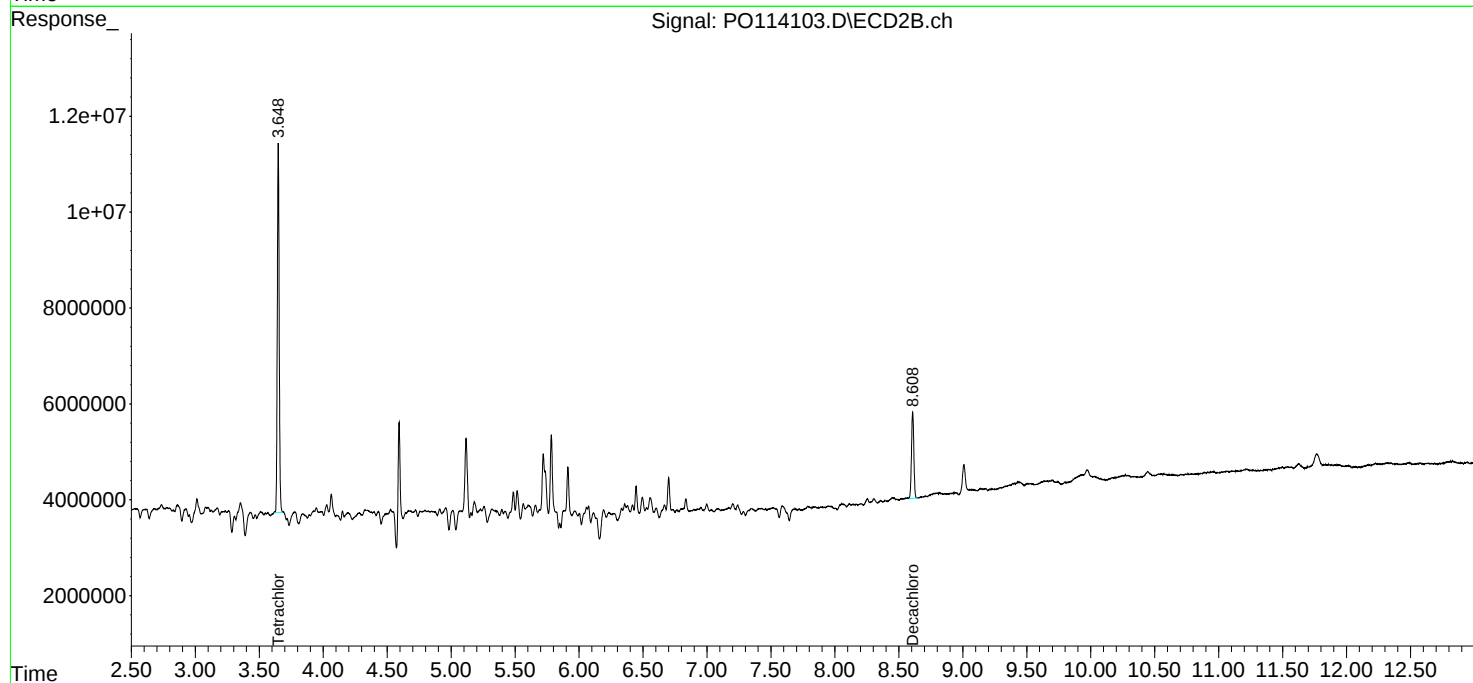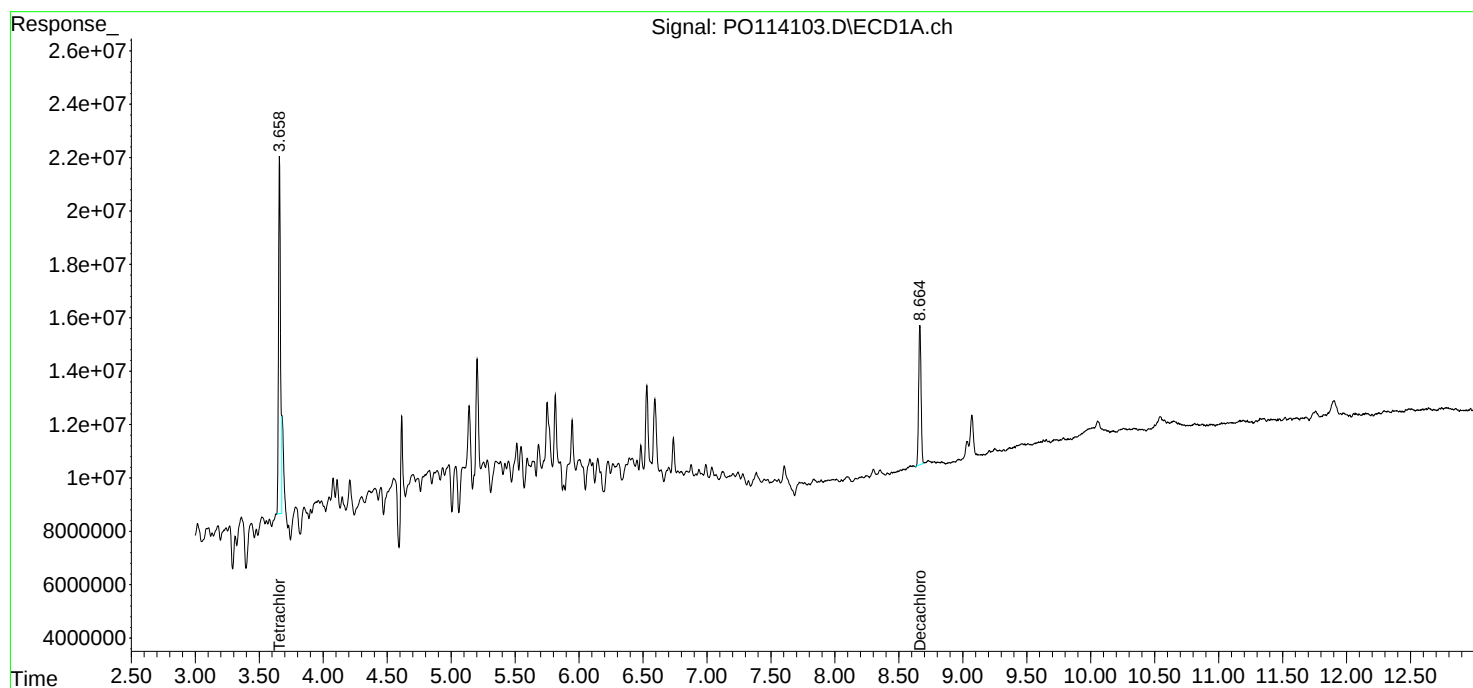

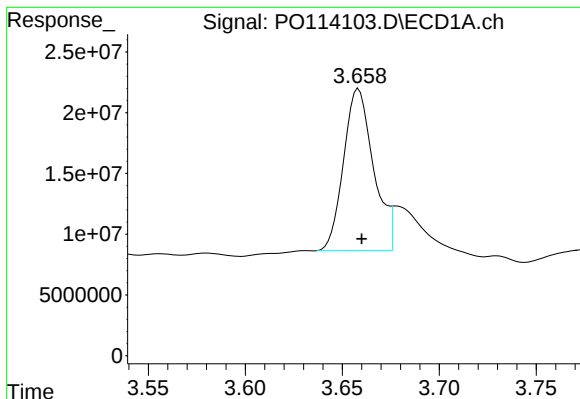


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.002 min
Response: 141044001
Conc: 15.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-01-092625


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

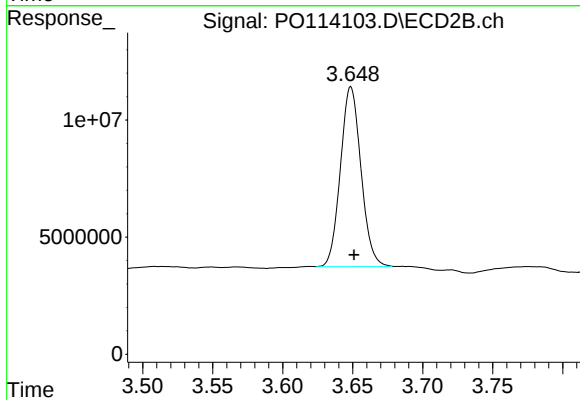


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 78569064
Conc: 14.71 ng/ml m

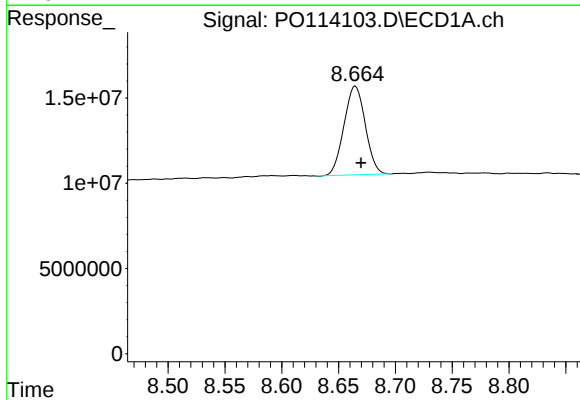

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.005 min
Response: 67959058
Conc: 10.16 ng/ml

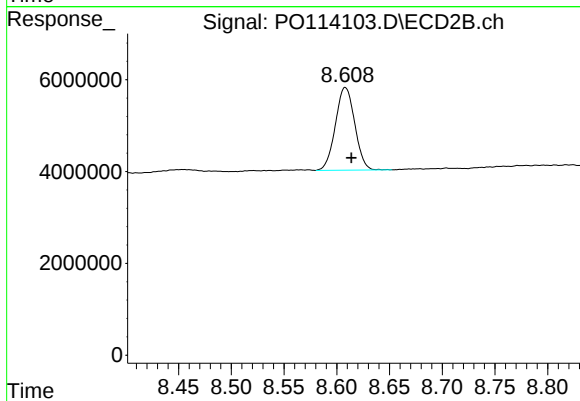

#2 Decachlorobiphenyl

R.T.: 8.608 min
Delta R.T.: -0.006 min
Response: 22973960
Conc: 11.00 ng/ml