

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092925\
 Data File : P0114126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Sep 2025 07:39
 Operator : YP/AJ
 Sample : Q3224-01 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 60159

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/30/2025
 Supervised By :mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 07:54:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.658	3.649	7962635	8092606	0.903m	1.515 #
2) SA Decachlor...	8.665	8.604	34094954	1643778	5.096	0.787m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092925\
Data File : PO114126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Sep 2025 07:39
Operator : YP/AJ
Sample : Q3224-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
60159


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 07:54:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

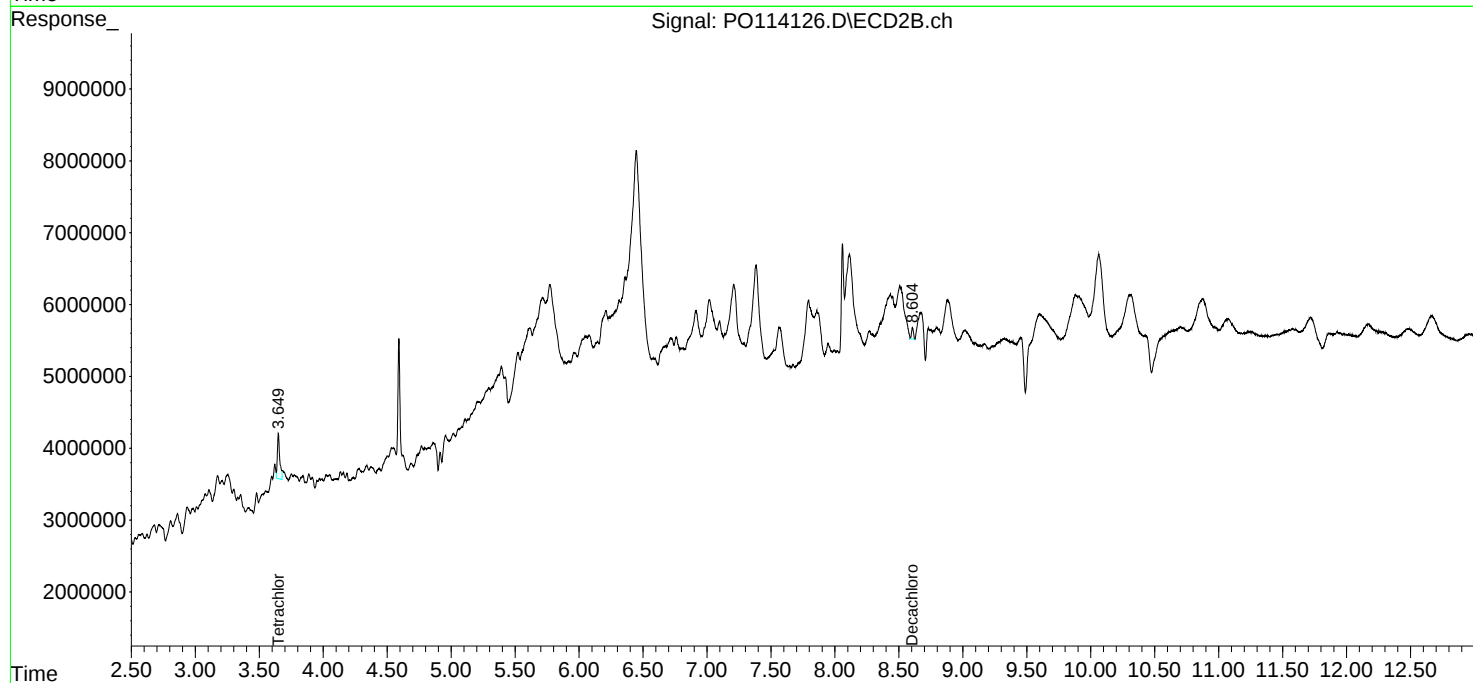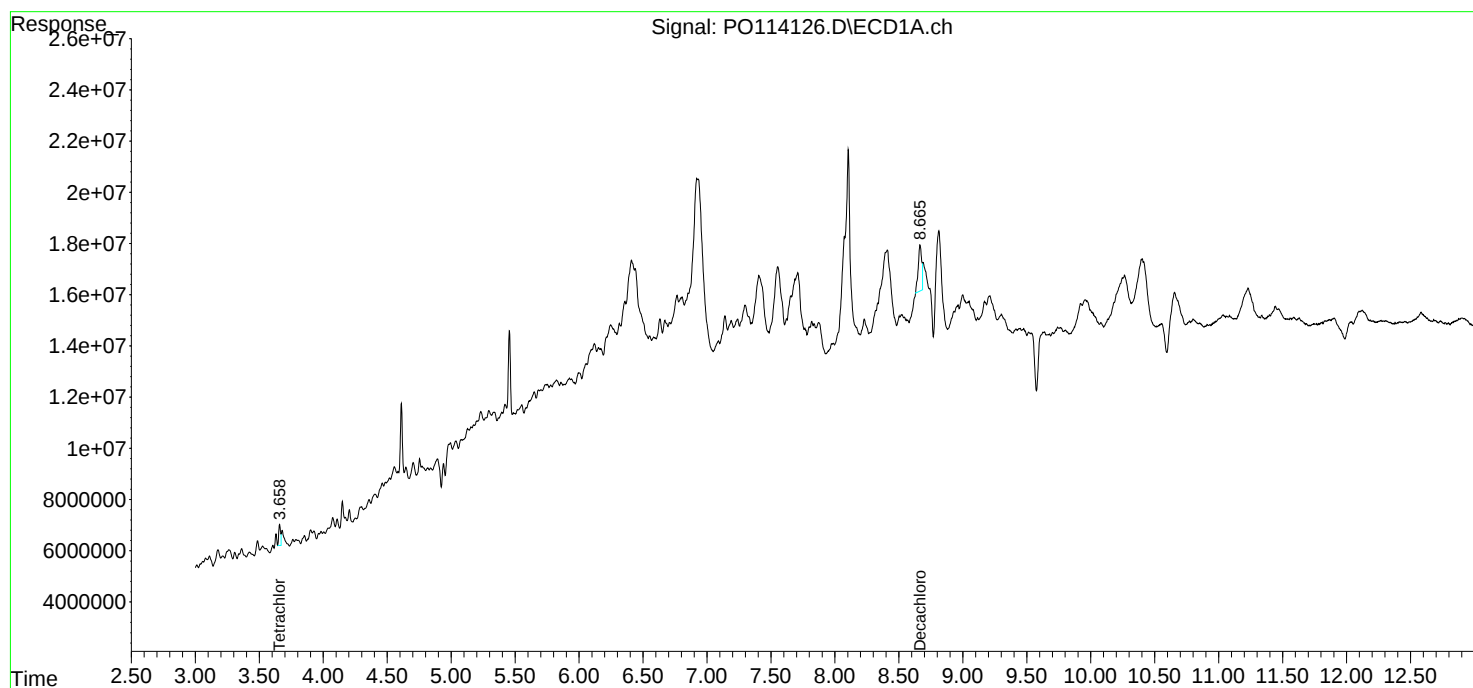

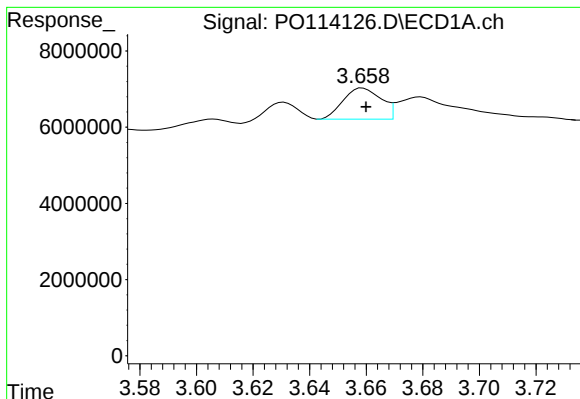


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.002 min
Response: 7962635
Conc: 0.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
60159


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/30/2025
Supervised By :mohammad ahmed 10/01/2025

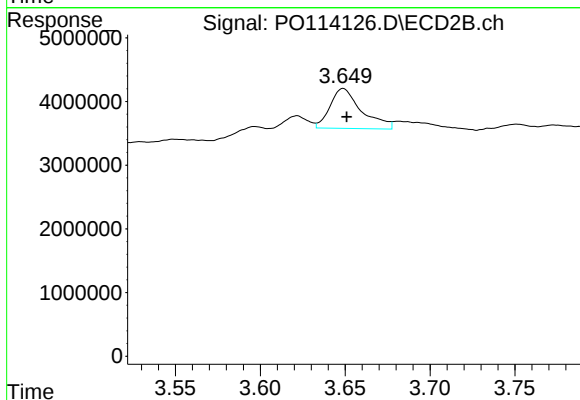


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 8092606
Conc: 1.52 ng/ml

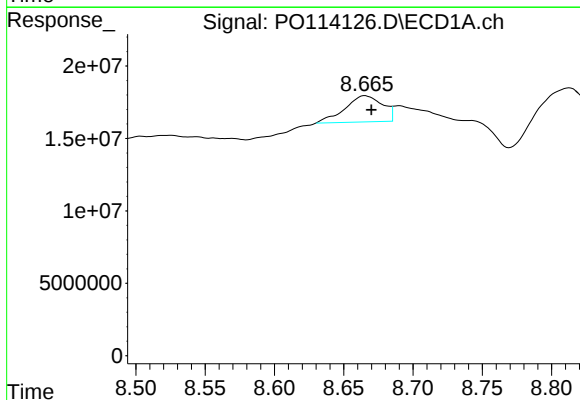

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.005 min
Response: 34094954
Conc: 5.10 ng/ml

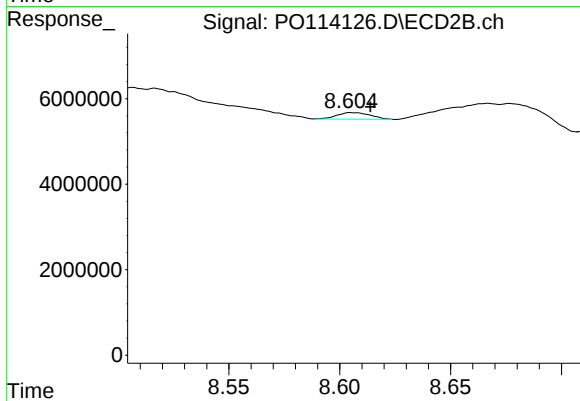

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: -0.010 min
Response: 1643778
Conc: 0.79 ng/ml m