

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2020 17:35
 Operator : DD\AJ
 Sample : L4157-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA9581-END-2

Manual Integrations
 APPROVED

Ankita
 10/1/2020 3:32:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 18:22:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.356	3.538	1529145	1118819	17.819m	27.165 #
2) SA Decachlor...	9.985f	8.732f	1788924	887069	15.571m	14.594m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093020\
Data File : PO071769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2020 17:35
Operator : DD\AJ
Sample : L4157-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA9581-END-2


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 18:22:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

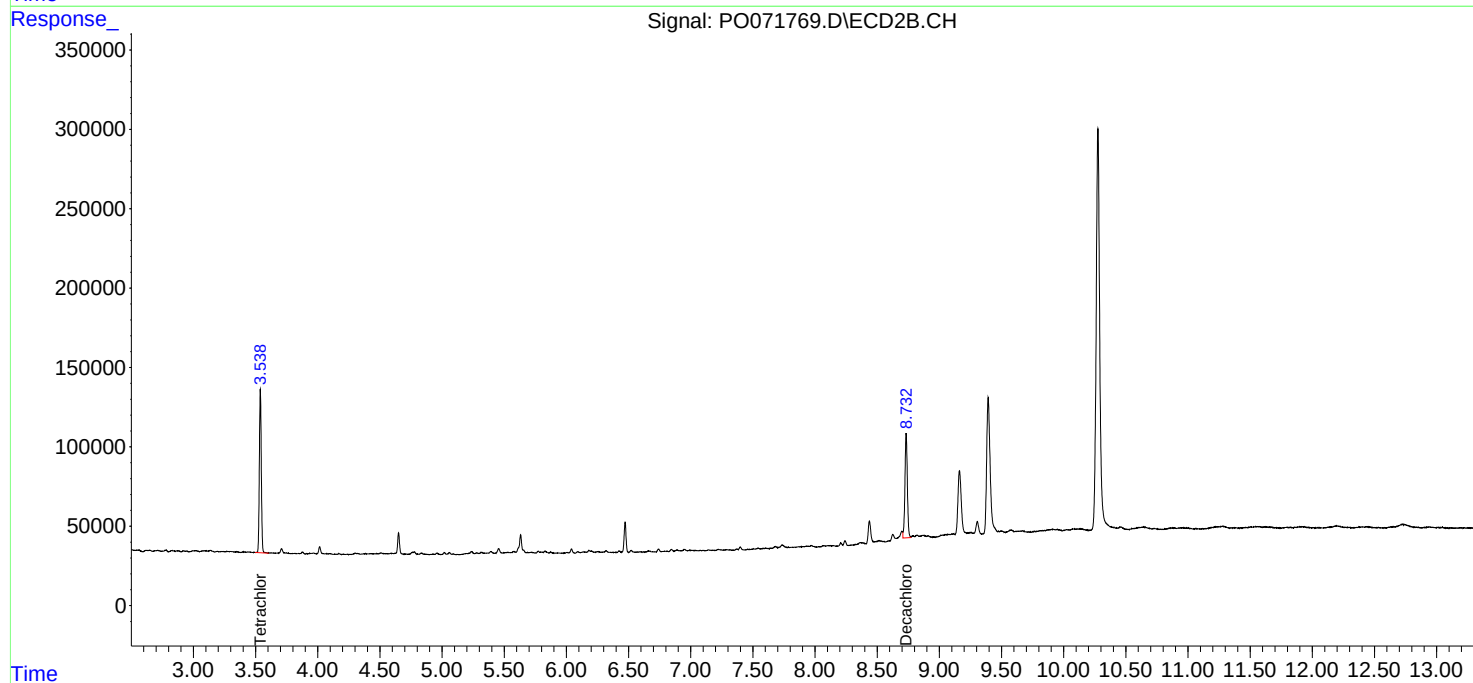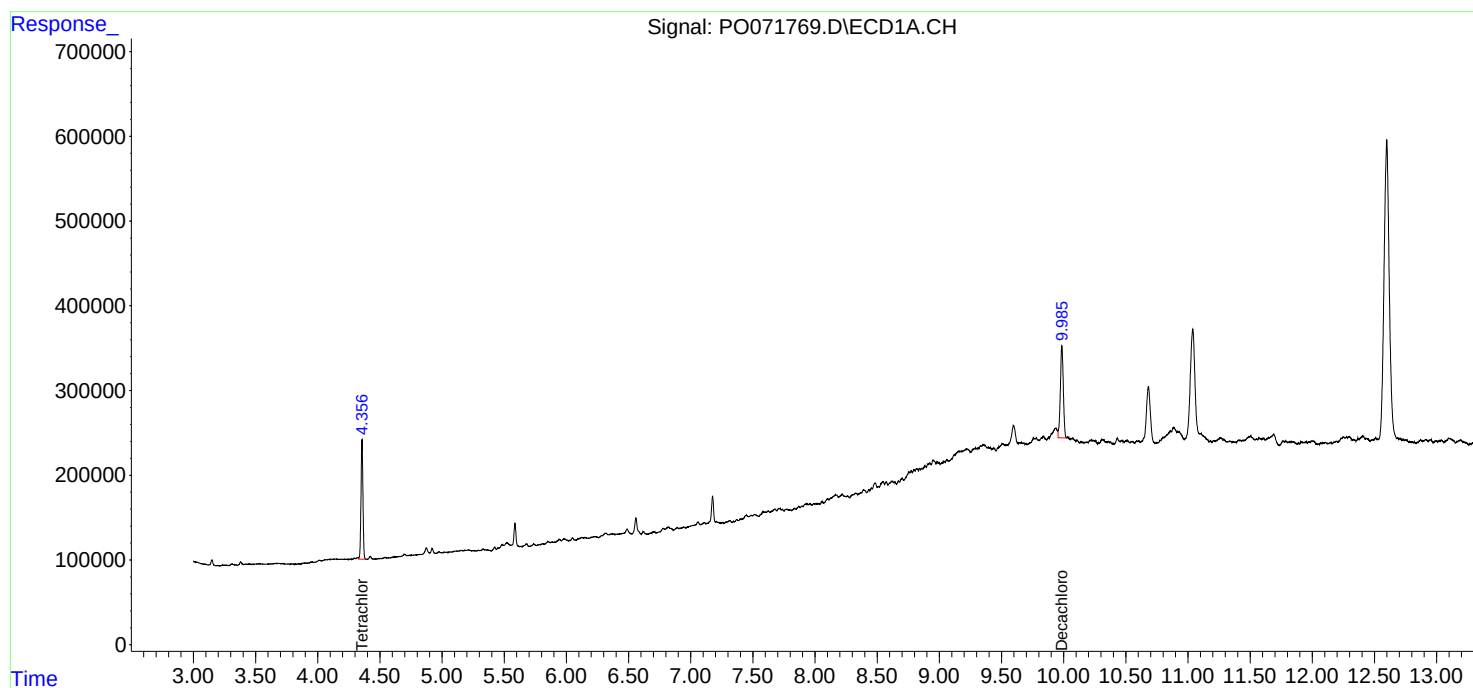

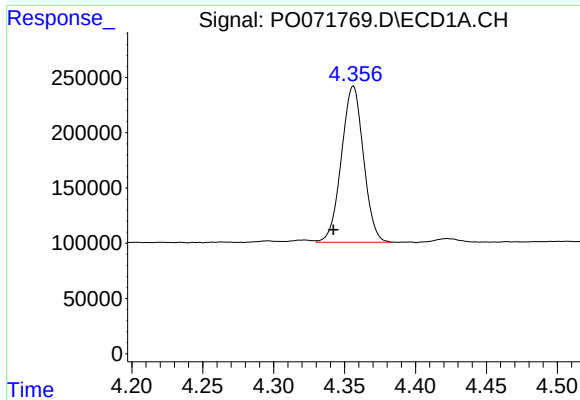


#1 Tetrachloro-m-xylene

R.T.: 4.356 min
Delta R.T.: 0.014 min
Response: 1529145
Conc: 17.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KMA9581-END-2


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:39 PM

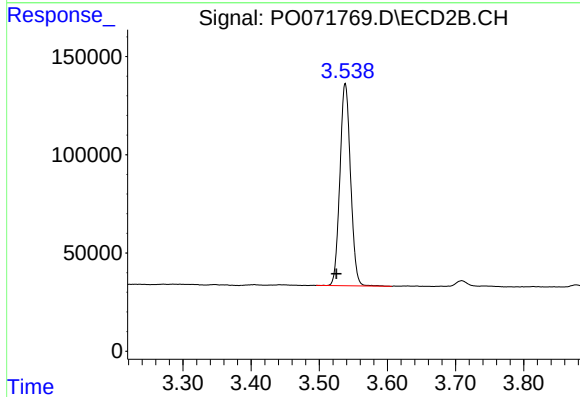


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.013 min
Response: 1118819
Conc: 27.17 ng/ml

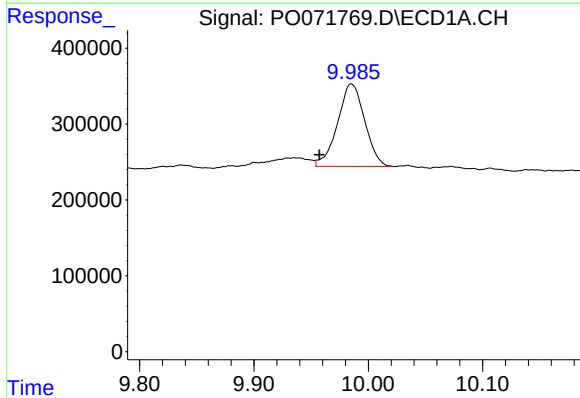

#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: 0.027 min
Response: 1788924
Conc: 15.57 ng/ml m

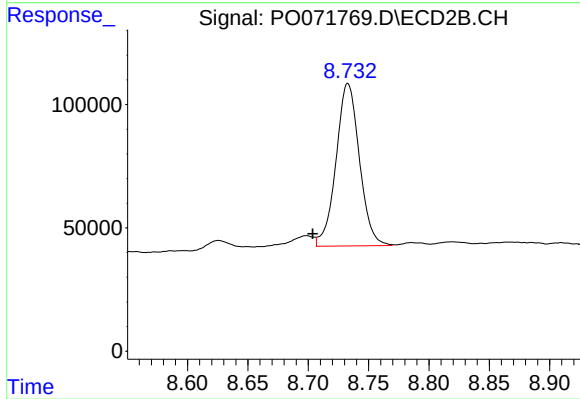

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: 0.029 min
Response: 887069
Conc: 14.59 ng/ml m