

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071770.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2020 17:52
 Operator : DD\AJ
 Sample : L4161-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH490H-END-2

Manual Integrations
 APPROVED

Ankita
 10/1/2020 3:32:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 18:23:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.357	3.539	1358797	1036901	15.834m	25.176 #
2) SA Decachlor...	9.976f	8.719f	1628022	861623	14.171m	14.175m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
Data File : P0071770.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2020 17:52
Operator : DD\AJ
Sample : L4161-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH490H-END-2


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 18:23:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

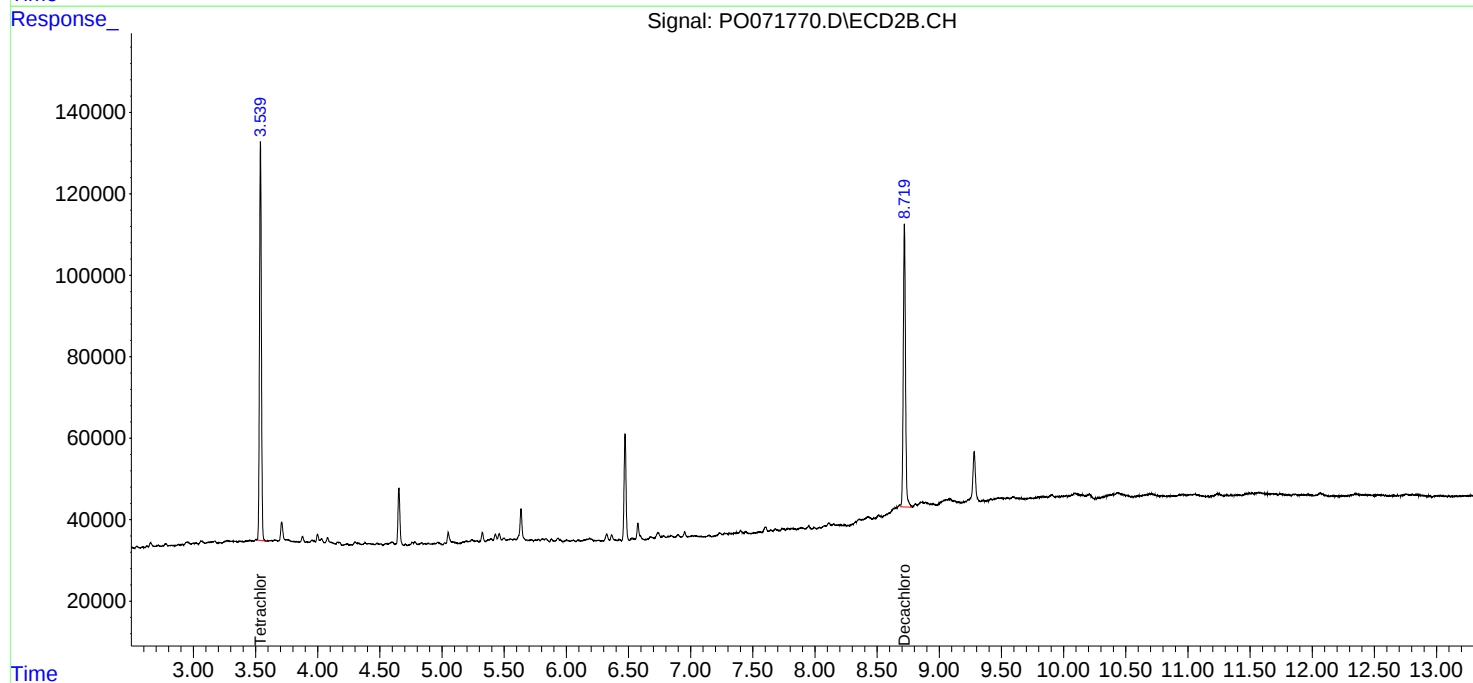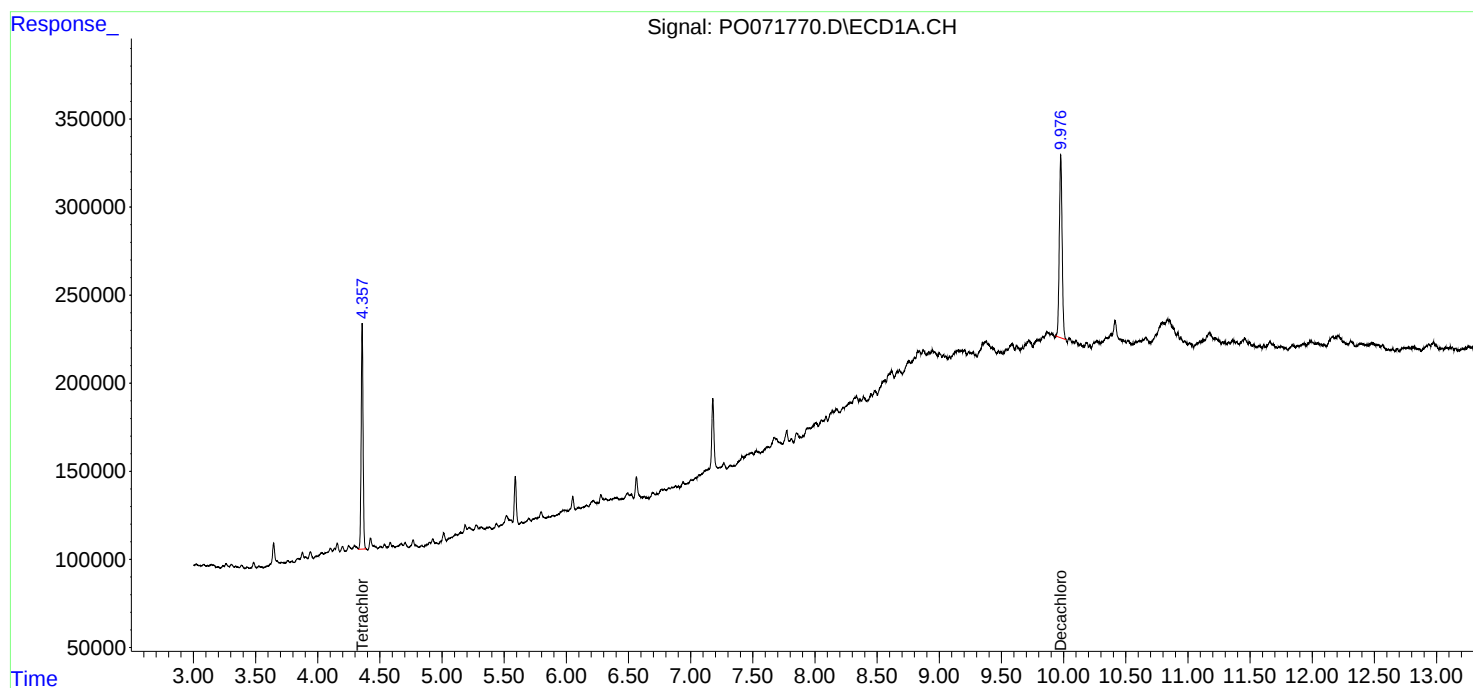

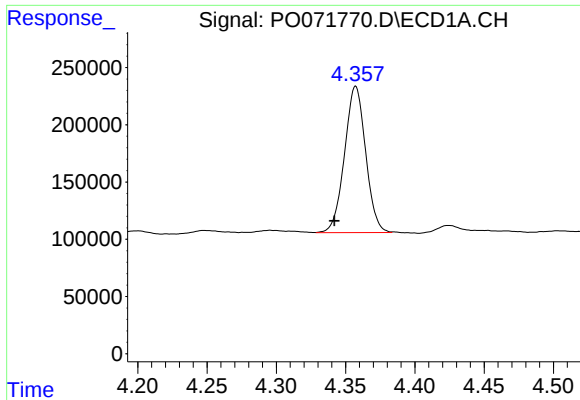


#1 Tetrachloro-m-xylene

R.T.: 4.357 min
Delta R.T.: 0.015 min
Response: 1358797
Conc: 15.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KMH490H-END-2


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:40 PM

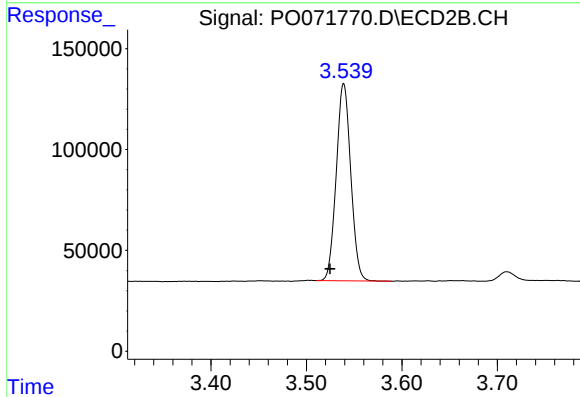


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.014 min
Response: 1036901
Conc: 25.18 ng/ml

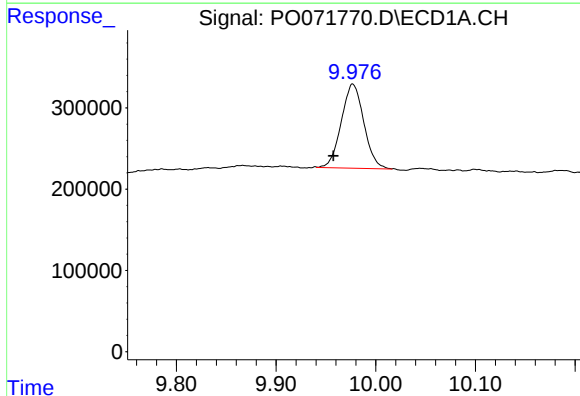

#2 Decachlorobiphenyl

R.T.: 9.976 min
Delta R.T.: 0.019 min
Response: 1628022
Conc: 14.17 ng/ml m

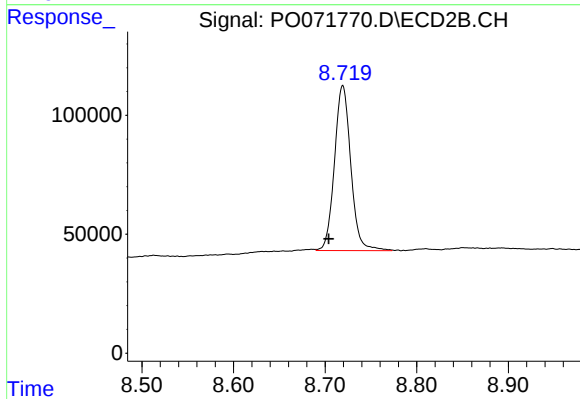

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: 0.015 min
Response: 861623
Conc: 14.17 ng/ml m