

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2020 19:35
 Operator : DD\AJ
 Sample : L4173-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3-(0-6FT)

Manual Integrations
 APPROVED

Ankita
 10/1/2020 3:32:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:47:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.533	2186120	1117827	25.475m	27.141
2) SA Decachlor...	9.963	8.707	1503397	853158	13.086	14.036

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
Data File : P0071776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2020 19:35
Operator : DD\AJ
Sample : L4173-10
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-3-(0-6FT)


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:47:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

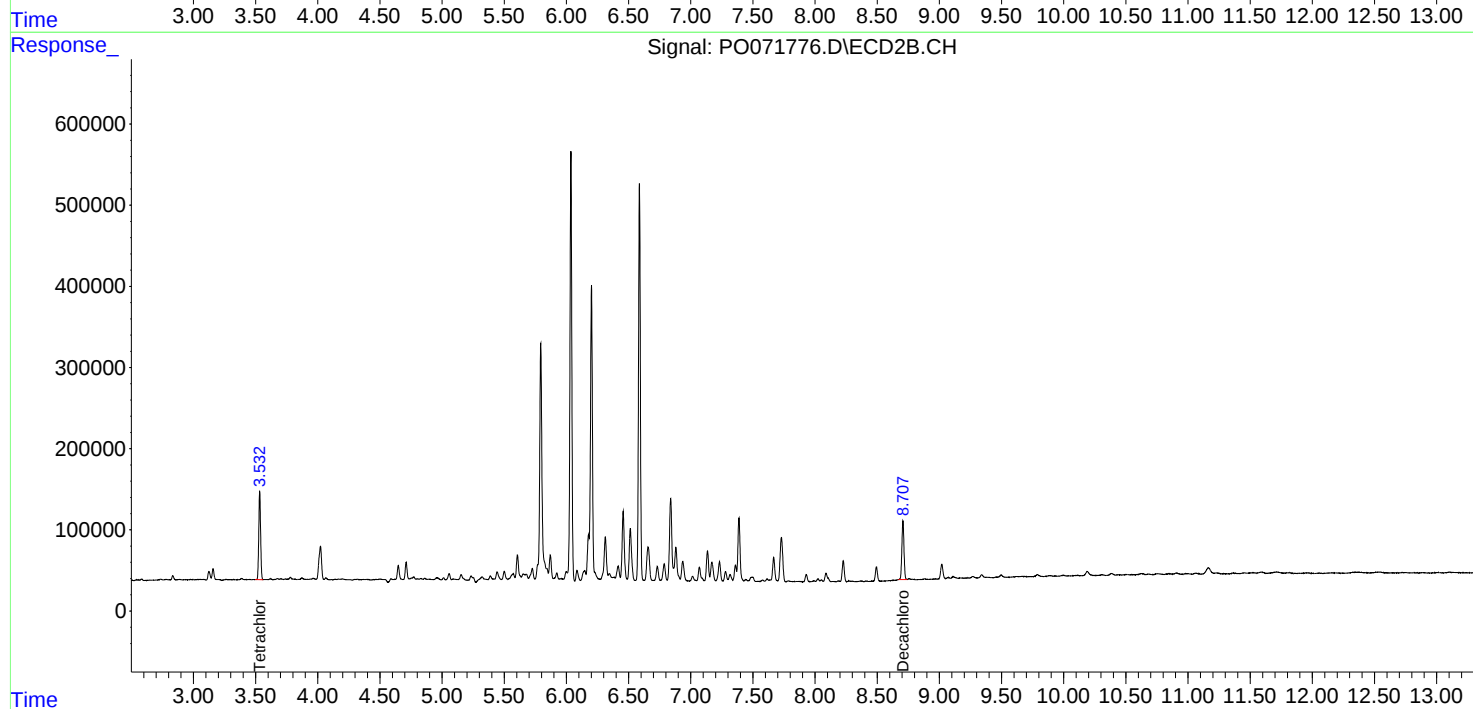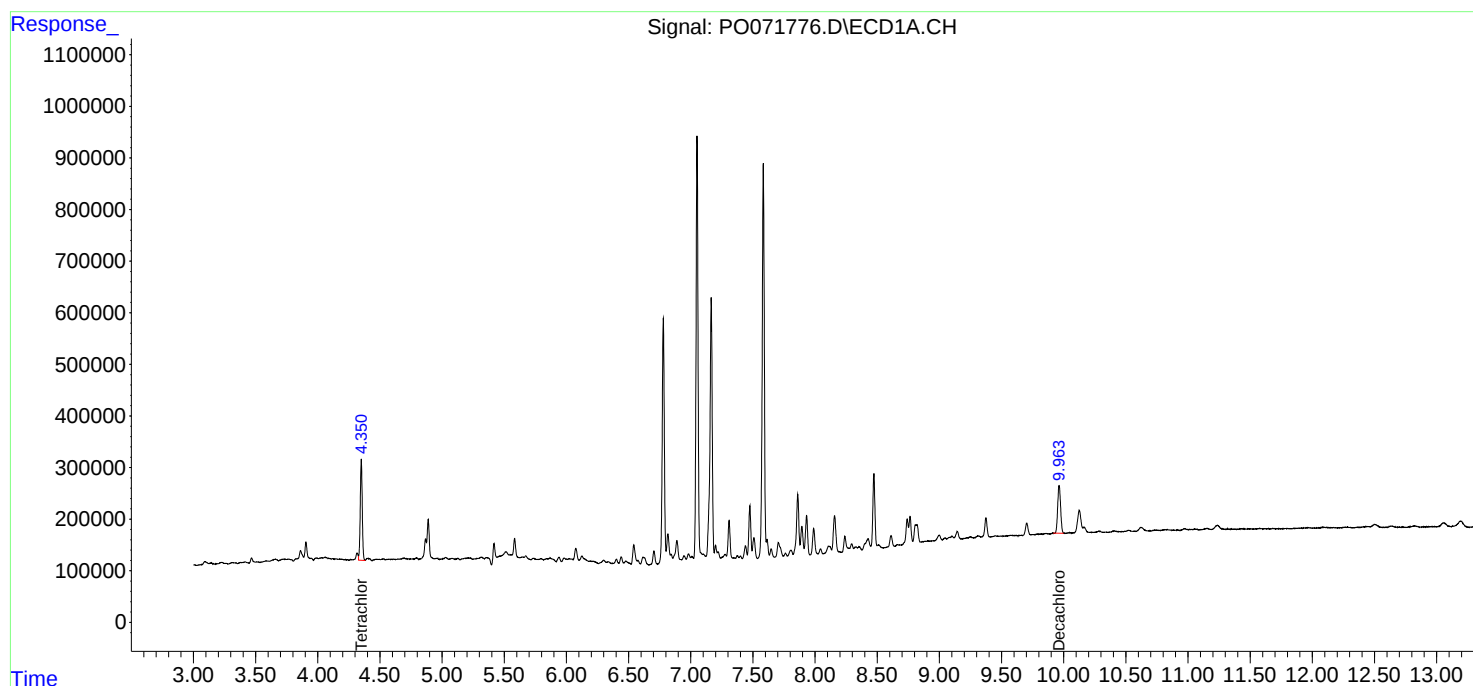

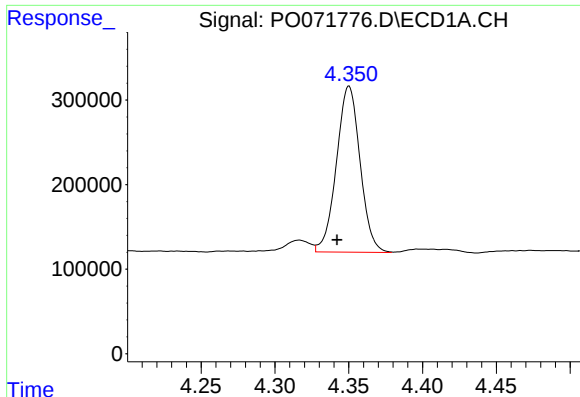


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: 0.008 min
Response: 2186120
Conc: 25.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-3-(0-6FT)


Manual Integrations
APPROVED

Ankita
10/1/2020 3:32:46 PM

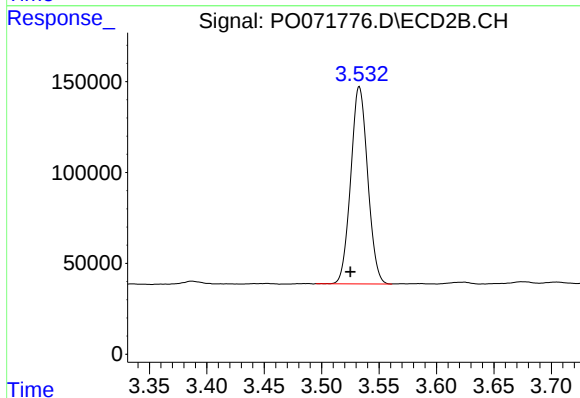


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: 0.008 min
Response: 1117827
Conc: 27.14 ng/ml

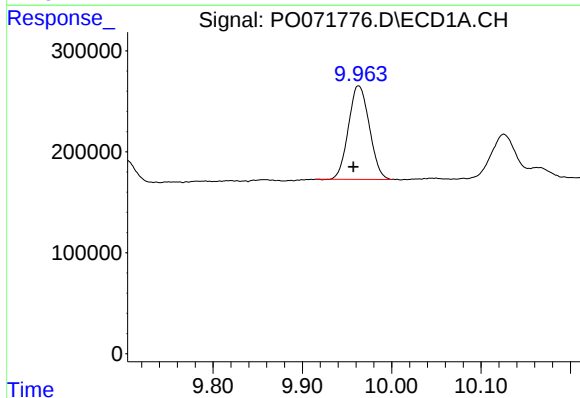

#2 Decachlorobiphenyl

R.T.: 9.963 min
Delta R.T.: 0.006 min
Response: 1503397
Conc: 13.09 ng/ml

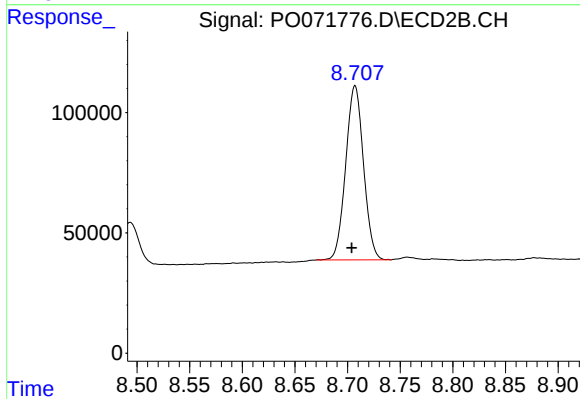

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.003 min
Response: 853158
Conc: 14.04 ng/ml