

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2020 23:17
 Operator : DD\AJ
 Sample : L4189-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-C-2334-C

Manual Integrations
 APPROVED

Ankita
 10/1/2020 3:33:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 01:51:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.530	1773847	933397	20.671	22.663
2) SA Decachlor...	9.959	8.704	2365656	1233660	20.591	20.295
Target Compounds						
31) L7 AR-1260-1	7.305	6.310	73401	53450	12.917	19.314m#
32) L7 AR-1260-2	7.573	6.512	101122	49831	11.648	14.098
33) L7 AR-1260-3	7.929	6.654	165497	51222	22.984	15.934 #
34) L7 AR-1260-4	8.155	7.132	140108	63959	21.147	22.168
35) L7 AR-1260-5	8.471	7.385	209476	134323	13.892	18.160 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093020\
Data File : PO071788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2020 23:17
Operator : DD\AJ
Sample : L4189-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 01:51:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

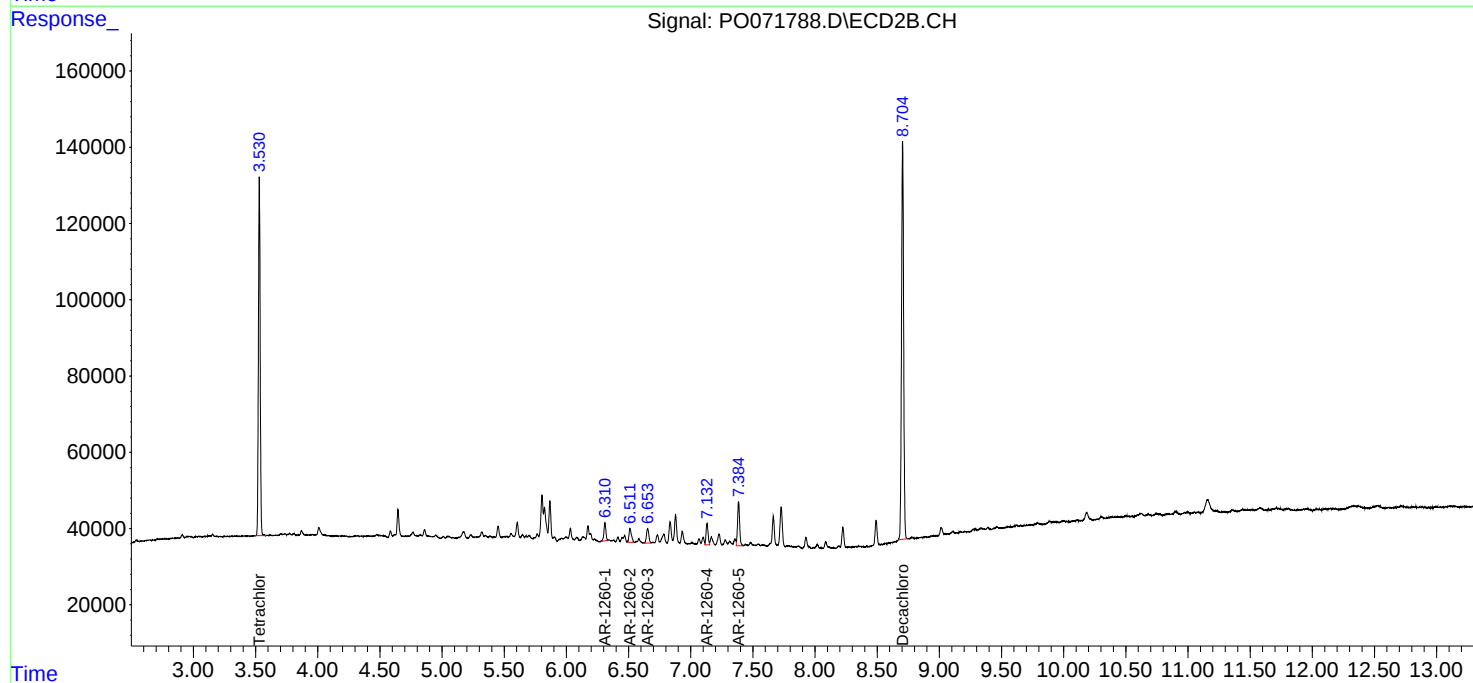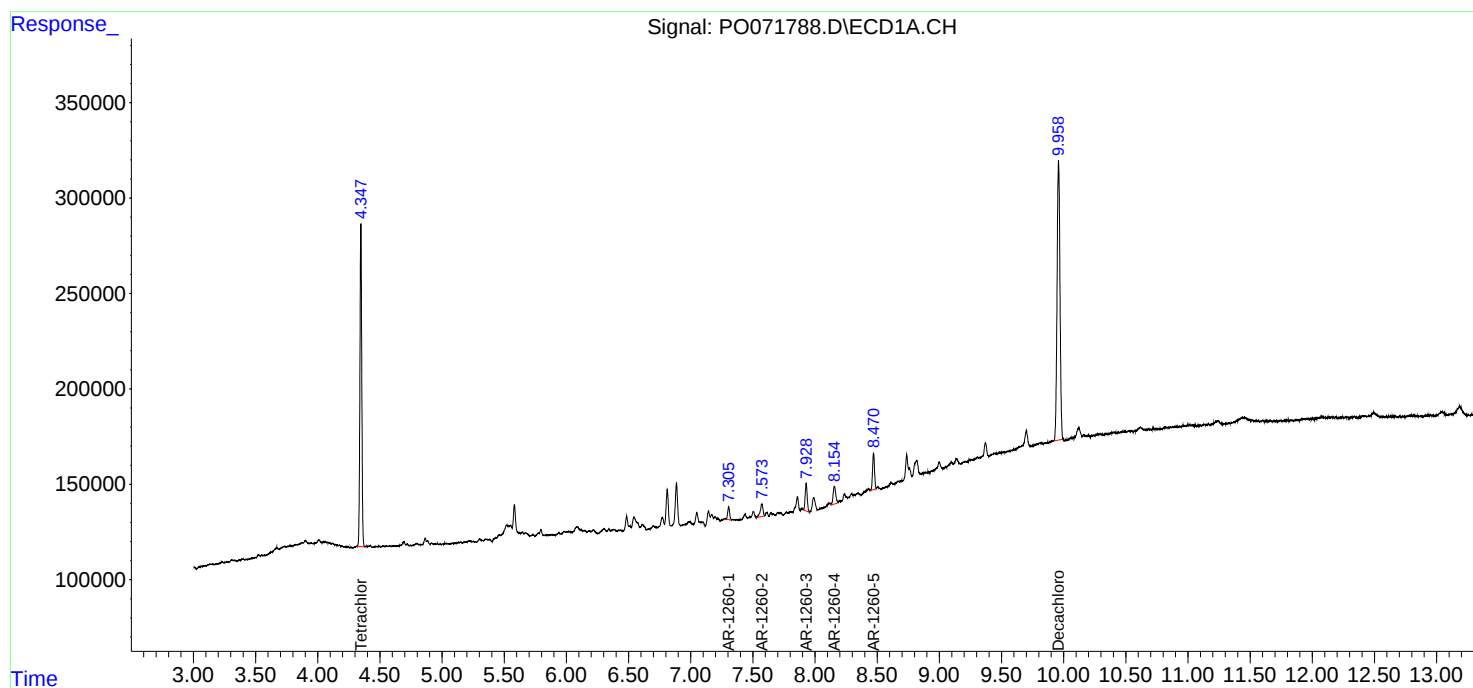

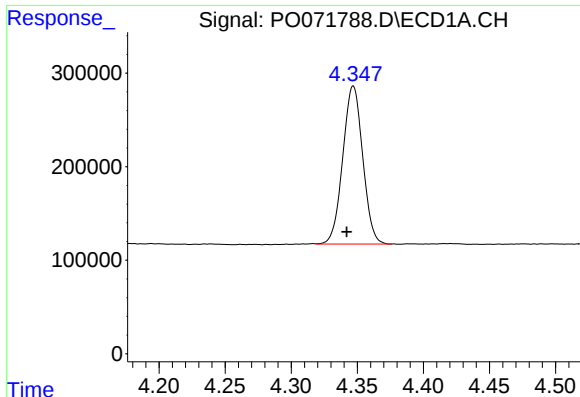


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: 0.005 min
Response: 1773847
Conc: 20.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:04 PM

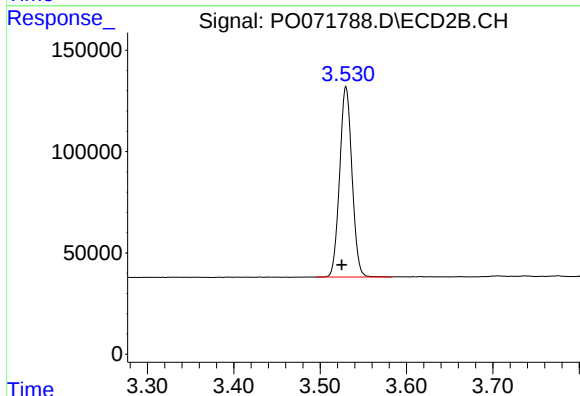


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.005 min
Response: 933397
Conc: 22.66 ng/ml

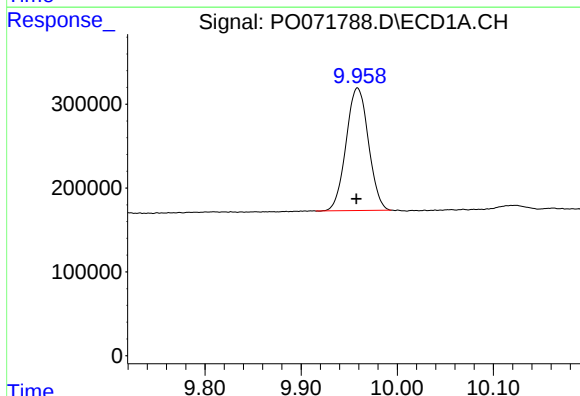


#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.001 min
Response: 2365656
Conc: 20.59 ng/ml

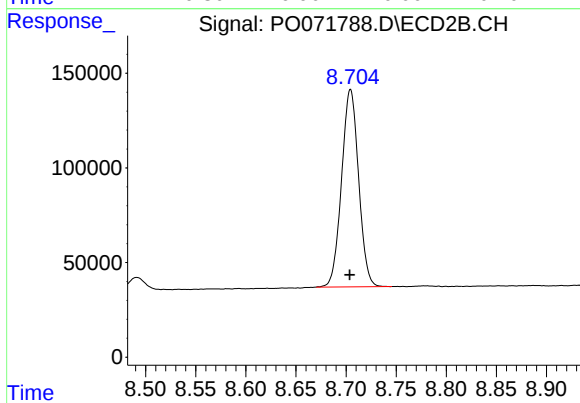

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 1233660
Conc: 20.30 ng/ml

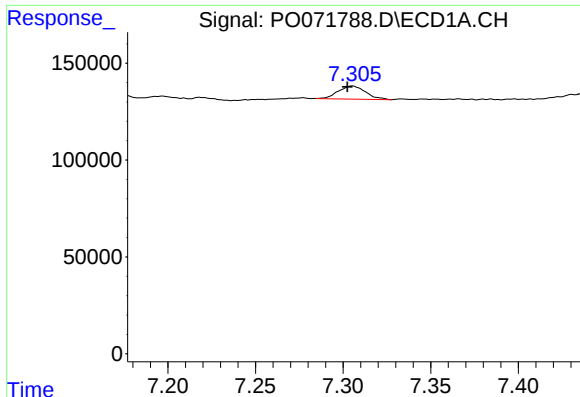


#31 AR-1260-1

R.T.: 7.305 min
Delta R.T.: 0.003 min
Response: 73401
Conc: 12.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:04 PM

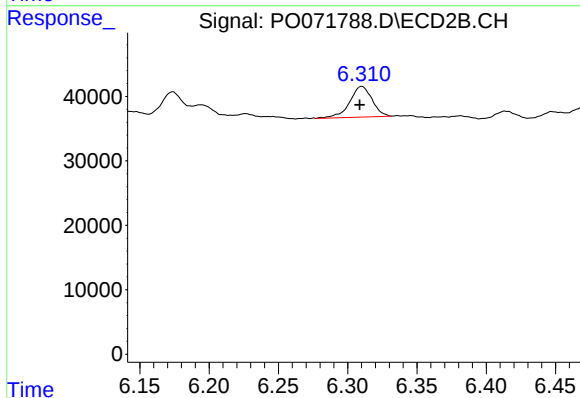


#31 AR-1260-1

R.T.: 6.310 min
Delta R.T.: 0.001 min
Response: 53450
Conc: 19.31 ng/ml m

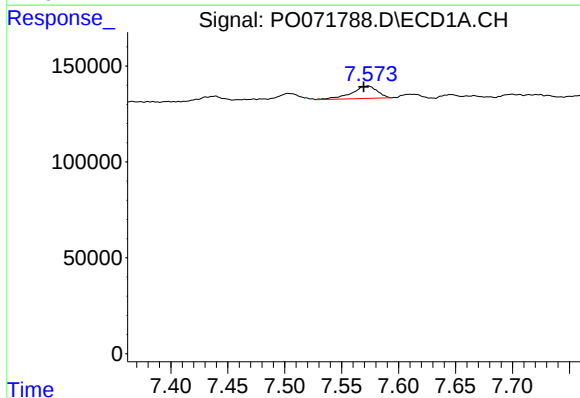


#32 AR-1260-2

R.T.: 7.573 min
Delta R.T.: 0.004 min
Response: 101122
Conc: 11.65 ng/ml

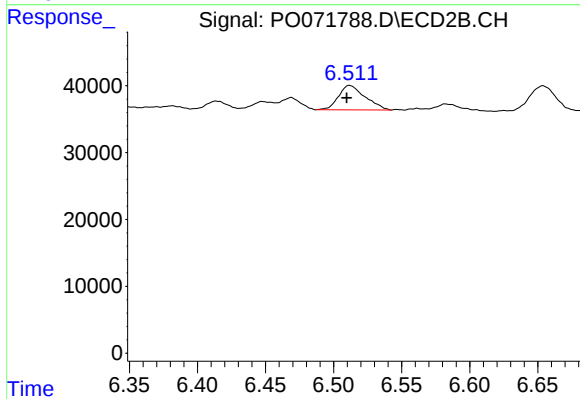

#32 AR-1260-2

R.T.: 6.512 min
Delta R.T.: 0.002 min
Response: 49831
Conc: 14.10 ng/ml

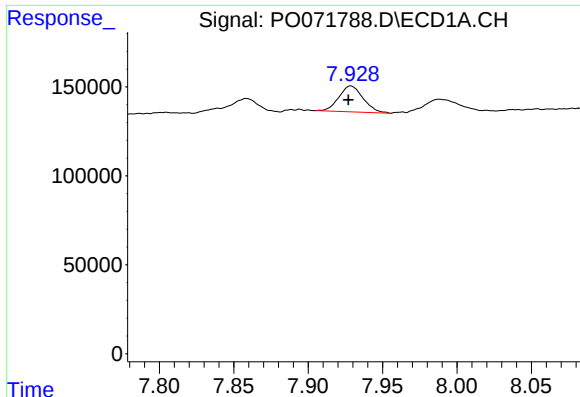


#33 AR-1260-3

R.T.: 7.929 min
Delta R.T.: 0.002 min
Response: 165497
Conc: 22.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-C-2334-C


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:04 PM

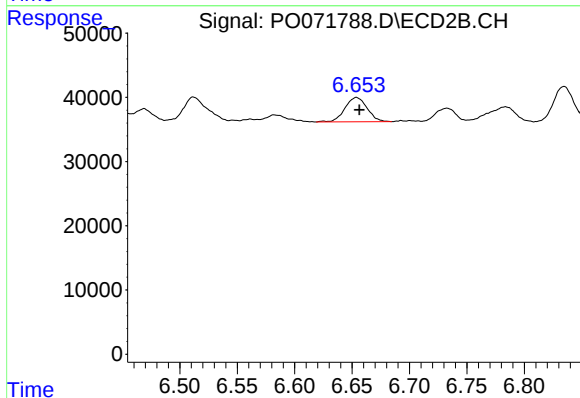


#33 AR-1260-3

R.T.: 6.654 min
Delta R.T.: -0.002 min
Response: 51222
Conc: 15.93 ng/ml

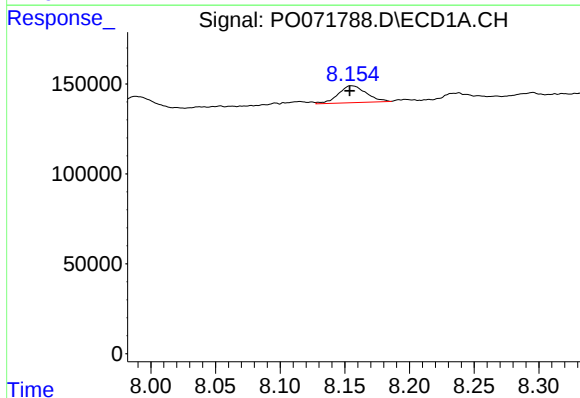


#34 AR-1260-4

R.T.: 8.155 min
Delta R.T.: 0.000 min
Response: 140108
Conc: 21.15 ng/ml

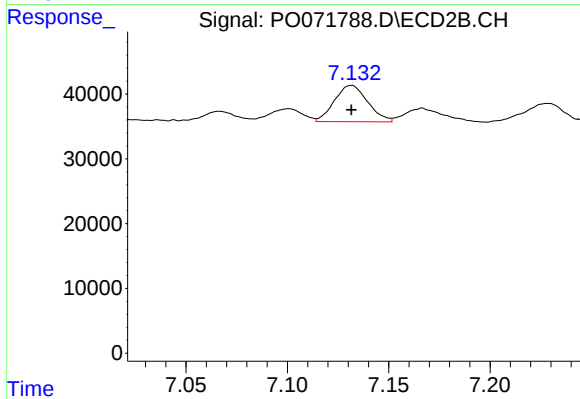

#34 AR-1260-4

R.T.: 7.132 min
Delta R.T.: 0.000 min
Response: 63959
Conc: 22.17 ng/ml

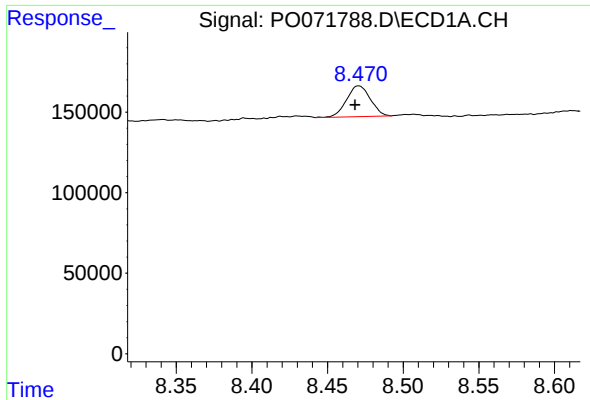


#35 AR-1260-5

R.T.: 8.471 min
Delta R.T.: 0.002 min
Response: 209476
Conc: 13.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-C-2334-C

Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:04 PM

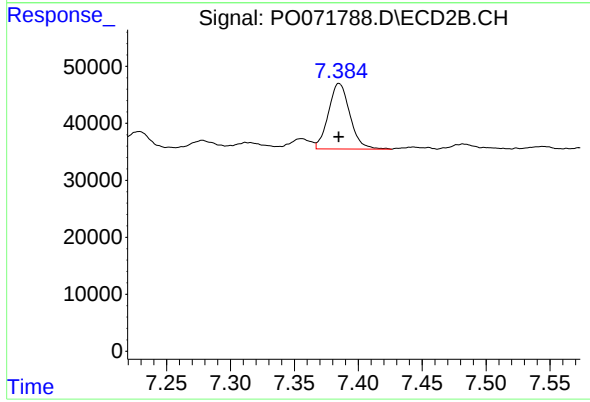

#35 AR-1260-5

R.T.: 7.385 min
Delta R.T.: 0.000 min
Response: 134323
Conc: 18.16 ng/ml