

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071806.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 5:00
 Operator : DD\AJ
 Sample : L4161-03 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH607V-END-1

Manual Integrations
 APPROVED

Ankita
 10/1/2020 3:33:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 05:21:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.532	292018	216936	3.403m	5.267 #
2) SA Decachlor...	9.959	8.704	456114	240823	3.970	3.962

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
Data File : P0071806.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 5:00
Operator : DD\AJ
Sample : L4161-03 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH607V-END-1


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 05:21:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

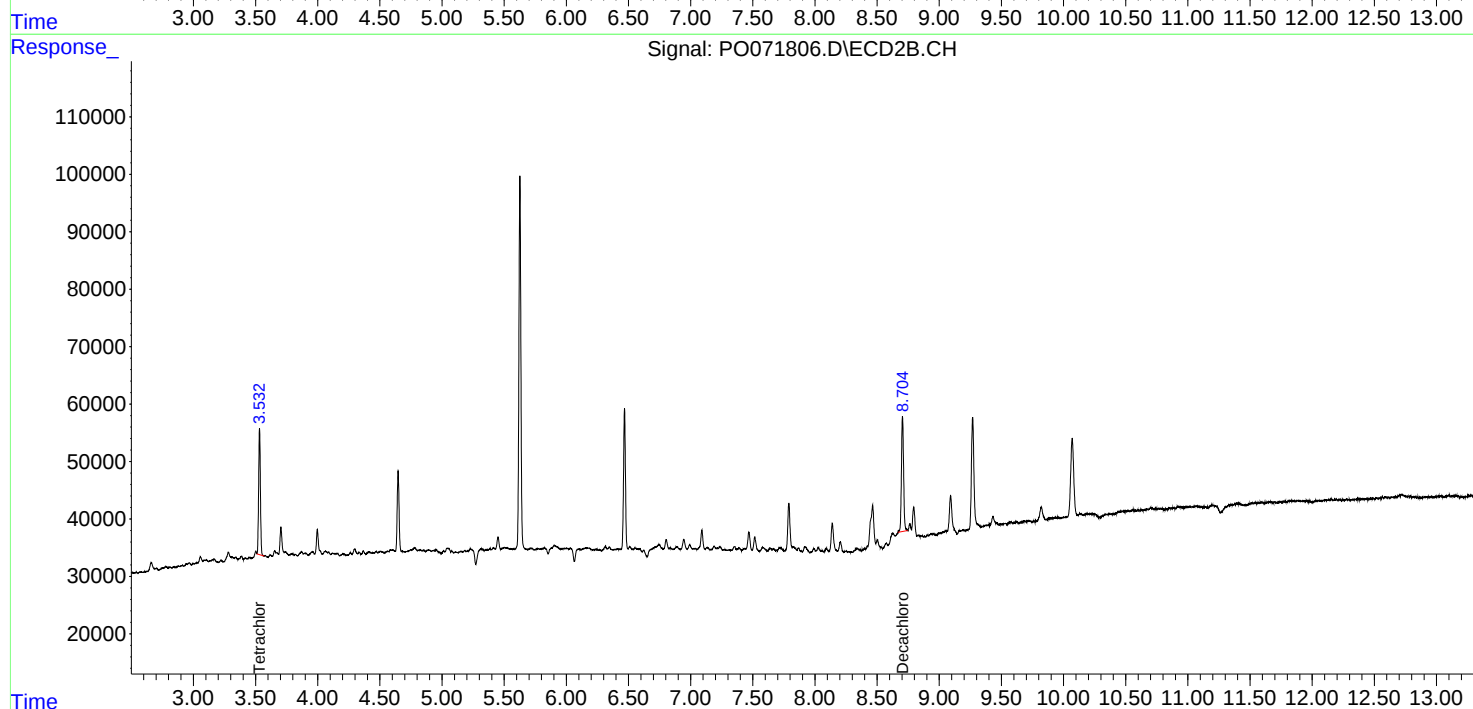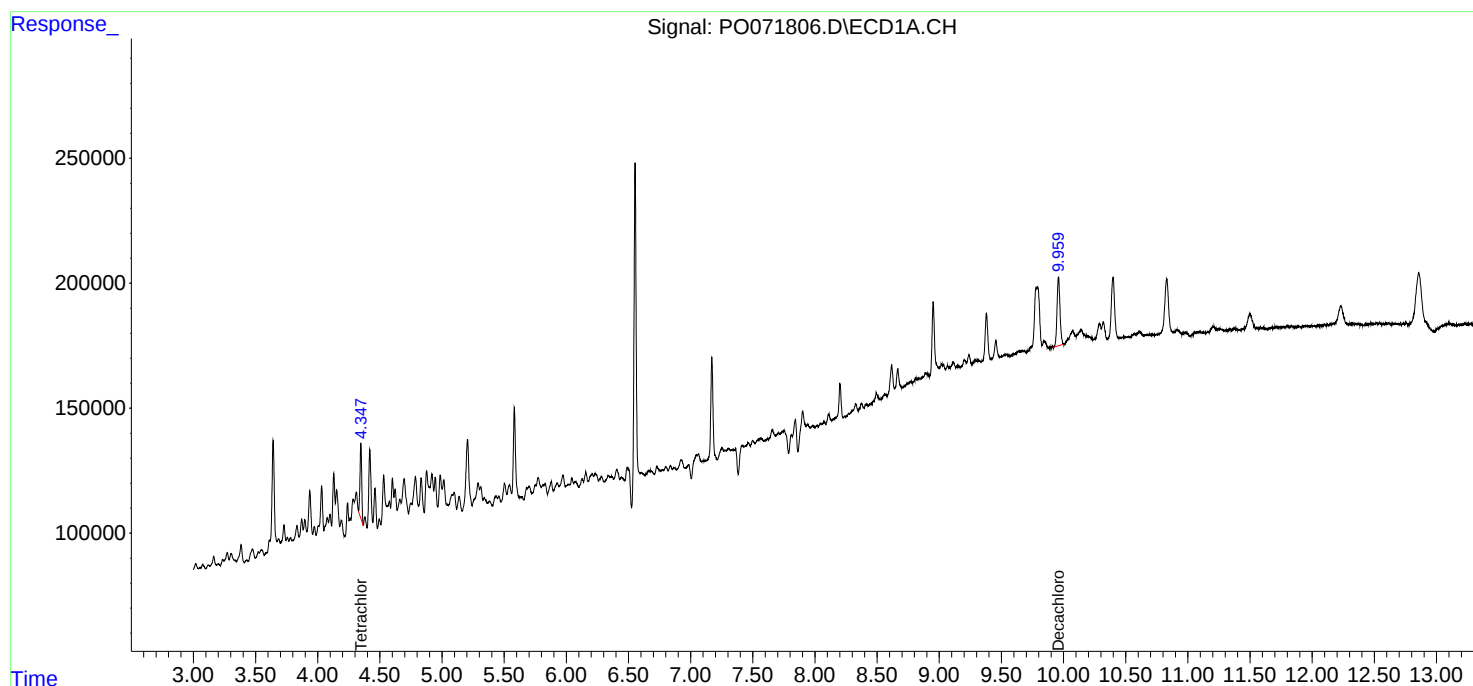

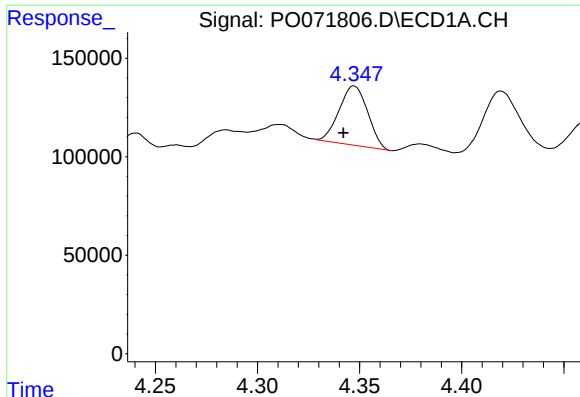


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: 0.005 min
Response: 292018
Conc: 3.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
JEH607V-END-1


Manual Integrations
APPROVED

Ankita
10/1/2020 3:33:43 PM

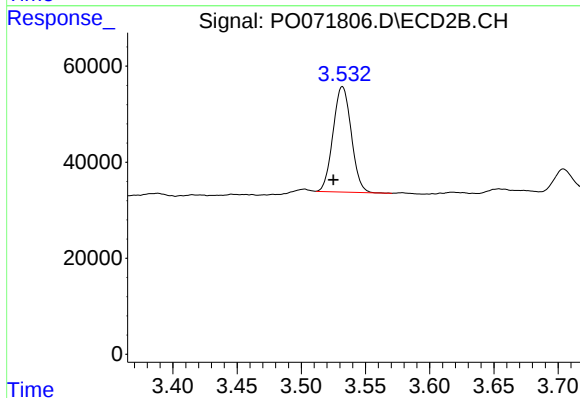


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.007 min
Response: 216936
Conc: 5.27 ng/ml

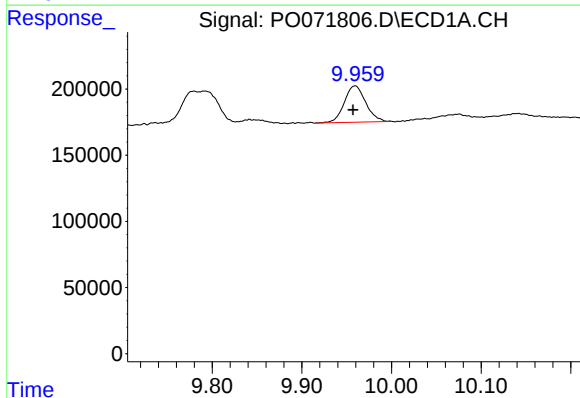

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: 0.002 min
Response: 456114
Conc: 3.97 ng/ml

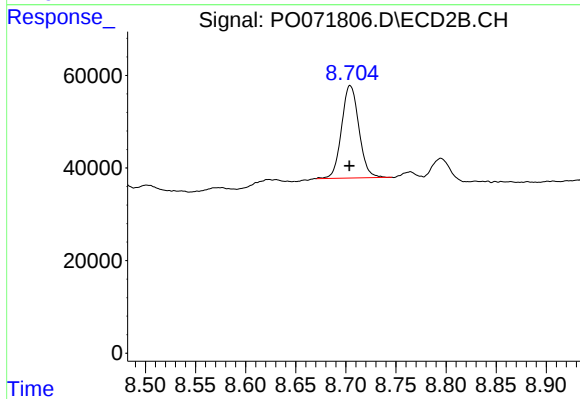

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.000 min
Response: 240823
Conc: 3.96 ng/ml