

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071808.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 5:35
 Operator : DD\AJ
 Sample : L4161-06 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA696E-END-2-1-2

Manual Integrations
 APPROVED

Ankita
 10/1/2020 5:22:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 06:52:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.531	209250	135895	2.438	3.300m#
2) SA Decachlor...	9.963	8.709	217877	111074	1.896	1.827m
Target Compounds						
26) L6 AR-1254-1	6.551	5.606	775806	133767	211.855m	56.483 #
27) L6 AR-1254-2	6.768	5.766	328201	137340	54.434	65.571
28) L6 AR-1254-3	7.143	6.174	279085	204745	44.080	60.507m#
29) L6 AR-1254-4	7.437	6.416	281827	121314	45.745m	50.955
30) L6 AR-1254-5	7.856	6.836	240022	157449	40.385m	48.678

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093020\
Data File : PO071808.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 5:35
Operator : DD\AJ
Sample : L4161-06 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA696E-END-2-1-2


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 06:52:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

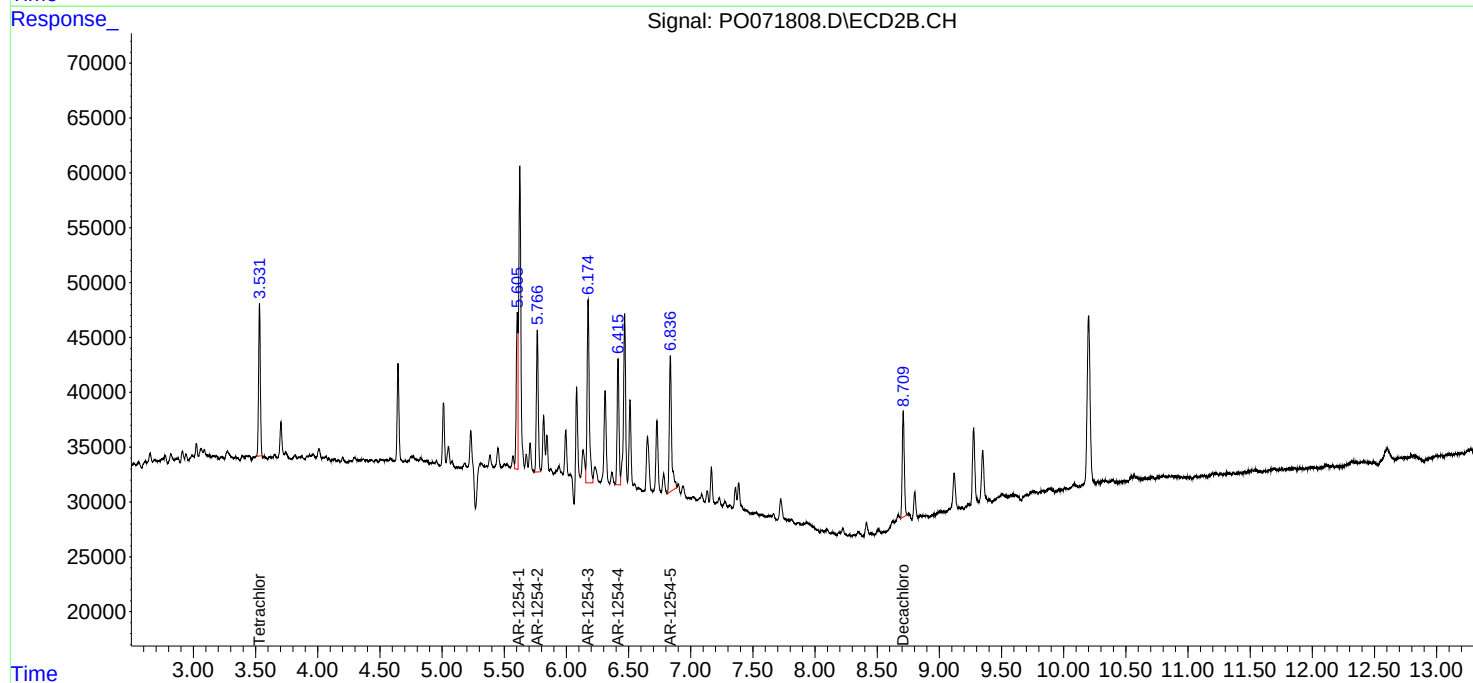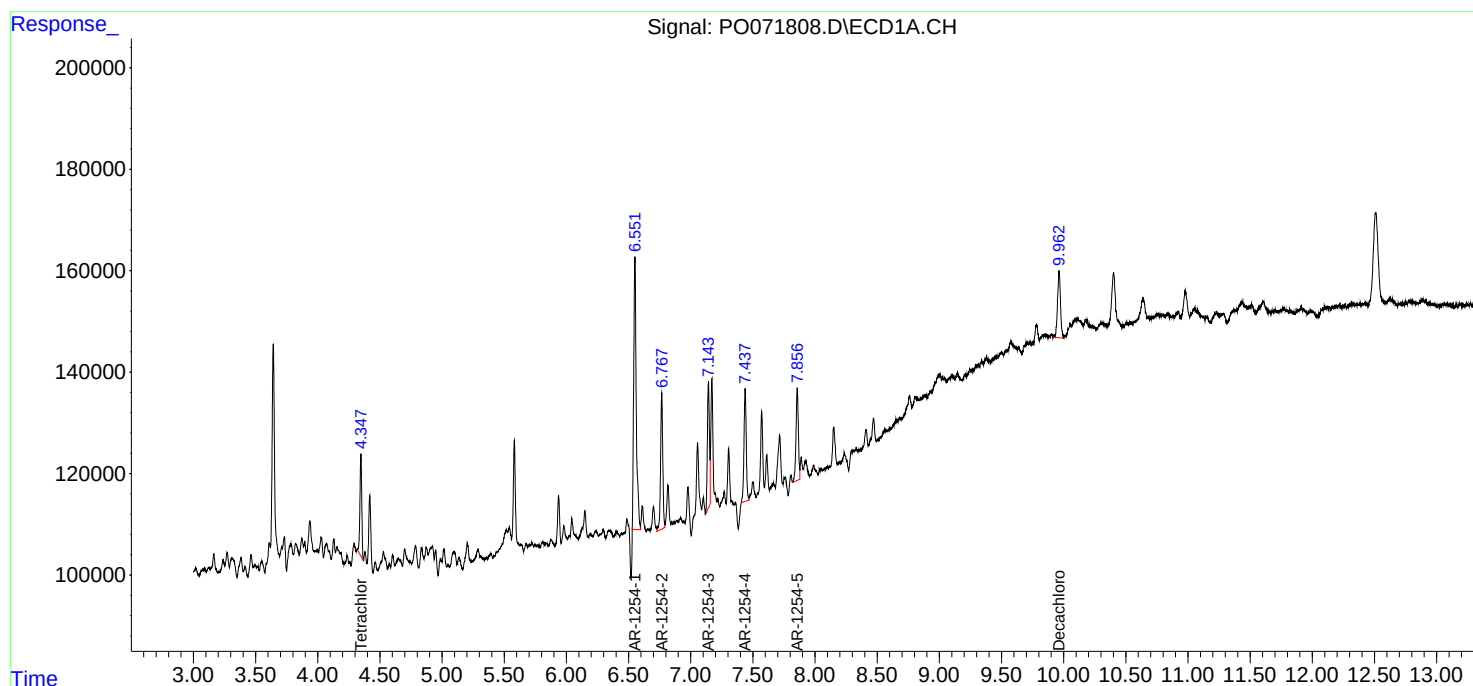

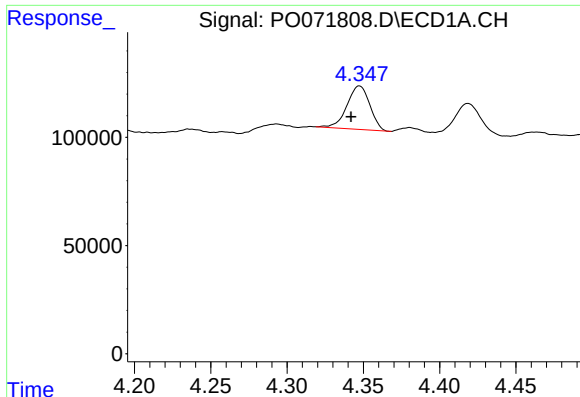


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: 0.005 min
Response: 209250
Conc: 2.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA696E-END-2-1-2


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:46 PM

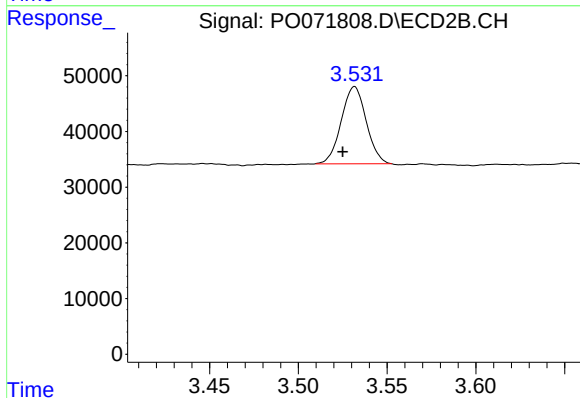


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.006 min
Response: 135895
Conc: 3.30 ng/ml m

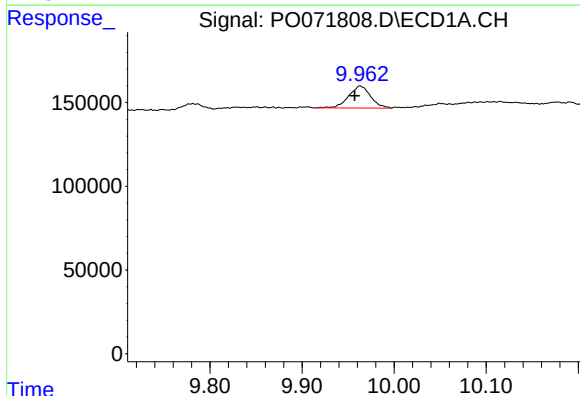


#2 Decachlorobiphenyl

R.T.: 9.963 min
Delta R.T.: 0.006 min
Response: 217877
Conc: 1.90 ng/ml

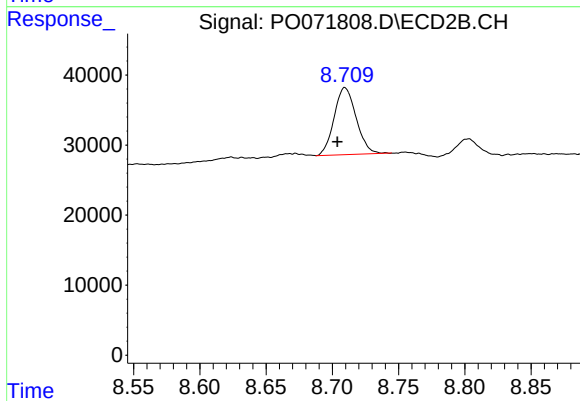

#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: 0.005 min
Response: 111074
Conc: 1.83 ng/ml m

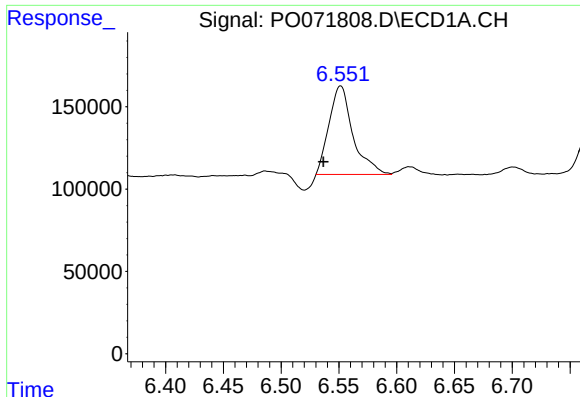


#26 AR-1254-1

R.T.: 6.551 min
Delta R.T.: 0.015 min
Response: 775806
Conc: 211.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KMA696E-END-2-1-2


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:46 PM

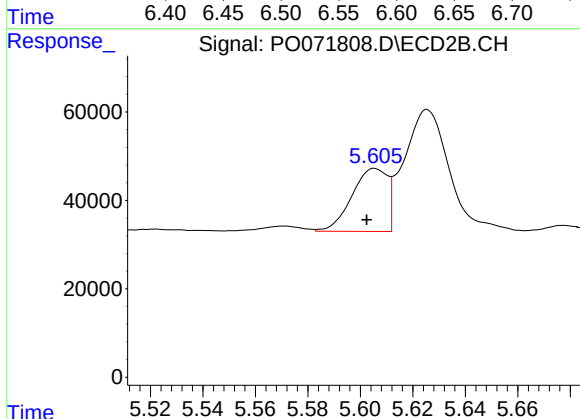


#26 AR-1254-1

R.T.: 5.606 min
Delta R.T.: 0.003 min
Response: 133767
Conc: 56.48 ng/ml

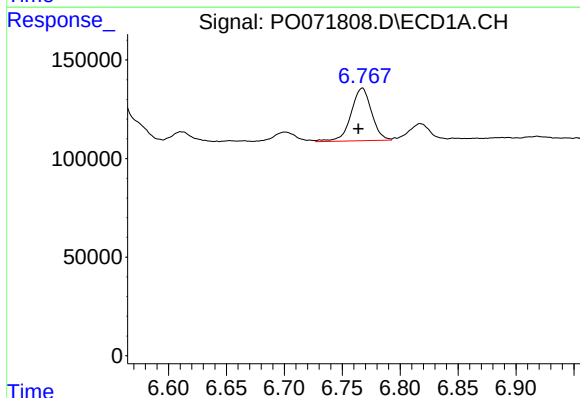


#27 AR-1254-2

R.T.: 6.768 min
Delta R.T.: 0.004 min
Response: 328201
Conc: 54.43 ng/ml

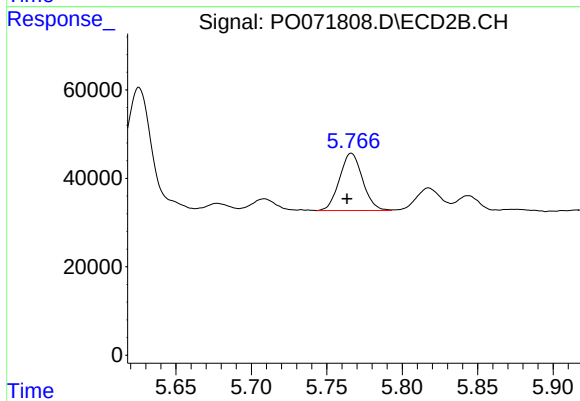

#27 AR-1254-2

R.T.: 5.766 min
Delta R.T.: 0.003 min
Response: 137340
Conc: 65.57 ng/ml

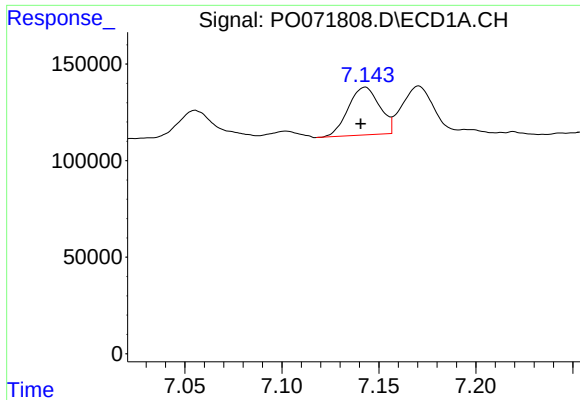


#28 AR-1254-3

R.T.: 7.143 min
Delta R.T.: 0.002 min
Response: 279085
Conc: 44.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA696E-END-2-1-2


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:46 PM

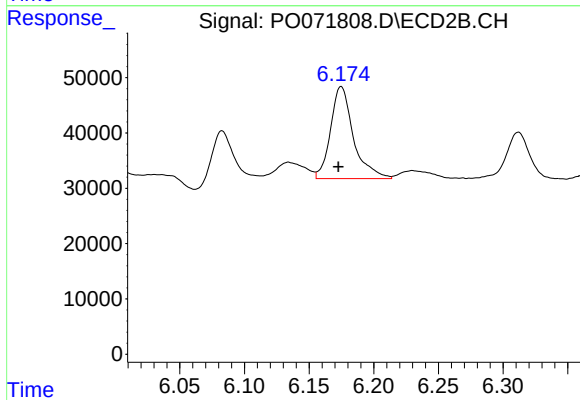


#28 AR-1254-3

R.T.: 6.174 min
Delta R.T.: 0.002 min
Response: 204745
Conc: 60.51 ng/ml m

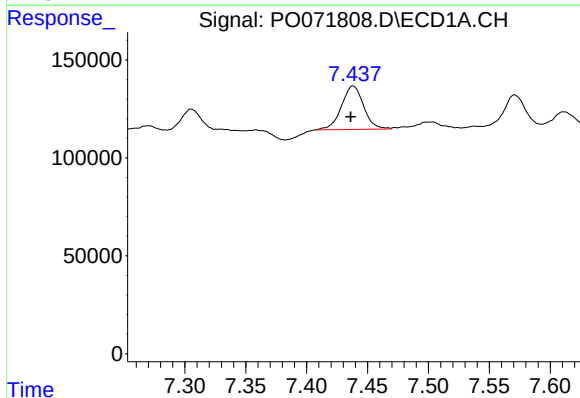


#29 AR-1254-4

R.T.: 7.437 min
Delta R.T.: 0.001 min
Response: 281827
Conc: 45.74 ng/ml m

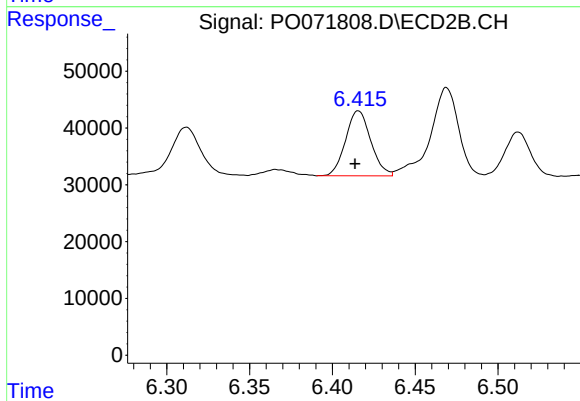

#29 AR-1254-4

R.T.: 6.416 min
Delta R.T.: 0.002 min
Response: 121314
Conc: 50.96 ng/ml

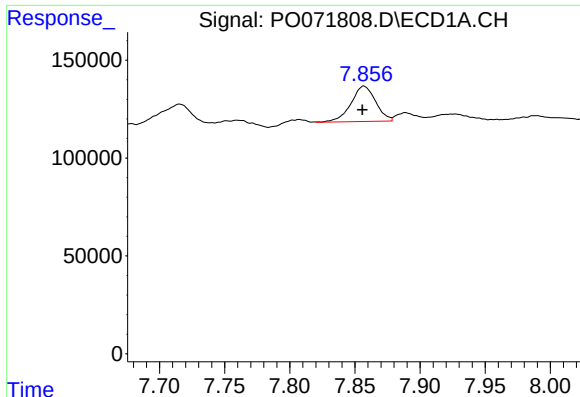


#30 AR-1254-5

R.T.: 7.856 min
Delta R.T.: 0.000 min
Response: 240022
Conc: 40.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KMA696E-END-2-1-2

Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:46 PM

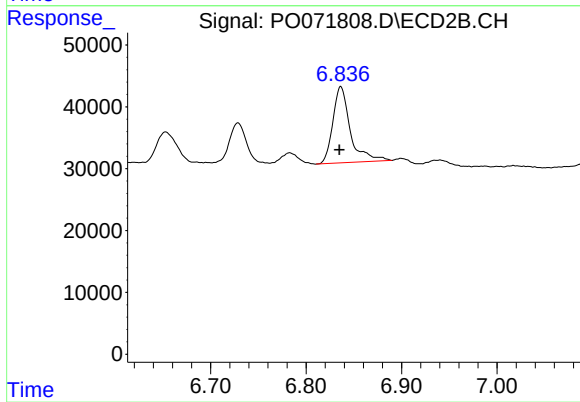

#30 AR-1254-5

R.T.: 6.836 min
Delta R.T.: 0.001 min
Response: 157449
Conc: 48.68 ng/ml