

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 6:44
 Operator : DD\AJ
 Sample : L4161-09 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH735C-END-1

Manual Integrations
 APPROVED

Ankita
 10/1/2020 5:22:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 08:25:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.531	194089	135620	2.262	3.293m#
2) SA Decachlor...	9.960	8.706	171268	99120	1.491	1.631

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
Data File : P0071812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 6:44
Operator : DD\AJ
Sample : L4161-09 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
JEH735C-END-1


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 08:25:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

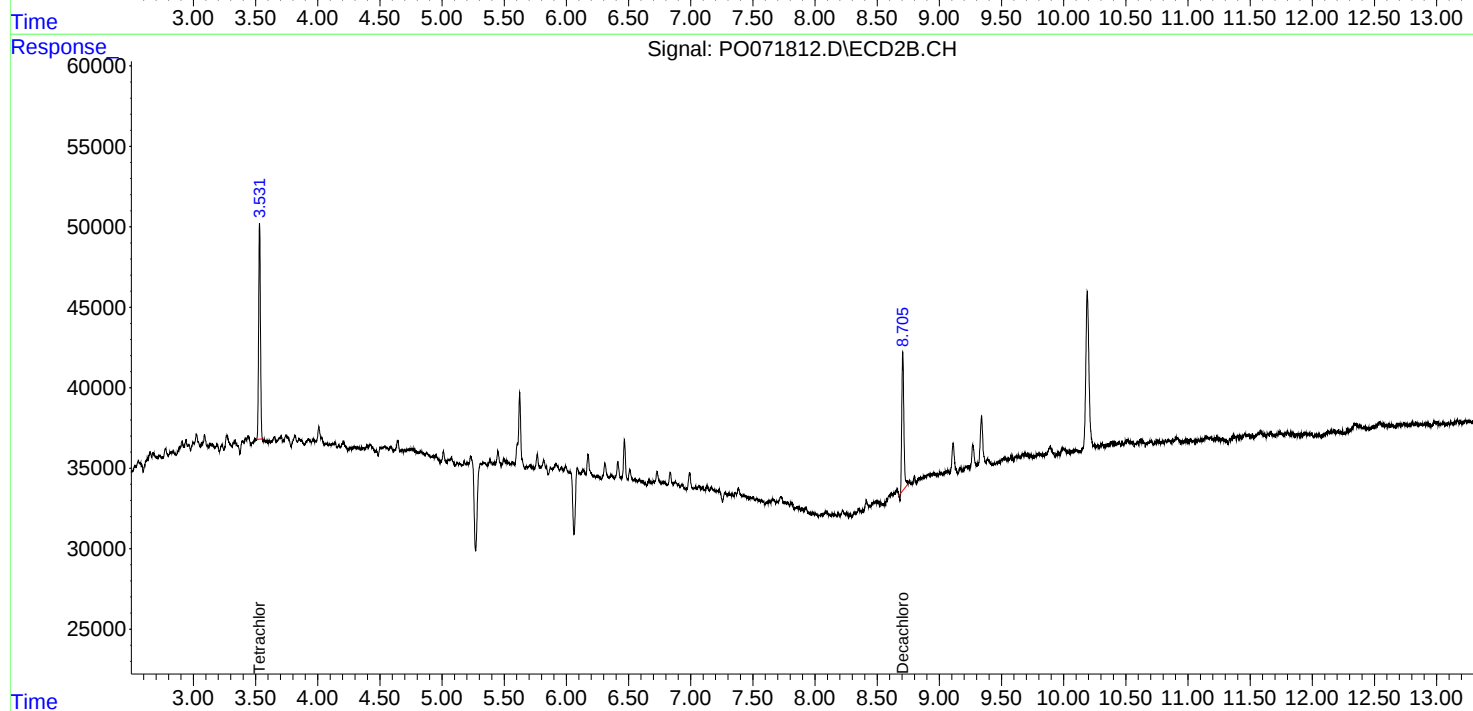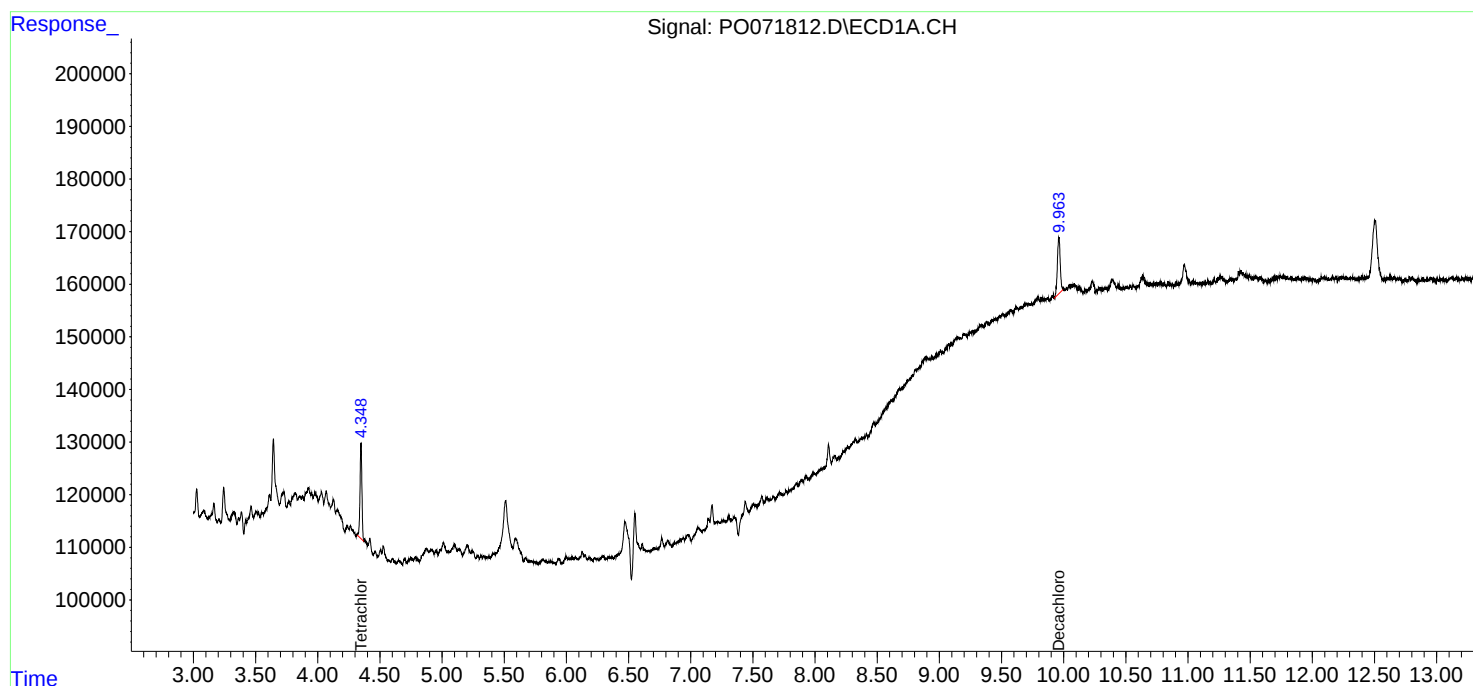

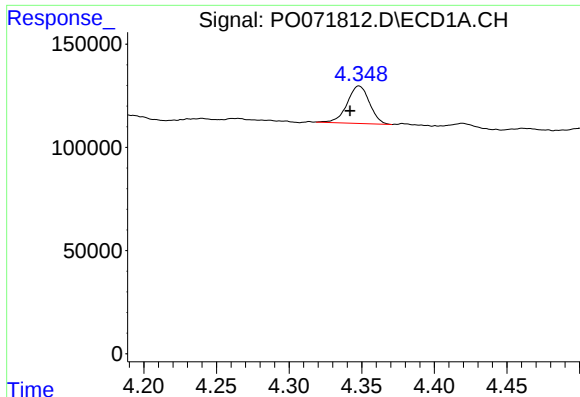


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.006 min
Response: 194089
Conc: 2.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEH735C-END-1


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:47 PM

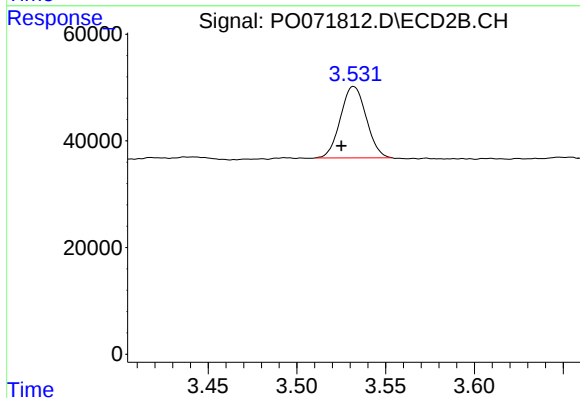


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.006 min
Response: 135620
Conc: 3.29 ng/ml m

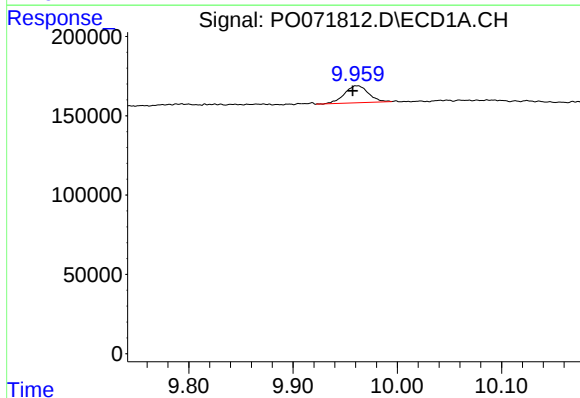

#2 Decachlorobiphenyl

R.T.: 9.960 min
Delta R.T.: 0.003 min
Response: 171268
Conc: 1.49 ng/ml

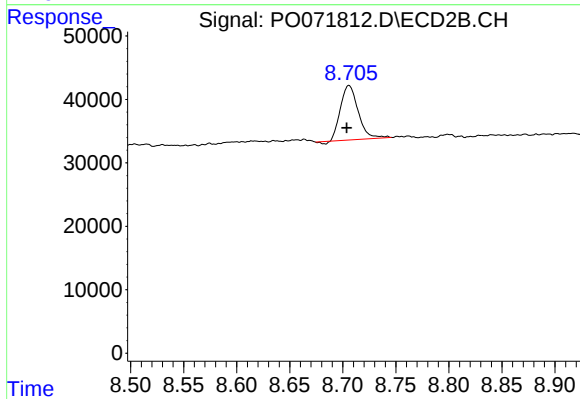

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: 0.002 min
Response: 99120
Conc: 1.63 ng/ml