

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071815.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 7:35
 Operator : DD\AJ
 Sample : L4183-01 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 32676

Manual Integrations
 APPROVED

Ankita
 10/1/2020 5:22:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 08:26:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.531	412533	186030	4.807	4.517
2) SA Decachlor...	9.961	8.707	162830	146185	1.417m	2.405m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093020\
Data File : PO071815.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 7:35
Operator : DD\AJ
Sample : L4183-01 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
32676


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 08:26:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

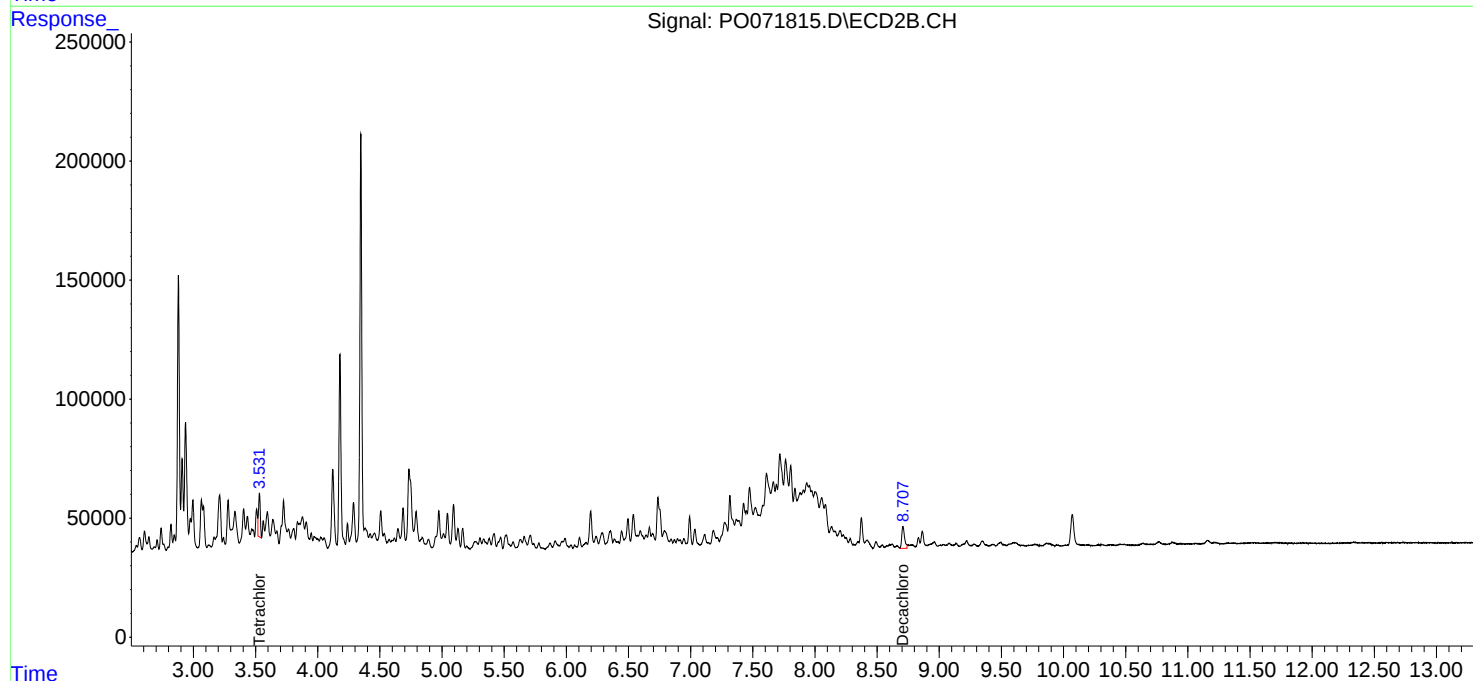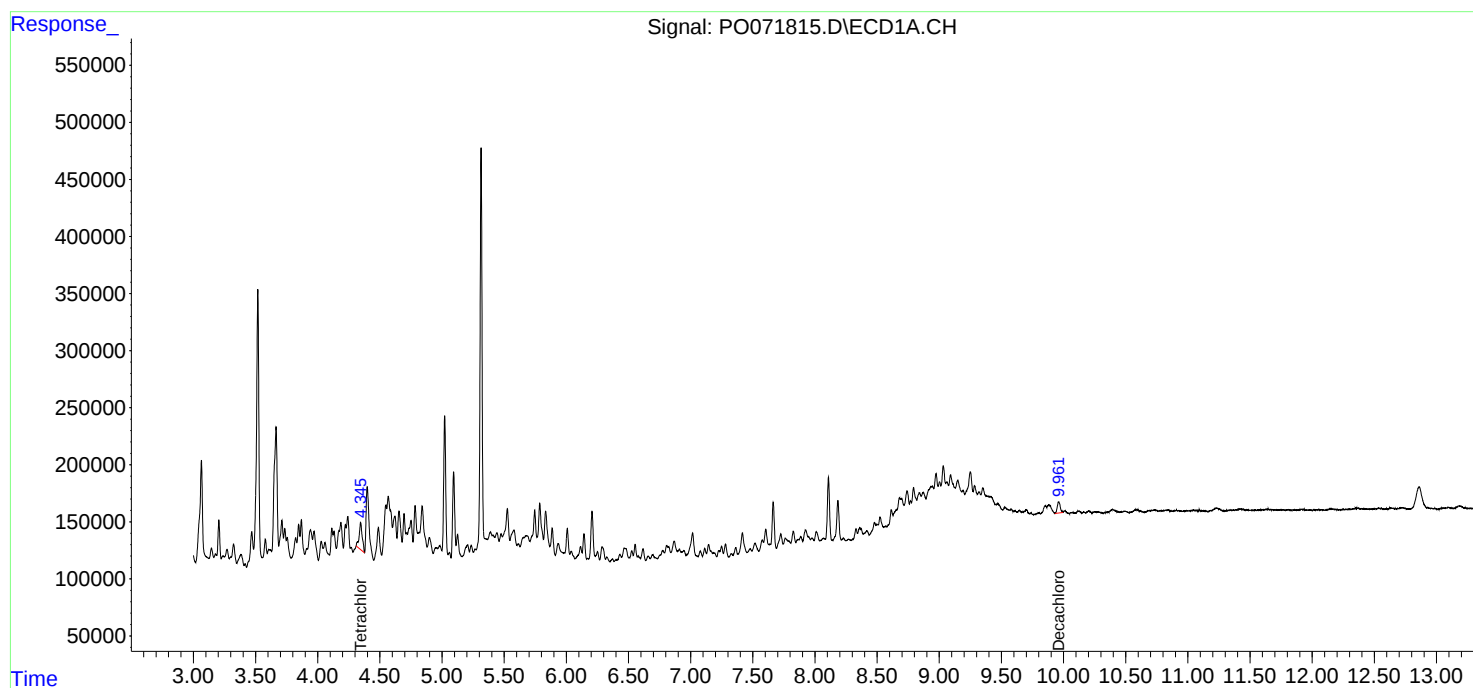

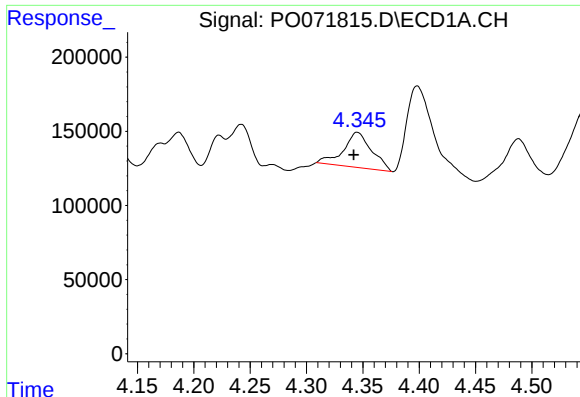


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: 0.003 min
Response: 412533
Conc: 4.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
32676


Manual Integrations
APPROVED

Ankita
10/1/2020 5:22:49 PM

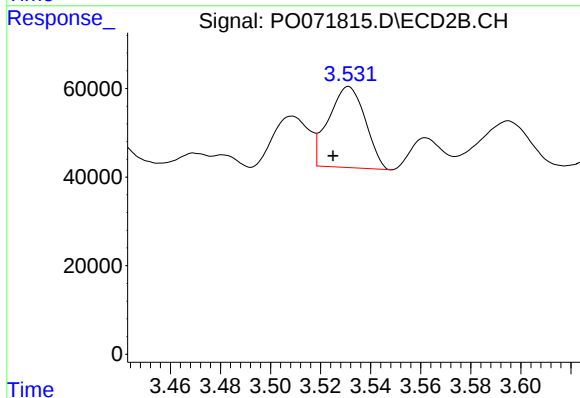


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.006 min
Response: 186030
Conc: 4.52 ng/ml

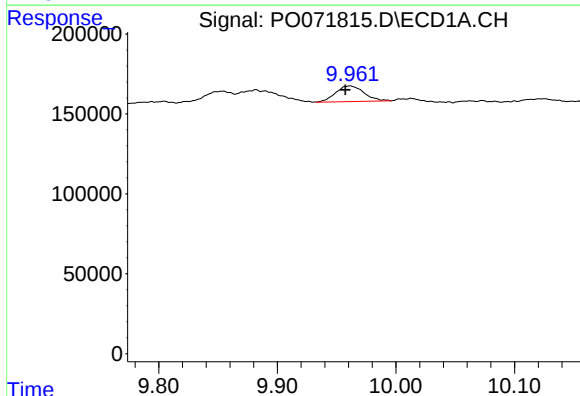

#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: 0.004 min
Response: 162830
Conc: 1.42 ng/ml m

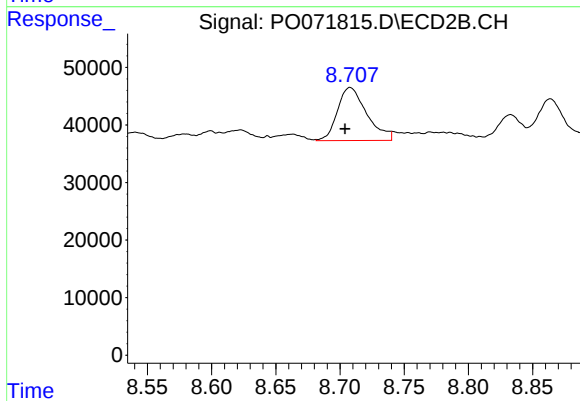

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.004 min
Response: 146185
Conc: 2.40 ng/ml m