

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093020\
 Data File : P0071822.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 9:35
 Operator : DD\AJ
 Sample : L4189-03 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-C-2334-GW

Manual Integrations
 APPROVED

Ankita
 10/2/2020 5:00:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 10:28:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359f	3.535	718989	116457	8.379m	2.828m#
2) SA Decachlor...	9.966	8.709	187070	113785	1.628m	1.872

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093020\
Data File : PO071822.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 9:35
Operator : DD\AJ
Sample : L4189-03 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-C-2334-GW


Manual Integrations
APPROVED

Ankita
10/2/2020 5:00:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 10:28:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

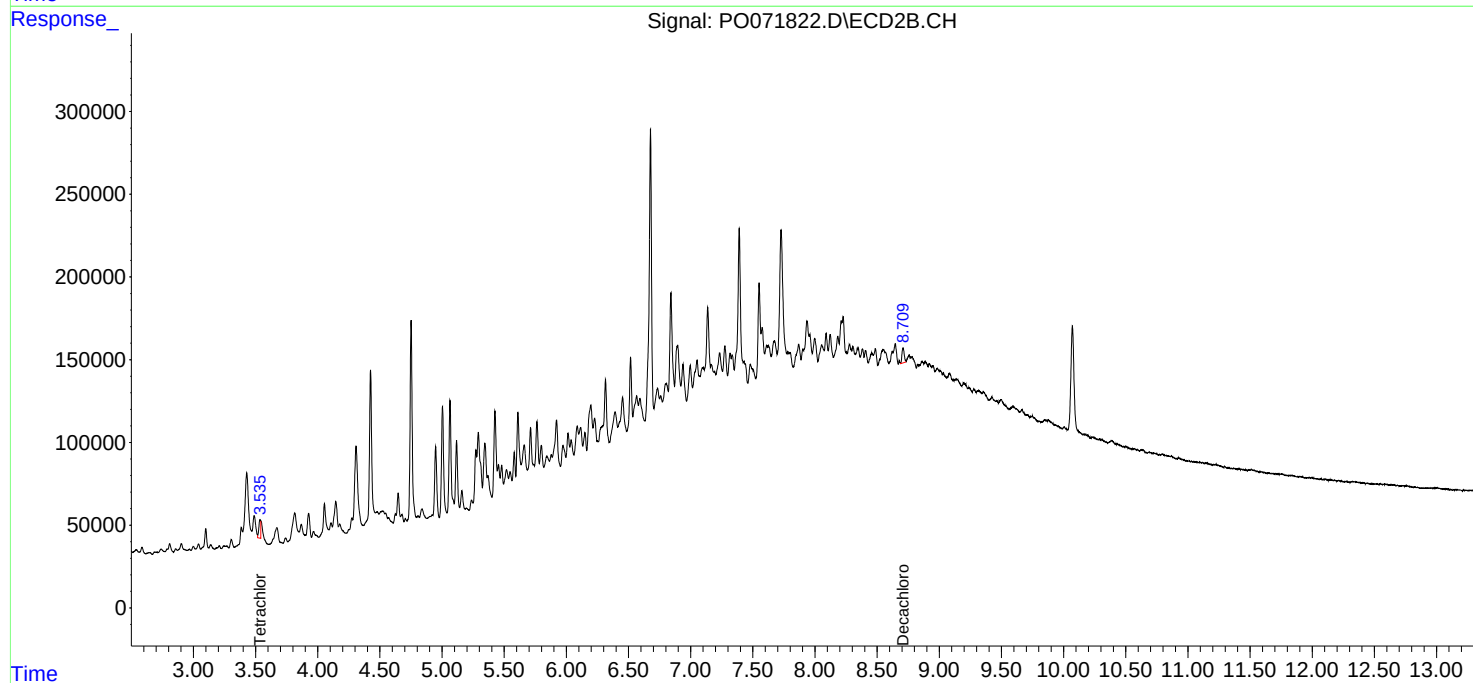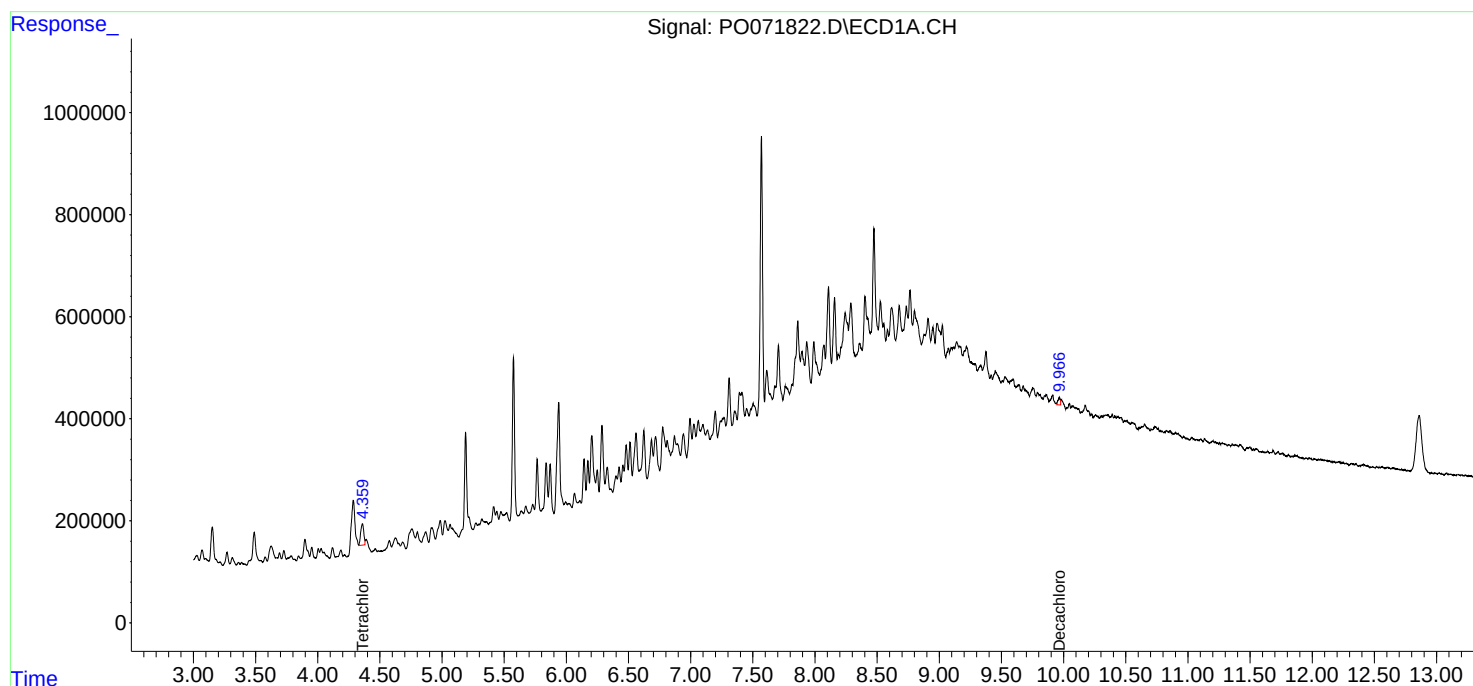

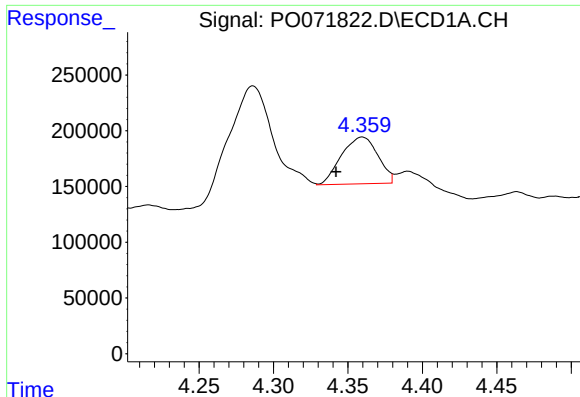


#1 Tetrachloro-m-xylene

R.T.: 4.359 min
Delta R.T.: 0.017 min
Response: 718989
Conc: 8.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-C-2334-GW


Manual Integrations
APPROVED

Ankita
10/2/2020 5:00:14 PM

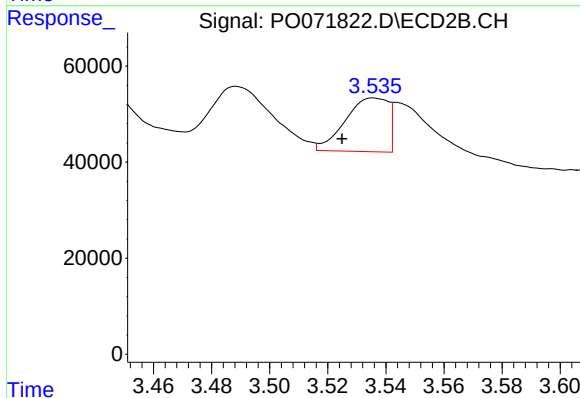


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.010 min
Response: 116457
Conc: 2.83 ng/ml m

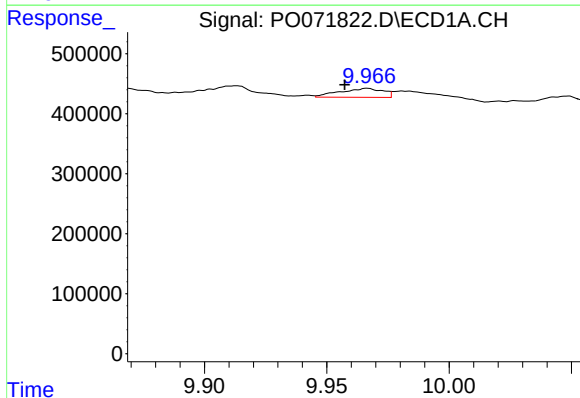

#2 Decachlorobiphenyl

R.T.: 9.966 min
Delta R.T.: 0.009 min
Response: 187070
Conc: 1.63 ng/ml m

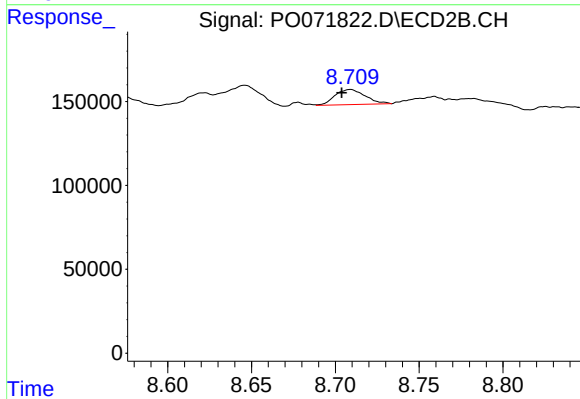

#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: 0.005 min
Response: 113785
Conc: 1.87 ng/ml