

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093021\
 Data File : P0081691.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 23:58
 Operator : AJ\MA
 Sample : M3969-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 02:56:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.867	3.983	2230855	637235	25.016	23.918
2)	SA Decachlor...	10.874	9.327	1827435	561183	24.533	24.165
Target Compounds							
8)	L2 AR-1221-1	5.117	0.000	39570	0	36.160	N.D. #
9)	L2 AR-1221-2	5.222	0.000	20283	0	25.725	N.D. #
20)	L4 AR-1242-5	7.174	0.000	176036	0	89.266	N.D. #
25)	L5 AR-1248-5	7.174	0.000	176036	0	52.069	N.D. #
35)	L7 AR-1260-5	9.089	0.000	50955	0	6.878	N.D. #
37)	L8 AR-1262-2	9.089	0.000	50955	0	5.713	N.D. #
38)	L8 AR-1262-3	9.381	0.000	30005	0	7.479	N.D. #
41)	L9 AR-1268-1	9.381	0.000	30005	0	2.795	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093021\
Data File : PO081691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 23:58
Operator : AJ\MA
Sample : M3969-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 02:56:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

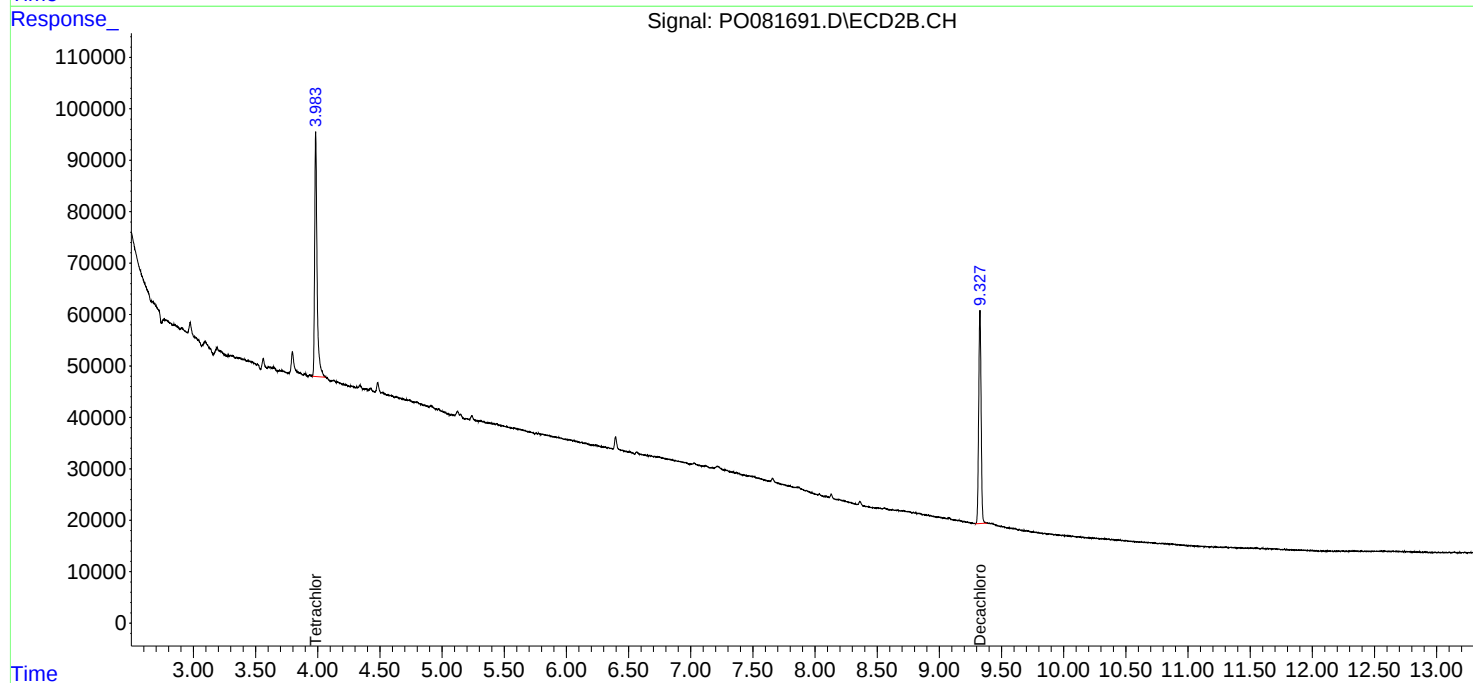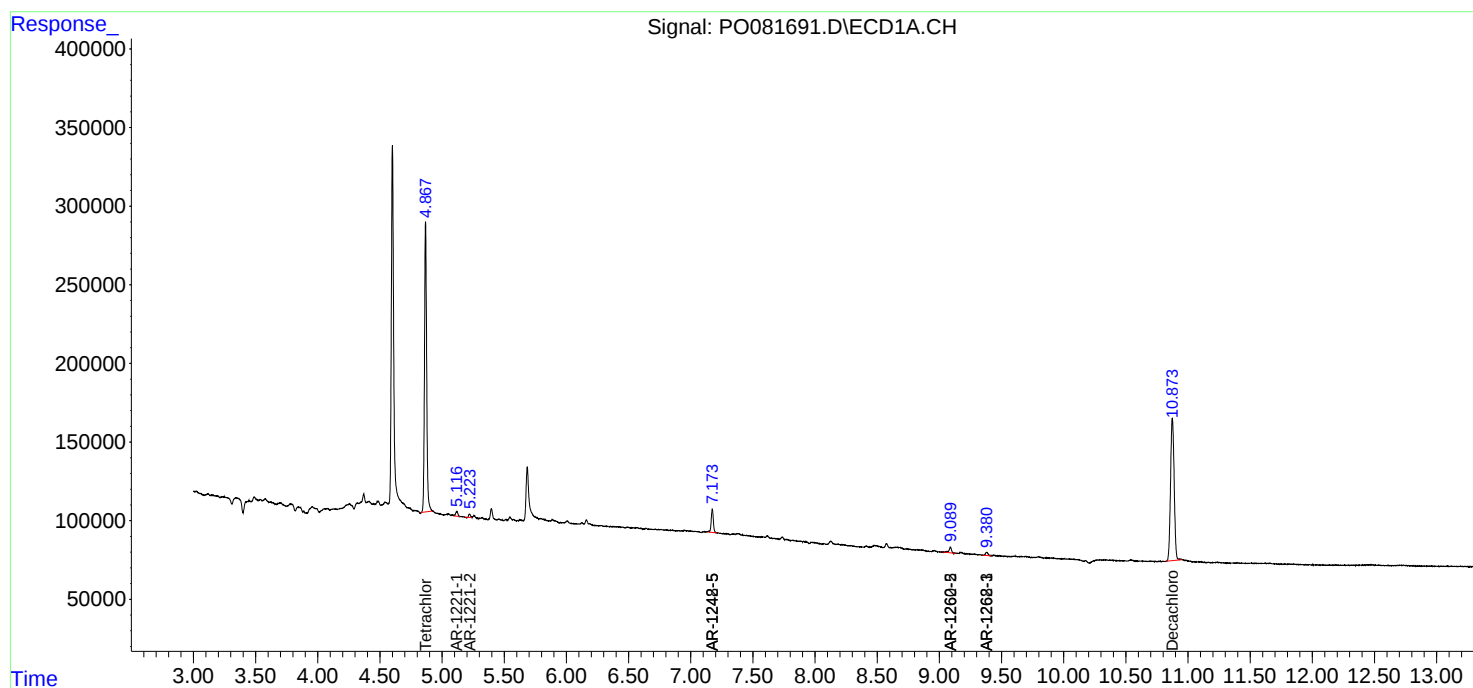


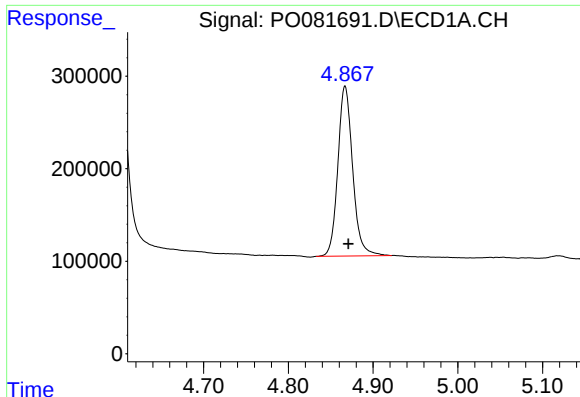

#1 Tetrachloro-m-xylene


R.T.: 4.867 min
Delta R.T.: -0.004 min
Response: 2230855
Conc: 25.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

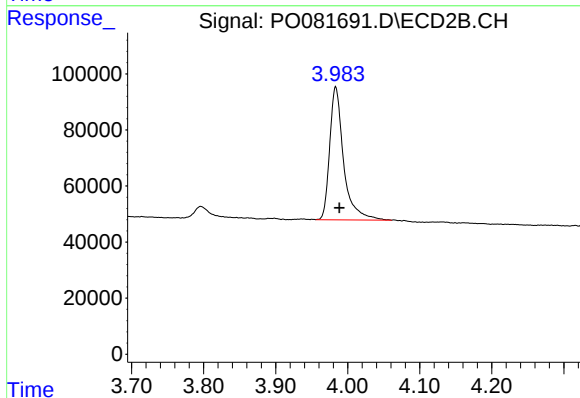


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.005 min
Response: 637235
Conc: 23.92 ng/ml

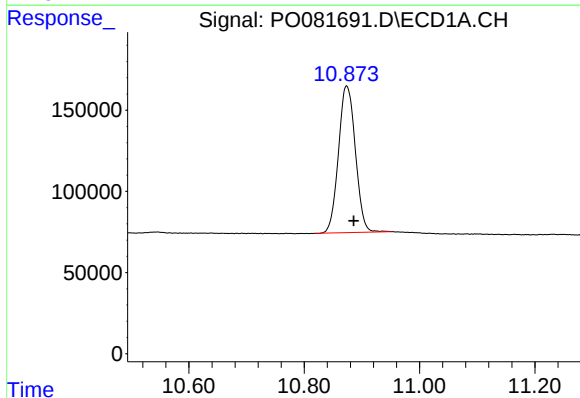


#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.012 min
Response: 1827435
Conc: 24.53 ng/ml

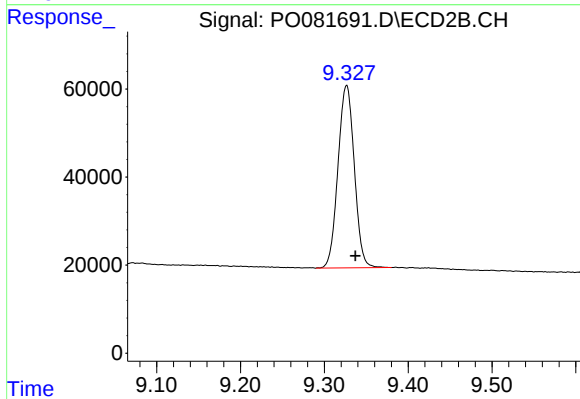

#2 Decachlorobiphenyl


R.T.: 9.327 min
Delta R.T.: -0.010 min
Response: 561183
Conc: 24.17 ng/ml

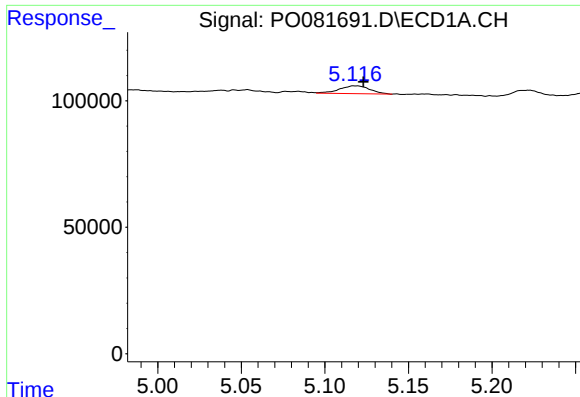

#8 AR-1221-1


R.T.: 5.117 min
Delta R.T.: -0.006 min
Response: 39570
Conc: 36.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

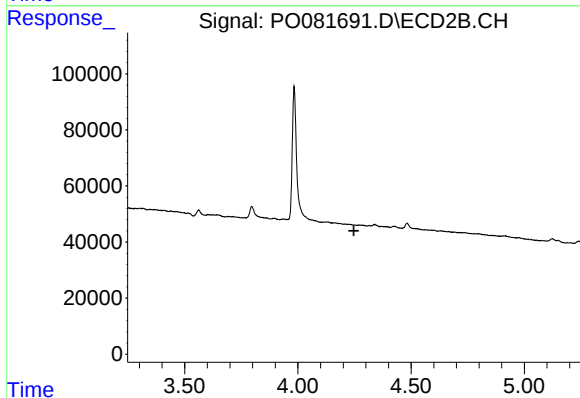


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.248 min
Response: 0
Conc: N.D.

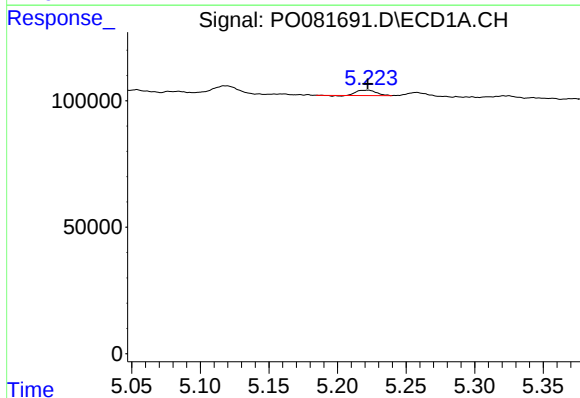


#9 AR-1221-2

R.T.: 5.222 min
Delta R.T.: 0.000 min
Response: 20283
Conc: 25.73 ng/ml

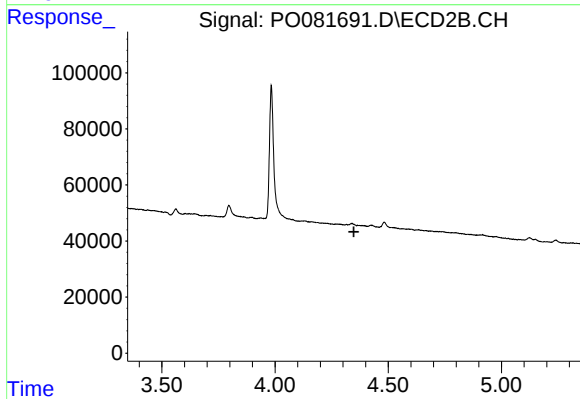

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.348 min
Response: 0
Conc: N.D.

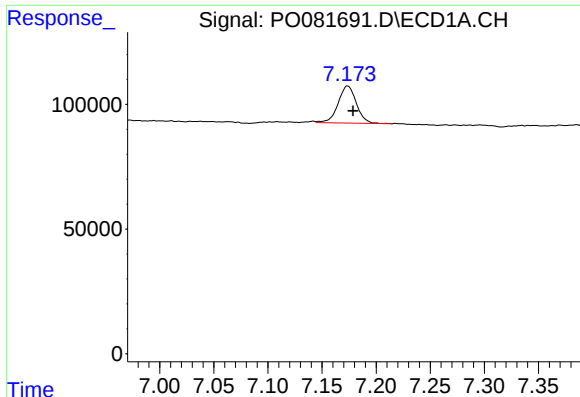

#20 AR-1242-5


R.T.: 7.174 min
Delta R.T.: -0.005 min
Response: 176036
Conc: 89.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

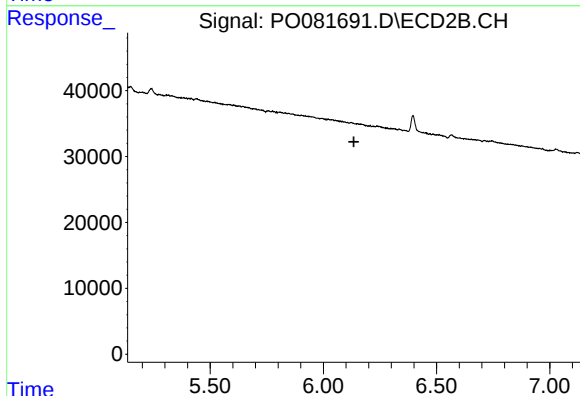


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.135 min
Response: 0
Conc: N.D.

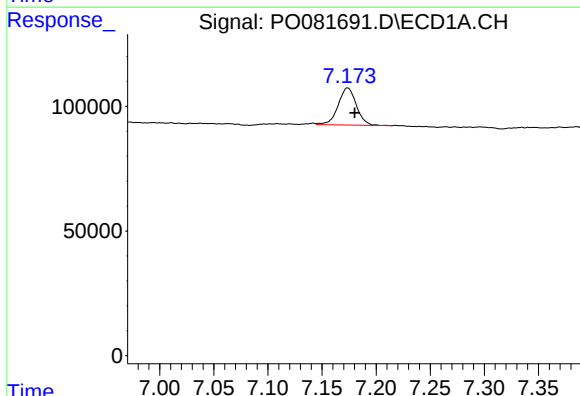


#25 AR-1248-5

R.T.: 7.174 min
Delta R.T.: -0.007 min
Response: 176036
Conc: 52.07 ng/ml

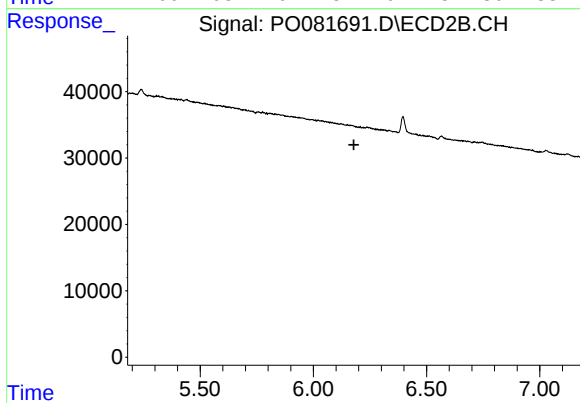

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.179 min
Response: 0
Conc: N.D.

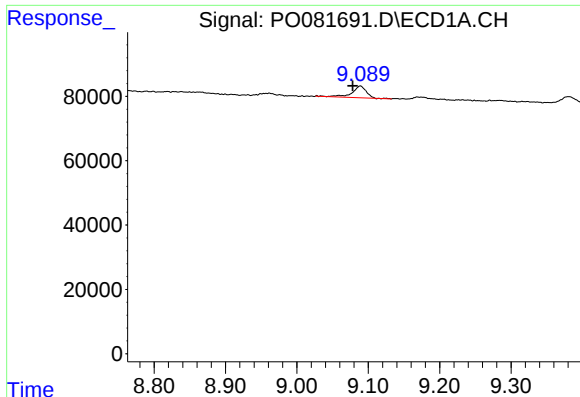

#35 AR-1260-5


R.T.: 9.089 min
Delta R.T.: 0.011 min
Response: 50955
Conc: 6.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

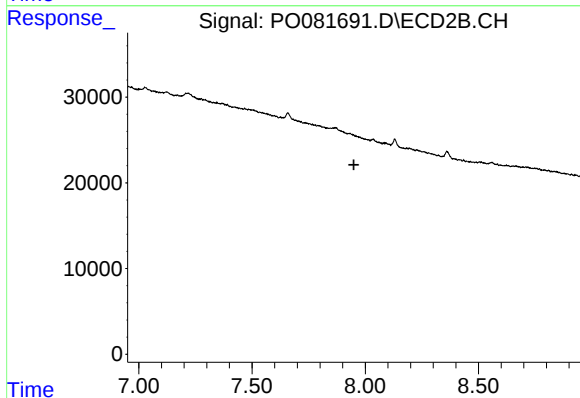


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.950 min
Response: 0
Conc: N.D.

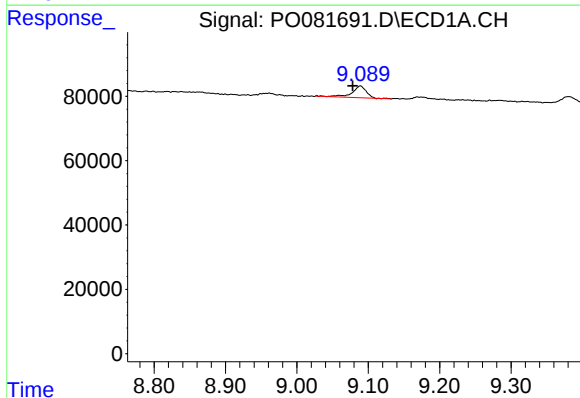


#37 AR-1262-2

R.T.: 9.089 min
Delta R.T.: 0.011 min
Response: 50955
Conc: 5.71 ng/ml

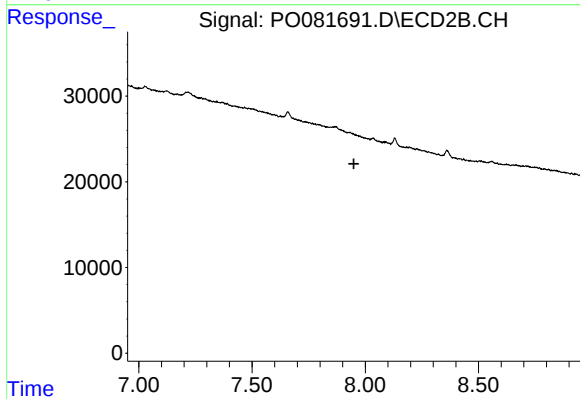

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.950 min
Response: 0
Conc: N.D.

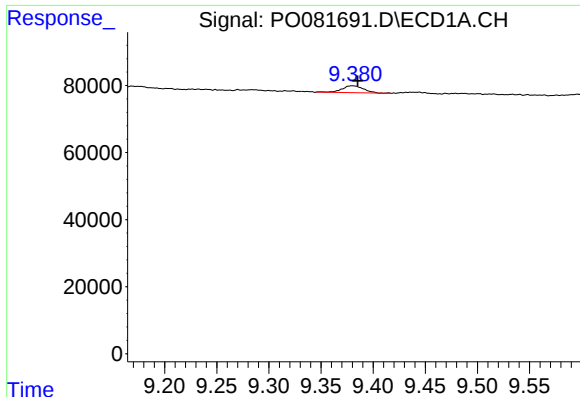

#38 AR-1262-3


R.T.: 9.381 min
Delta R.T.: -0.005 min
Response: 30005
Conc: 7.48 ng/ml

Instrument :
ECD_O
ClientSampleId :

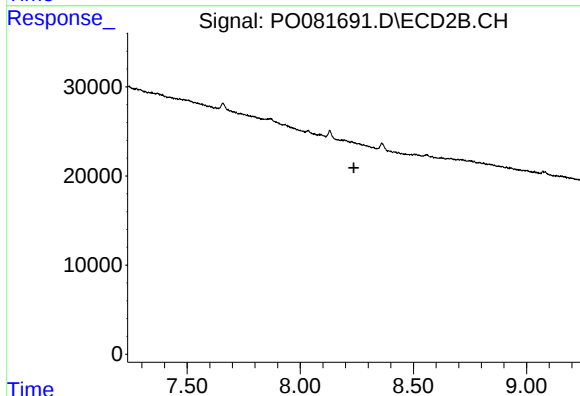


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

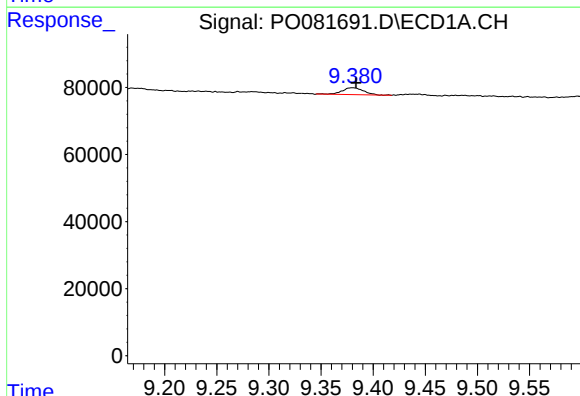

#41 AR-1268-1

R.T.: 9.381 min
Delta R.T.: -0.003 min
Response: 30005
Conc: 2.80 ng/ml

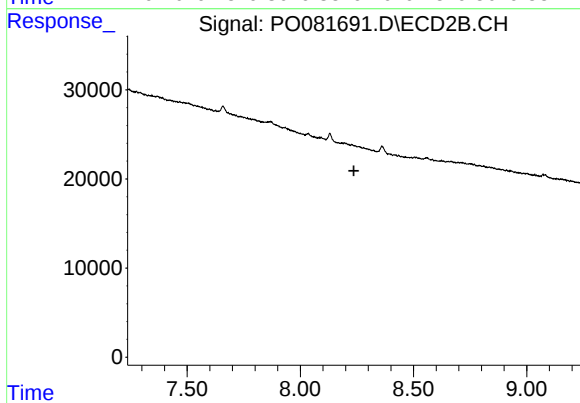

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.236 min
Response: 0
Conc: N.D.