

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0093021\
 Data File : P0081660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 13:54
 Operator : AJ\MA
 Sample : M3964-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CC-5

Manual Integrations
 APPROVED

mohammad
 10/1/2021 10:42:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 02:38:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.867	3.983	2205562	623793	24.733	23.414
2) SA Decachlor...	10.875	9.328	1894265	616864	25.431	26.563
Target Compounds						
26) L6 AR-1254-1	7.106	6.130	506662	272620	141.310	178.037 #
27) L6 AR-1254-2	7.337	6.290	1119510	223057	203.034	163.948
28) L6 AR-1254-3	7.718	6.714	1586666	491265	281.198m	246.970
29) L6 AR-1254-4	8.016	6.957	2085527	624631	507.172m	500.251
30) L6 AR-1254-5	8.445	7.389	1712371	679855	371.497m	363.672

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO093021\
Data File : PO081660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 13:54
Operator : AJ\MA
Sample : M3964-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CC-5


Manual Integrations
APPROVED

mohammad
10/1/2021 10:42:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 02:38:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

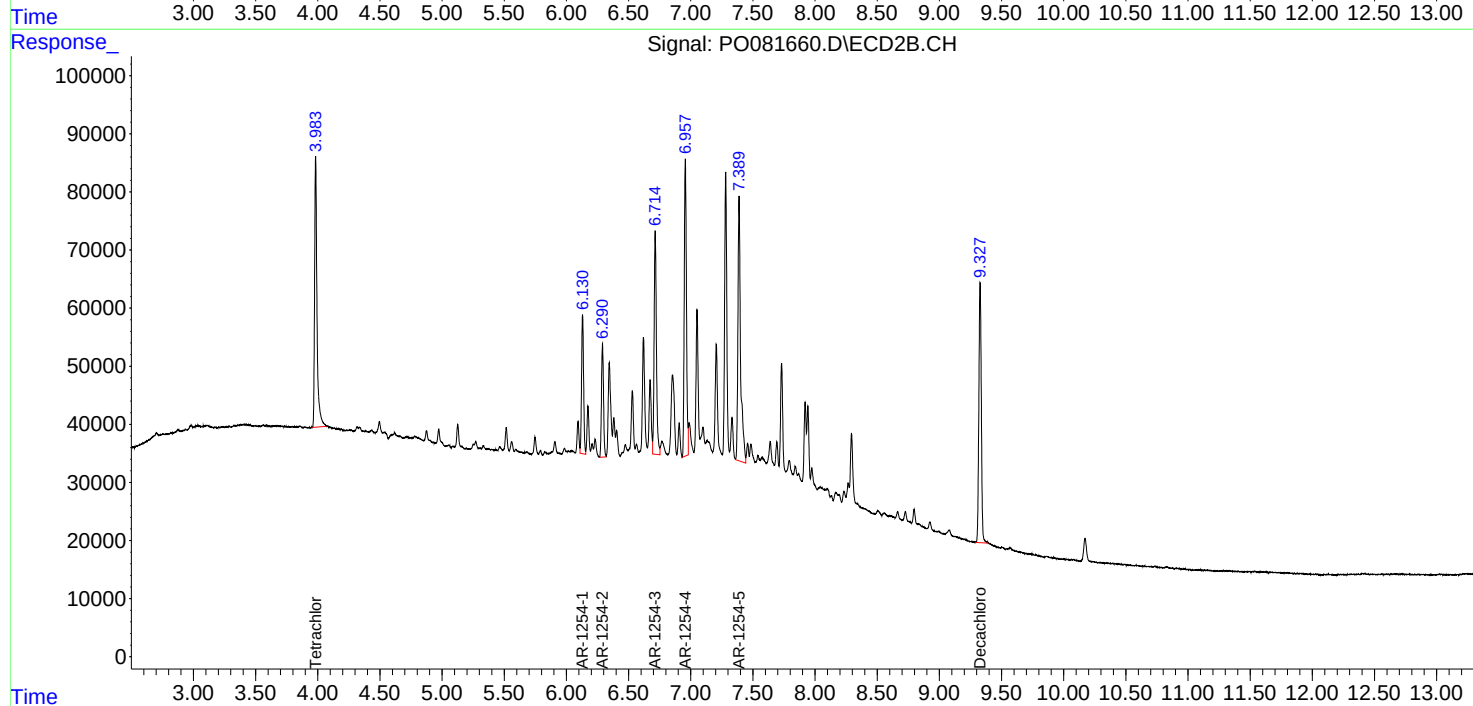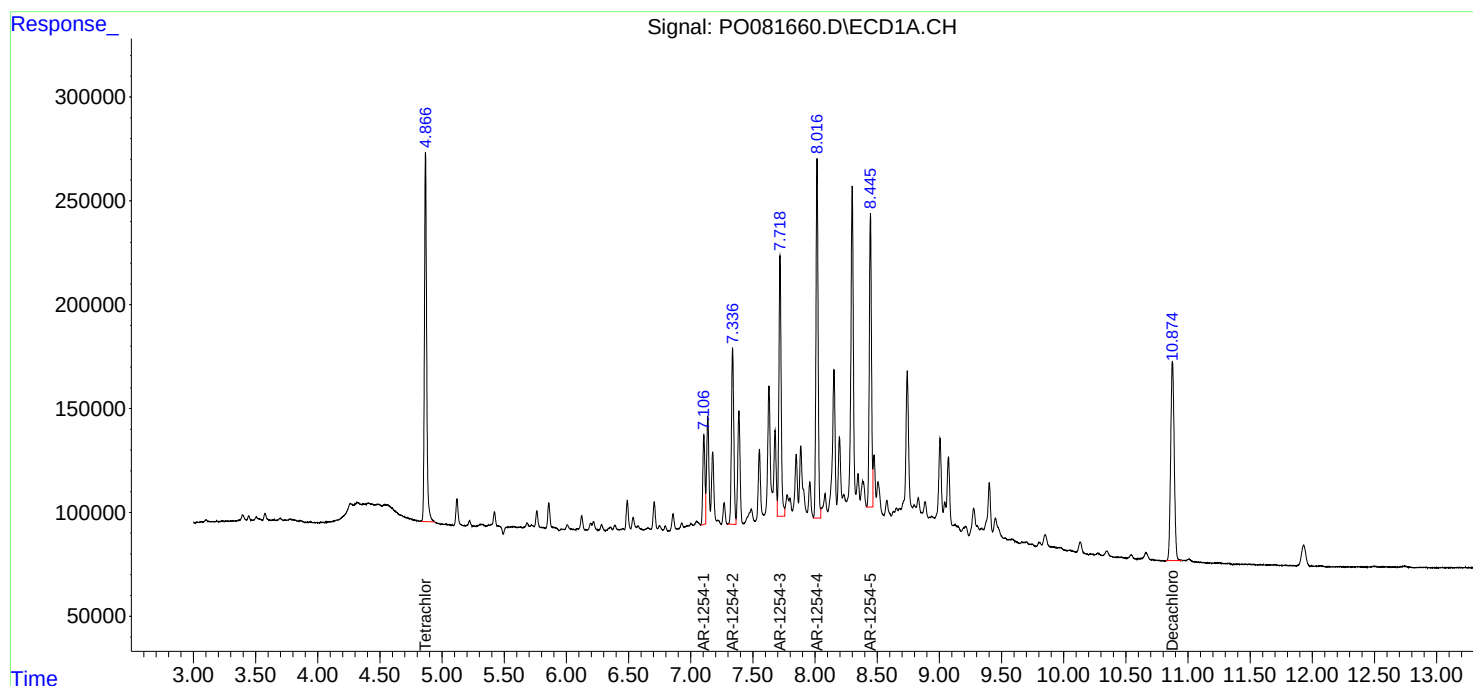

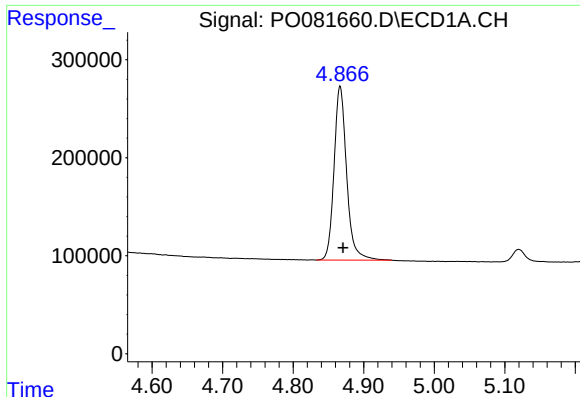


#1 Tetrachloro-m-xylene

R.T.: 4.867 min
Delta R.T.: -0.004 min
Response: 2205562
Conc: 24.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC-5


Manual Integrations
APPROVED

mohammad
10/1/2021 10:42:10 AM

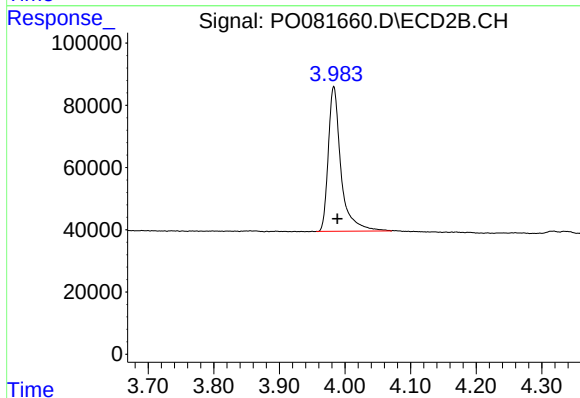


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.005 min
Response: 623793
Conc: 23.41 ng/ml

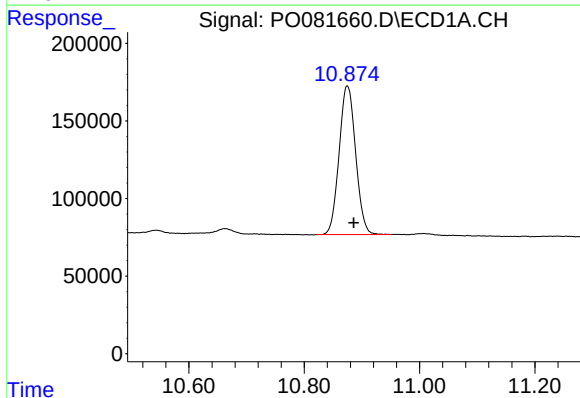


#2 Decachlorobiphenyl

R.T.: 10.875 min
Delta R.T.: -0.011 min
Response: 1894265
Conc: 25.43 ng/ml

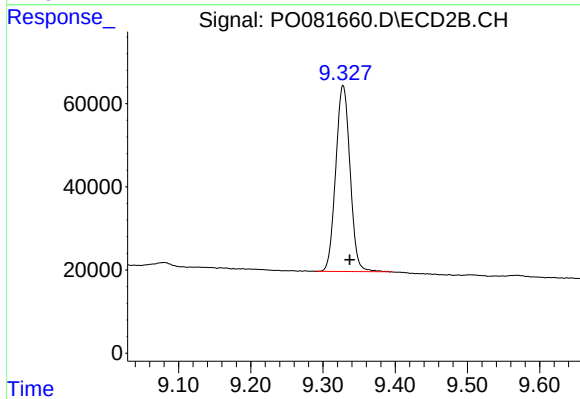

#2 Decachlorobiphenyl

R.T.: 9.328 min
Delta R.T.: -0.009 min
Response: 616864
Conc: 26.56 ng/ml

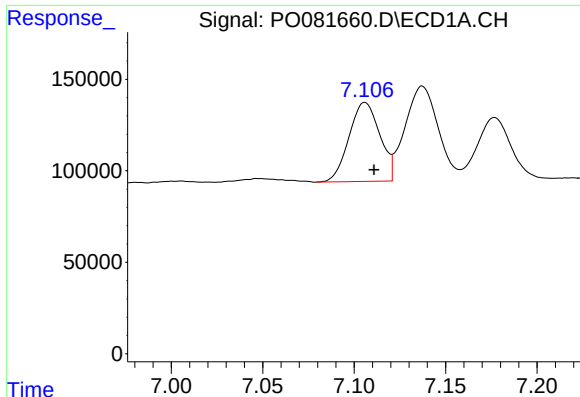


#26 AR-1254-1

R.T.: 7.106 min
Delta R.T.: -0.005 min
Response: 506662
Conc: 141.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC-5


Manual Integrations
APPROVED

mohammad
10/1/2021 10:42:10 AM

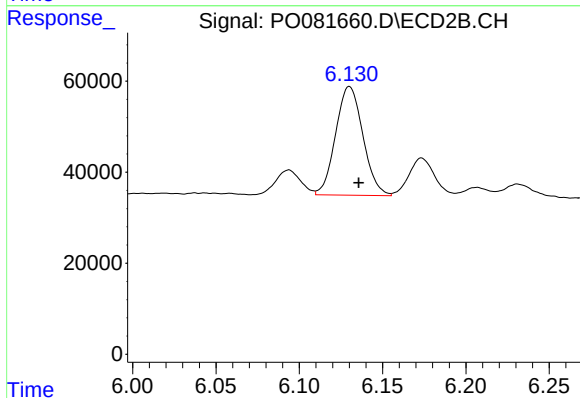


#26 AR-1254-1

R.T.: 6.130 min
Delta R.T.: -0.006 min
Response: 272620
Conc: 178.04 ng/ml

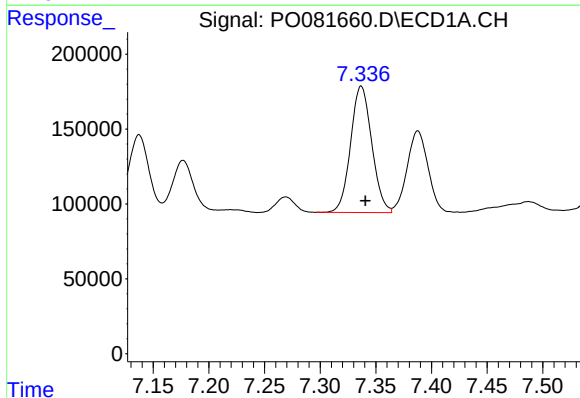


#27 AR-1254-2

R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 1119510
Conc: 203.03 ng/ml

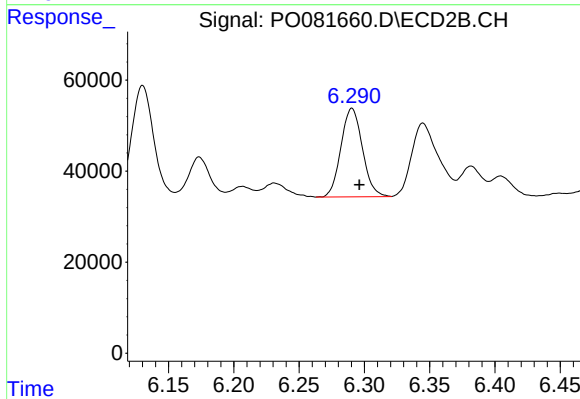

#27 AR-1254-2

R.T.: 6.290 min
Delta R.T.: -0.006 min
Response: 223057
Conc: 163.95 ng/ml

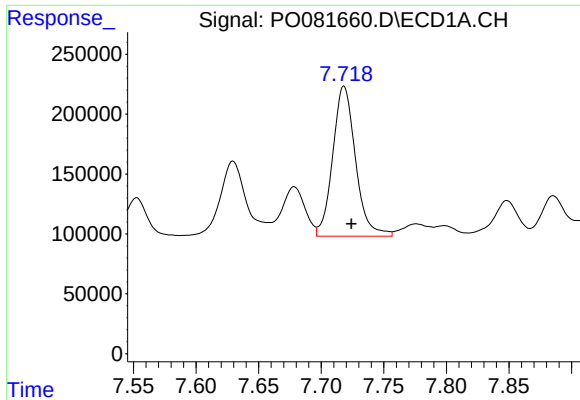


#28 AR-1254-3

R.T.: 7.718 min
Delta R.T.: -0.006 min
Response: 1586666
Conc: 281.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CC-5


Manual Integrations
APPROVED

mohammad
10/1/2021 10:42:10 AM

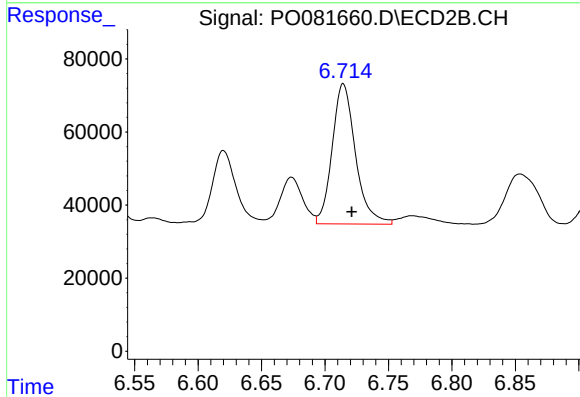


#28 AR-1254-3

R.T.: 6.714 min
Delta R.T.: -0.007 min
Response: 491265
Conc: 246.97 ng/ml

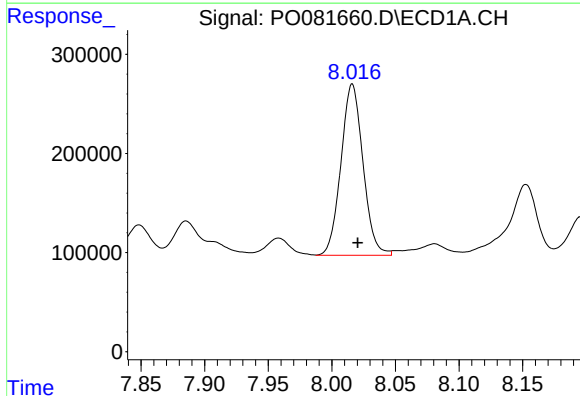


#29 AR-1254-4

R.T.: 8.016 min
Delta R.T.: -0.005 min
Response: 2085527
Conc: 507.17 ng/ml m

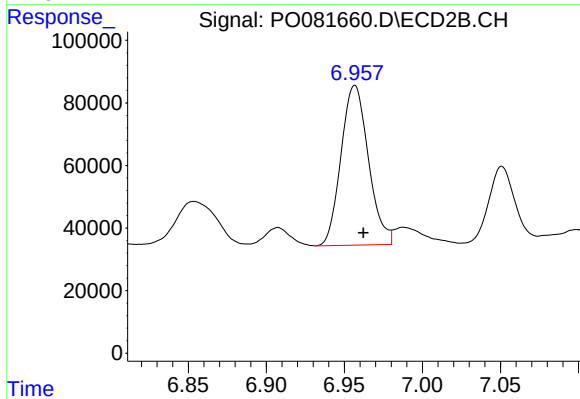

#29 AR-1254-4

R.T.: 6.957 min
Delta R.T.: -0.005 min
Response: 624631
Conc: 500.25 ng/ml

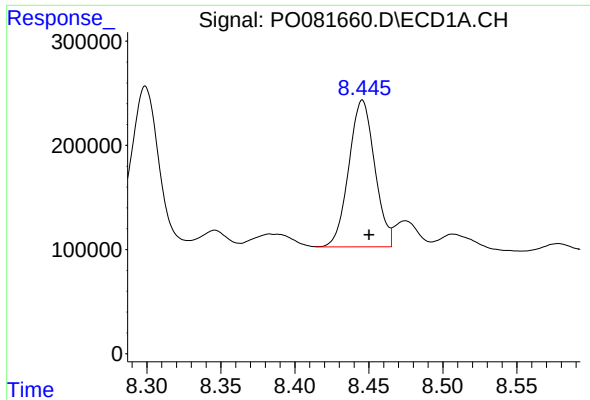


#30 AR-1254-5

R.T.: 8.445 min
Delta R.T.: -0.005 min
Response: 1712371
Conc: 371.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CC-5

Manual Integrations
APPROVED

mohammad
10/1/2021 10:42:10 AM

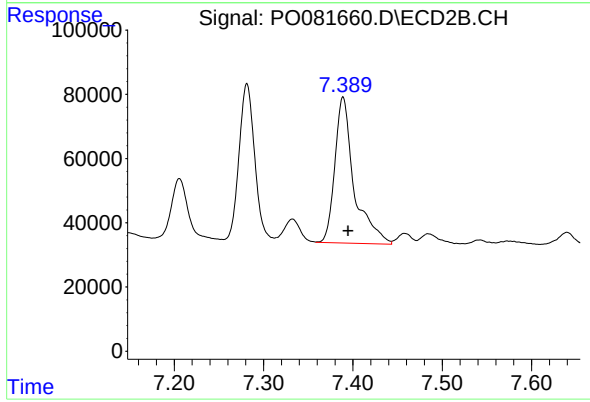

#30 AR-1254-5

R.T.: 7.389 min
Delta R.T.: -0.006 min
Response: 679855
Conc: 363.67 ng/ml