

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100120\
 Data File : P0071831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 14:48
 Operator : DD\AJ
 Sample : L4173-06RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 18:05:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.516	1533354	832129	17.868	20.204
2) SA Decachlor...	9.943	8.692	1408855	711151	12.263	11.699
Target Compounds						
12) L3 AR-1232-2	5.352	0.000	37831	0	39.108	N.D. #
34) L7 AR-1260-4	0.000	7.134	0	7109	N.D.	2.464 #
35) L7 AR-1260-5	0.000	7.382	0	2841	N.D.	0.384 #
37) L8 AR-1262-2	0.000	7.382	0	2841	N.D.	0.411 #
38) L8 AR-1262-3	0.000	7.657	0	6469	N.D.	2.169 #
39) L8 AR-1262-4	8.813	0.000	10120	0	2.666	N.D. #
41) L9 AR-1268-1	0.000	7.657	0	6469	N.D.	0.766 #
42) L9 AR-1268-2	8.813	0.000	10120	0	0.660	N.D. #
45) L9 AR-1268-5	0.000	8.487	0	25469	N.D.	1.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100120\
Data File : PO071831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 14:48
Operator : DD\AJ
Sample : L4173-06RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 18:05:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

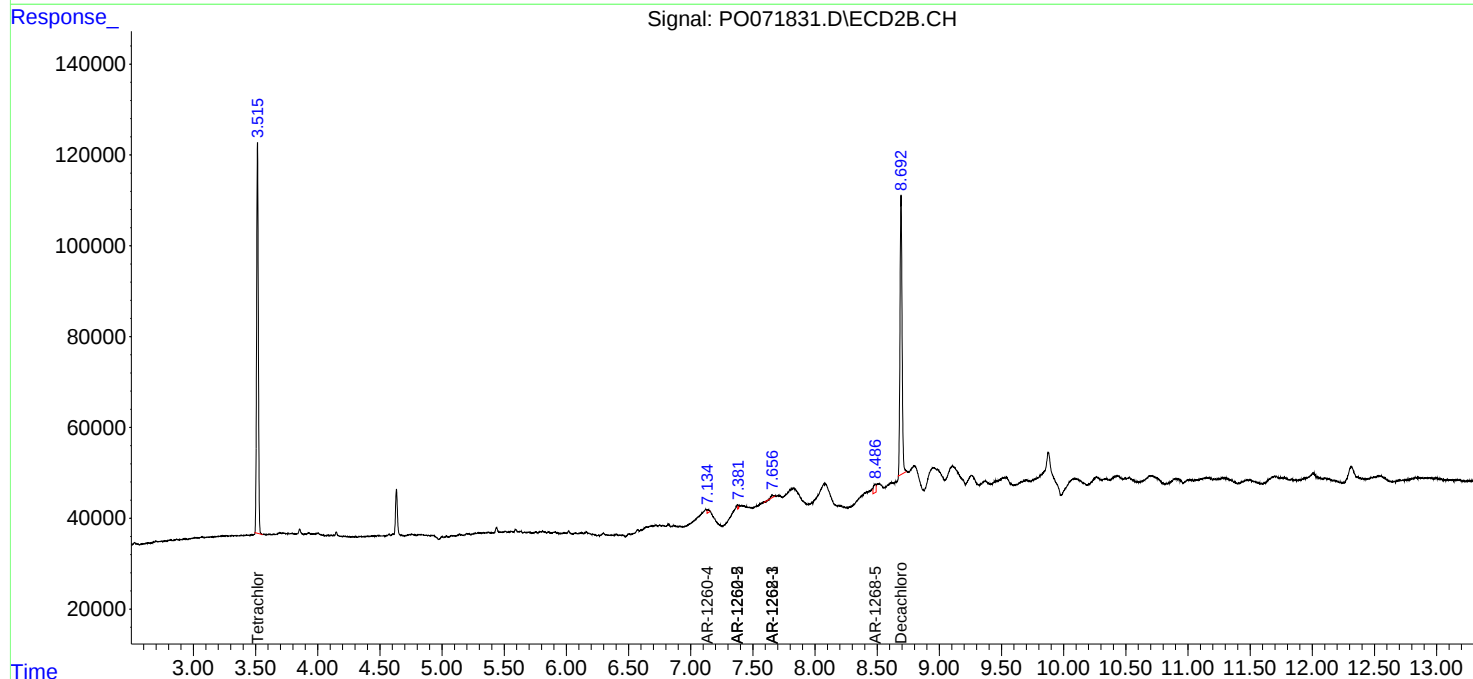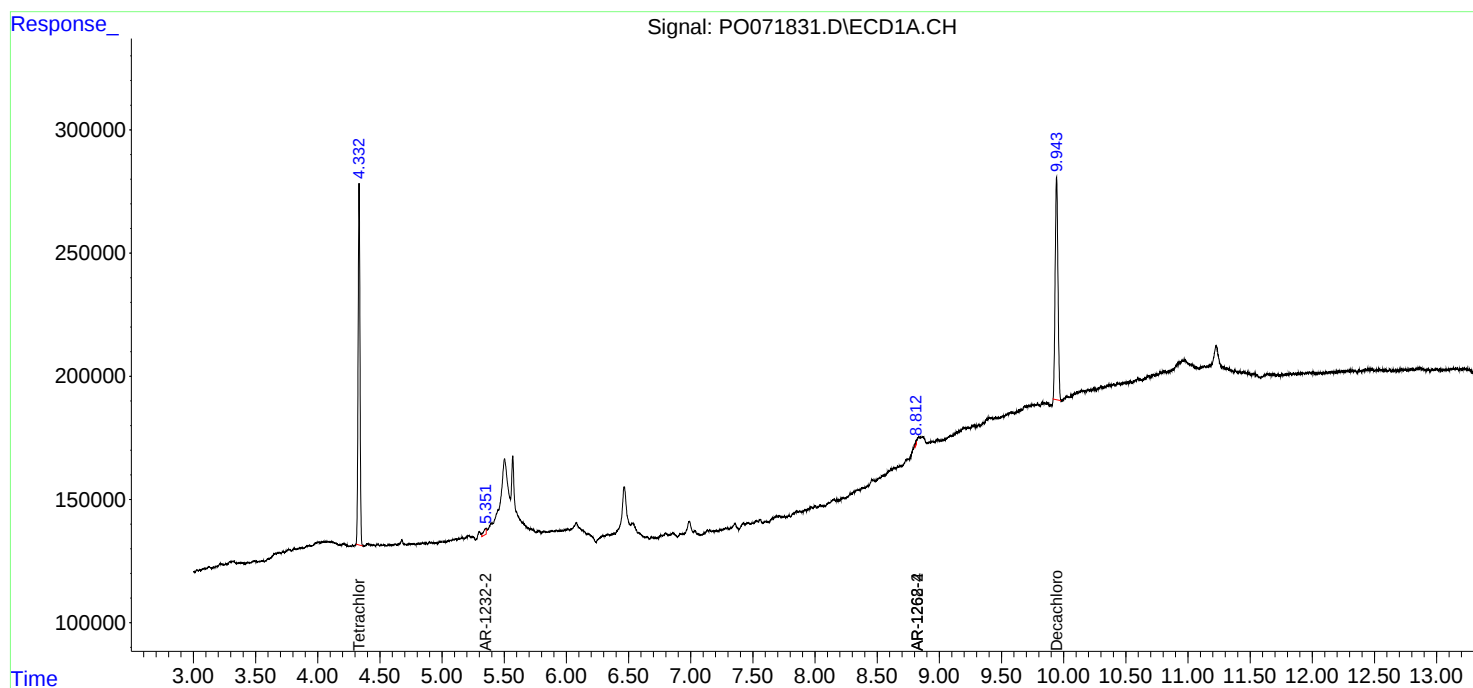


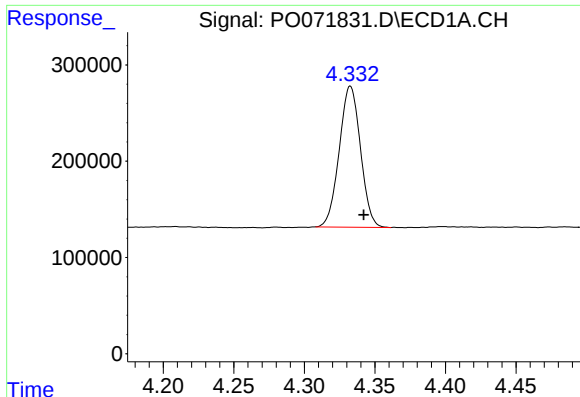

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.009 min
Response: 1533354
Conc: 17.87 ng/ml

Instrument :
ECD_O
ClientSampleId :

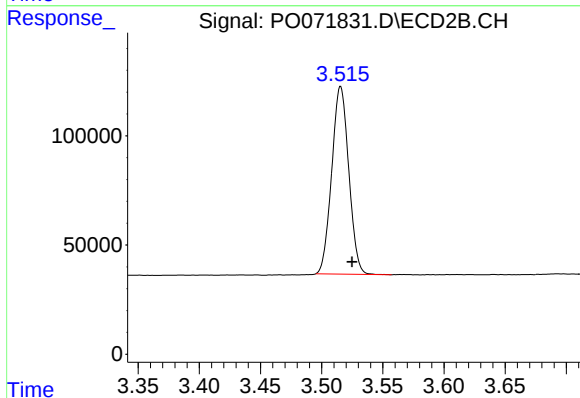


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 832129
Conc: 20.20 ng/ml

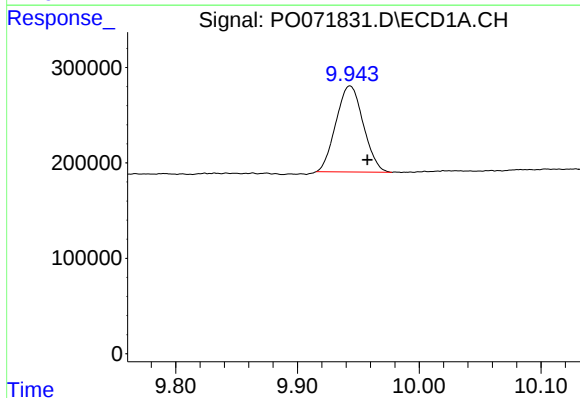


#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: -0.014 min
Response: 1408855
Conc: 12.26 ng/ml

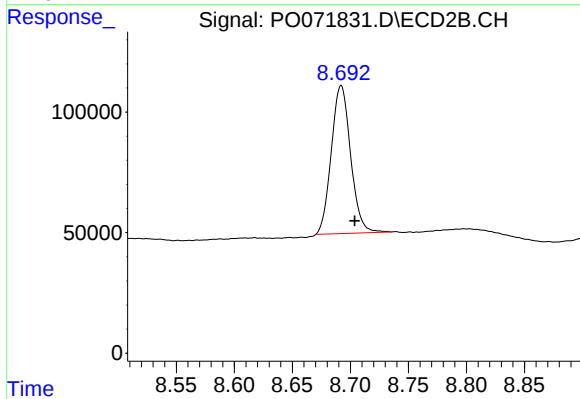

#2 Decachlorobiphenyl


R.T.: 8.692 min
Delta R.T.: -0.012 min
Response: 711151
Conc: 11.70 ng/ml

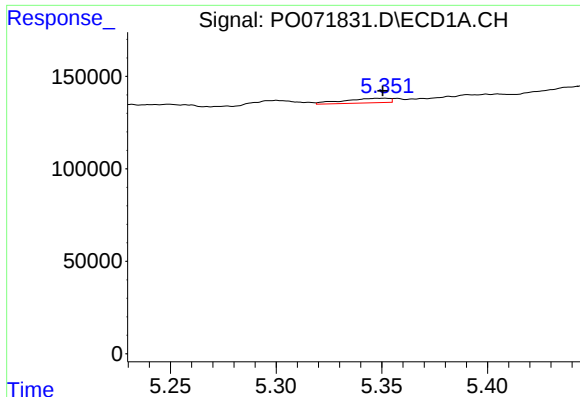

#12 AR-1232-2


R.T.: 5.352 min
Delta R.T.: 0.001 min
Response: 37831
Conc: 39.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

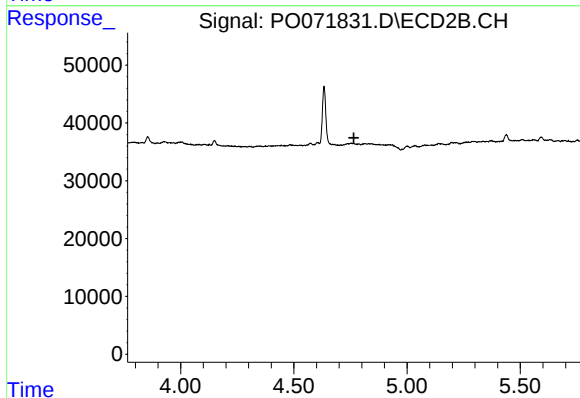


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

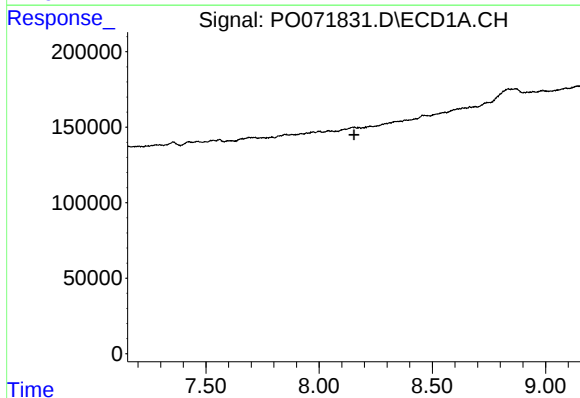


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.154 min
Response: 0
Conc: N.D.

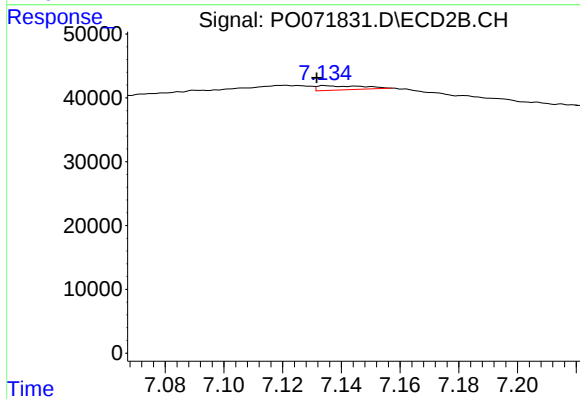

#34 AR-1260-4


R.T.: 7.134 min
Delta R.T.: 0.003 min
Response: 7109
Conc: 2.46 ng/ml

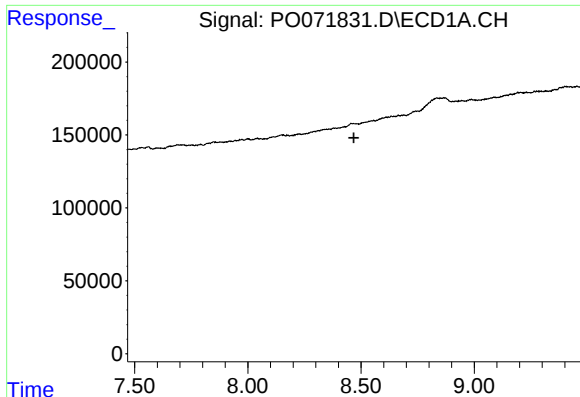

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

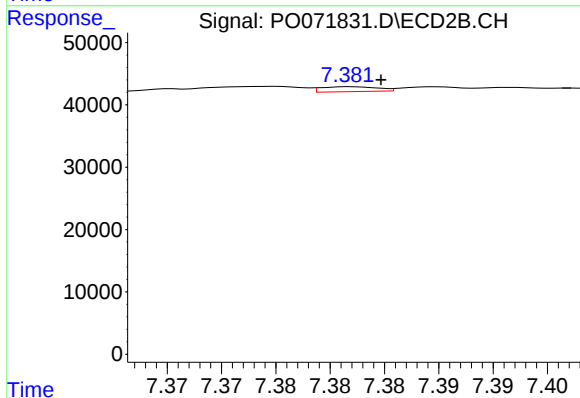


#35 AR-1260-5

R.T.: 7.382 min
Delta R.T.: -0.003 min
Response: 2841
Conc: 0.38 ng/ml

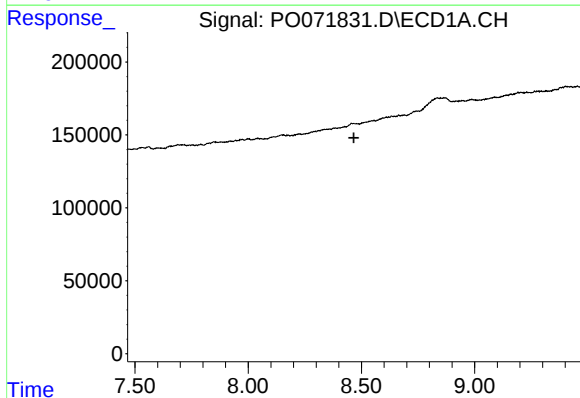


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

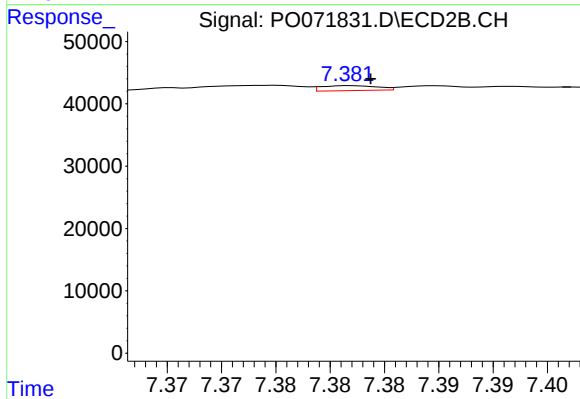

#37 AR-1262-2


R.T.: 7.382 min
Delta R.T.: -0.002 min
Response: 2841
Conc: 0.41 ng/ml

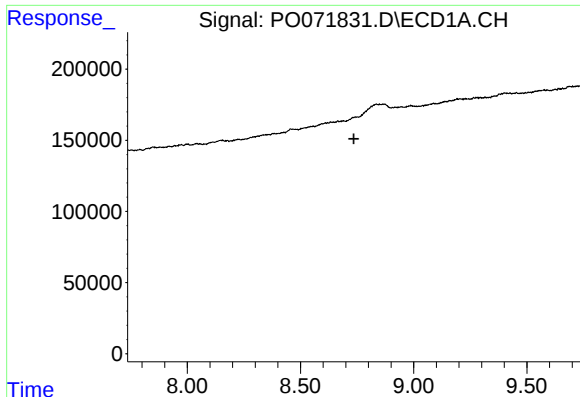

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

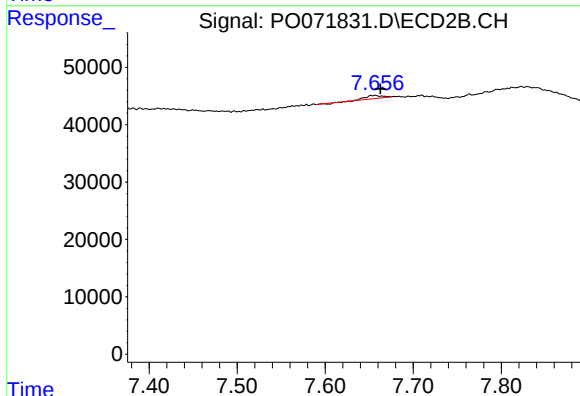


#38 AR-1262-3

R.T.: 7.657 min
Delta R.T.: -0.006 min
Response: 6469
Conc: 2.17 ng/ml

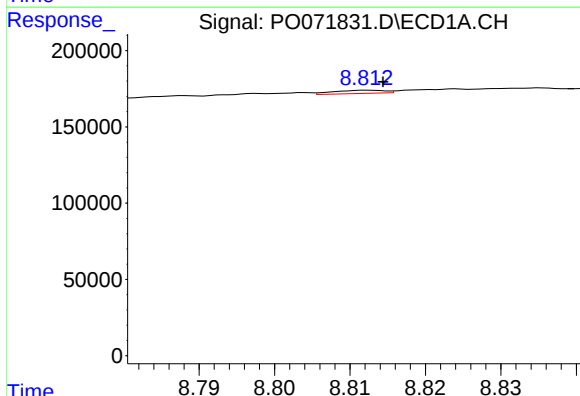


#39 AR-1262-4

R.T.: 8.813 min
Delta R.T.: -0.002 min
Response: 10120
Conc: 2.67 ng/ml

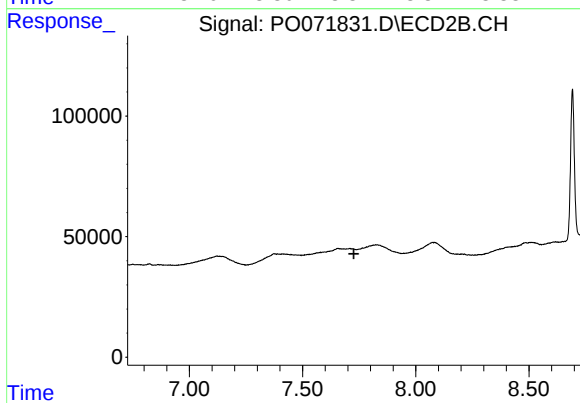

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

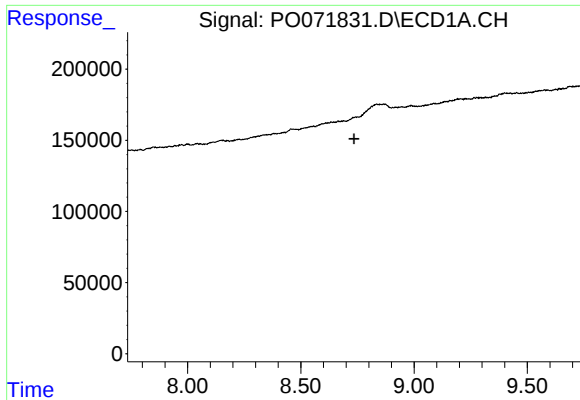

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.735 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

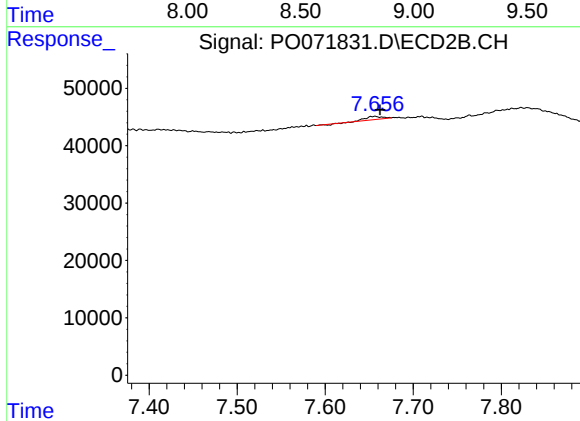


#41 AR-1268-1

R.T.: 7.657 min
Delta R.T.: -0.005 min
Response: 6469
Conc: 0.77 ng/ml

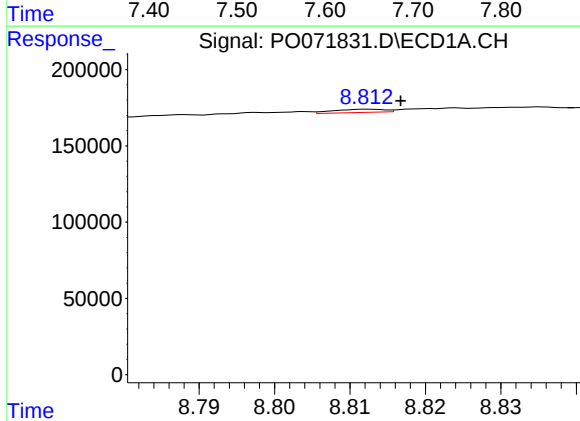


#42 AR-1268-2

R.T.: 8.813 min
Delta R.T.: -0.004 min
Response: 10120
Conc: 0.66 ng/ml

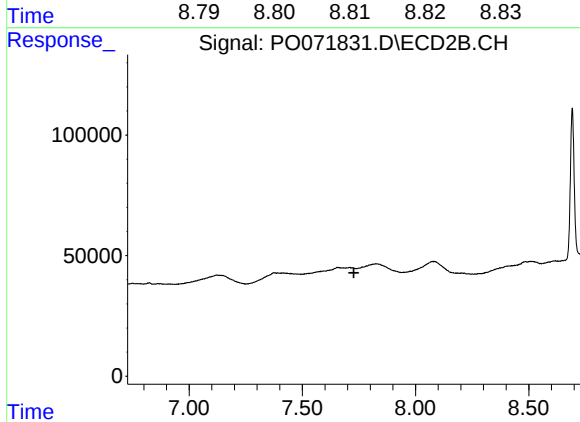

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.728 min
Response: 0
Conc: N.D.

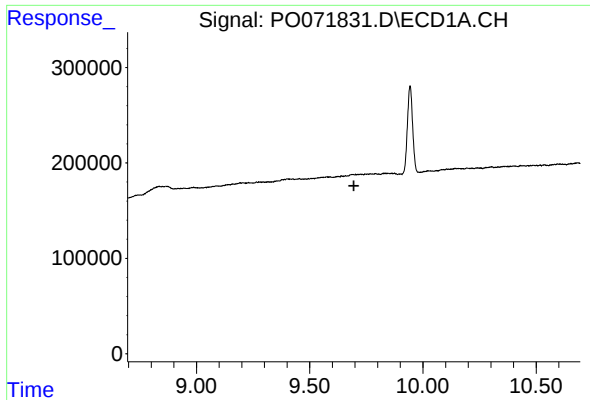

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.695 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

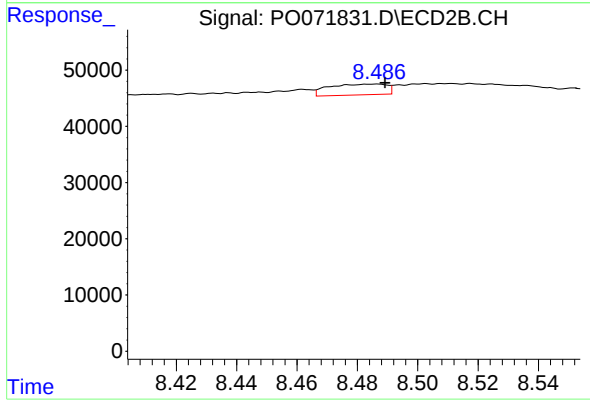

#45 AR-1268-5

R.T.: 8.487 min
Delta R.T.: -0.002 min
Response: 25469
Conc: 1.24 ng/ml