

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100120\
 Data File : P0071830.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2020 14:31
 Operator : DD\AJ
 Sample : L4173-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-(0-6FT)RE

Manual Integrations
 APPROVED

Ankita
 10/2/2020 2:56:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 18:05:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.516	1311714	682160	15.286m	16.563m
2) SA Decachlor...	9.943	8.692	1205337	611449	10.491m	10.059m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100120\
Data File : PO071830.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2020 14:31
Operator : DD\AJ
Sample : L4173-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1-(0-6FT)RE


Manual Integrations
APPROVED

Ankita
10/2/2020 2:56:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 18:05:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

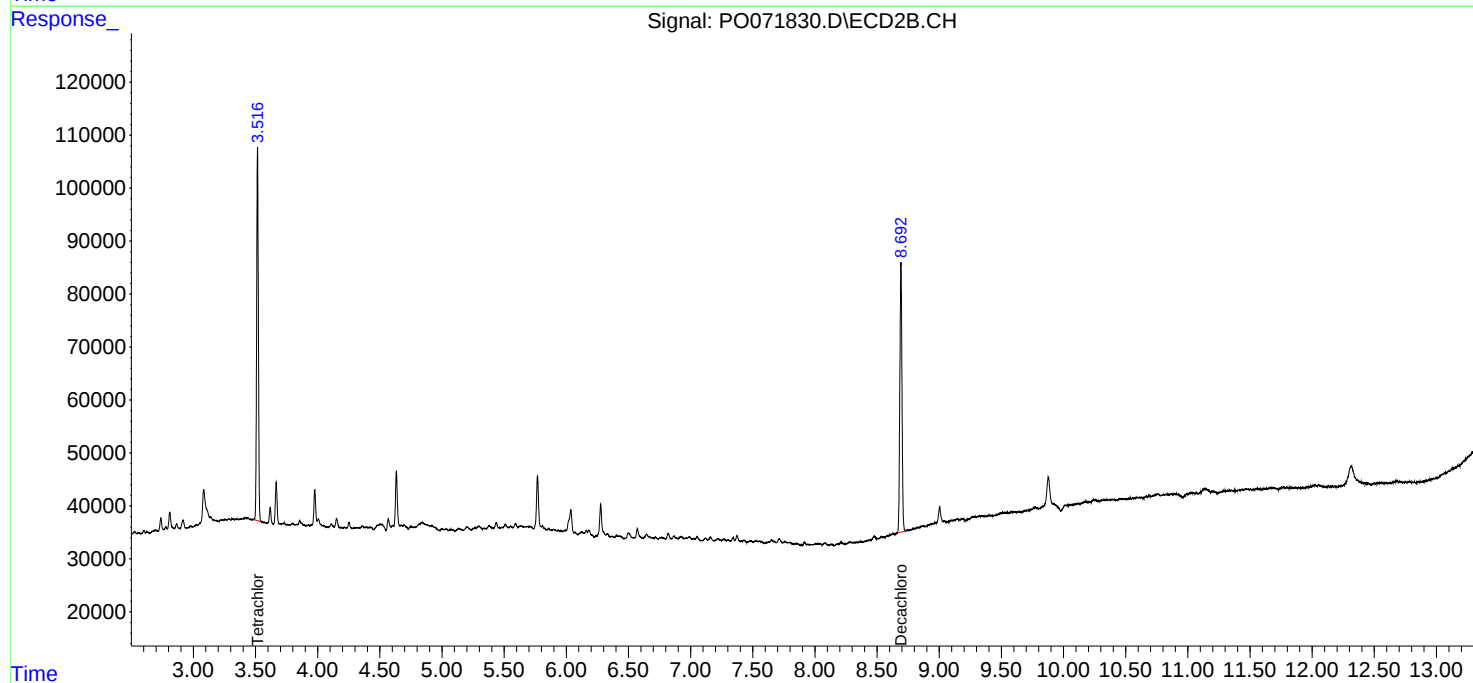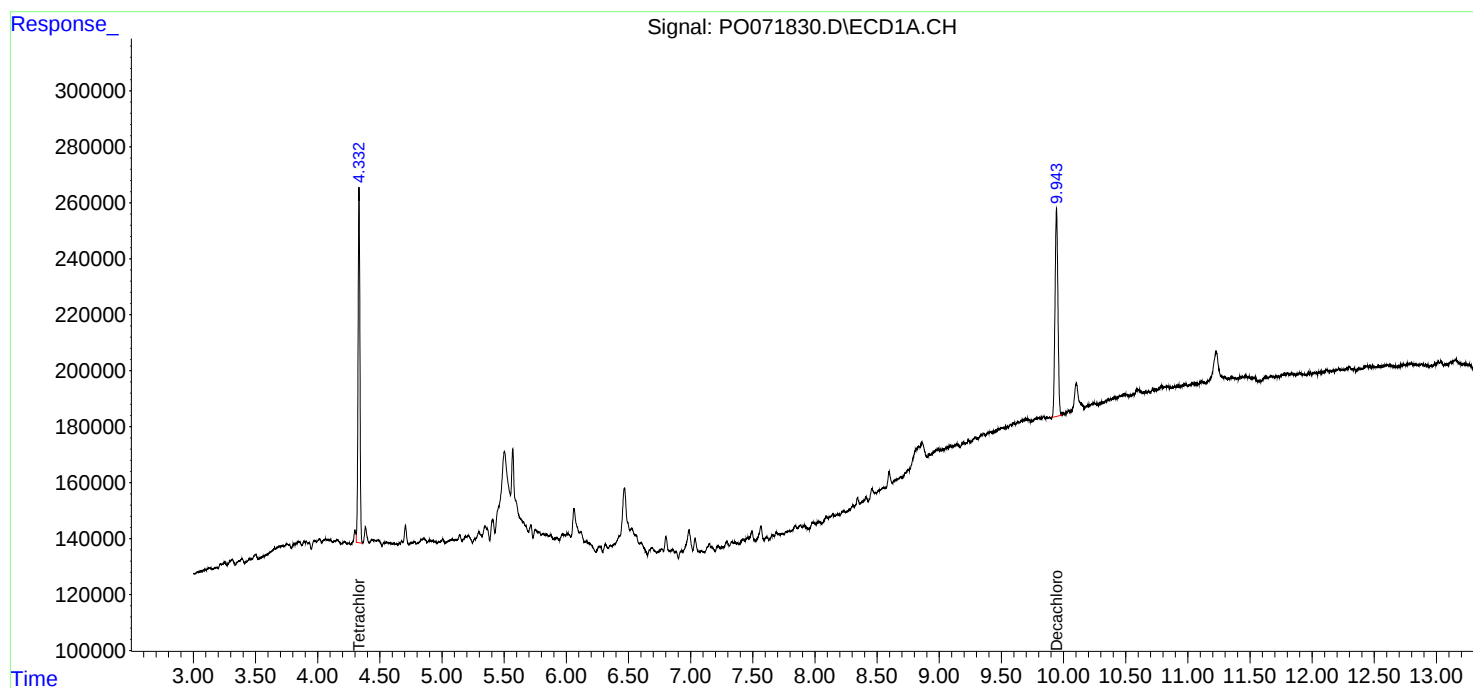

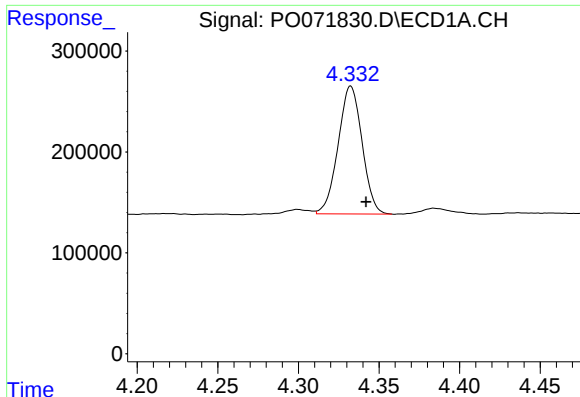


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: -0.010 min
Response: 1311714
Conc: 15.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1-(0-6FT)RE


Manual Integrations
APPROVED

Ankita
10/2/2020 2:56:44 PM

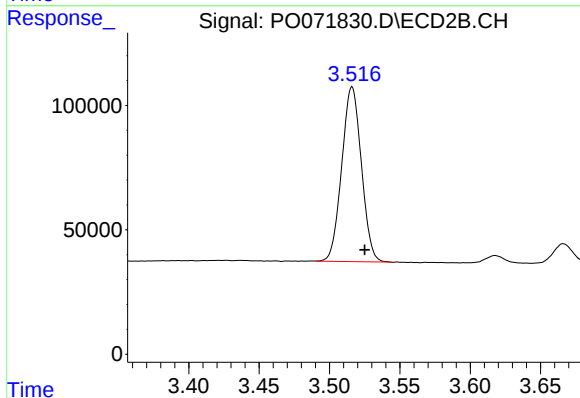


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 682160
Conc: 16.56 ng/ml m

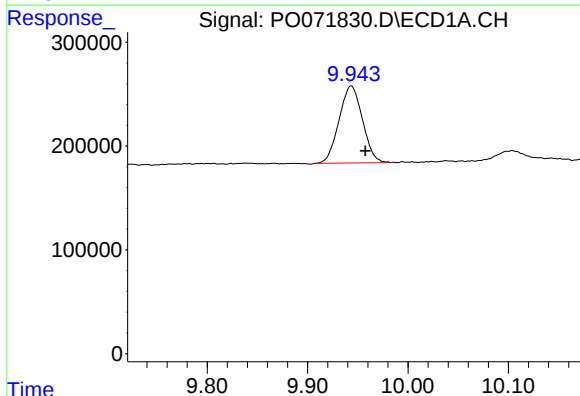

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: -0.014 min
Response: 1205337
Conc: 10.49 ng/ml m

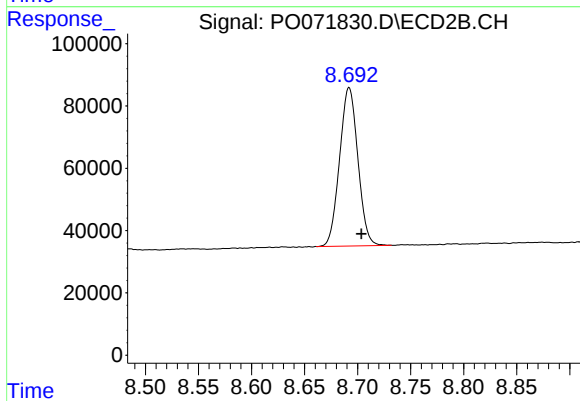

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.012 min
Response: 611449
Conc: 10.06 ng/ml m