

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100120\
 Data File : PO071876.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2020 3:38
 Operator : DD\AJ
 Sample : L4245-23
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FB-02-(20201001)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 08:56:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.516	1558083	806612	18.157	19.585
2)	SA Decachlor...	9.943	8.691	2187631	1163715	19.041	19.145

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100120\
Data File : P0071876.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 3:38
Operator : DD\AJ
Sample : L4245-23
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FB-02-(20201001)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 08:56:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

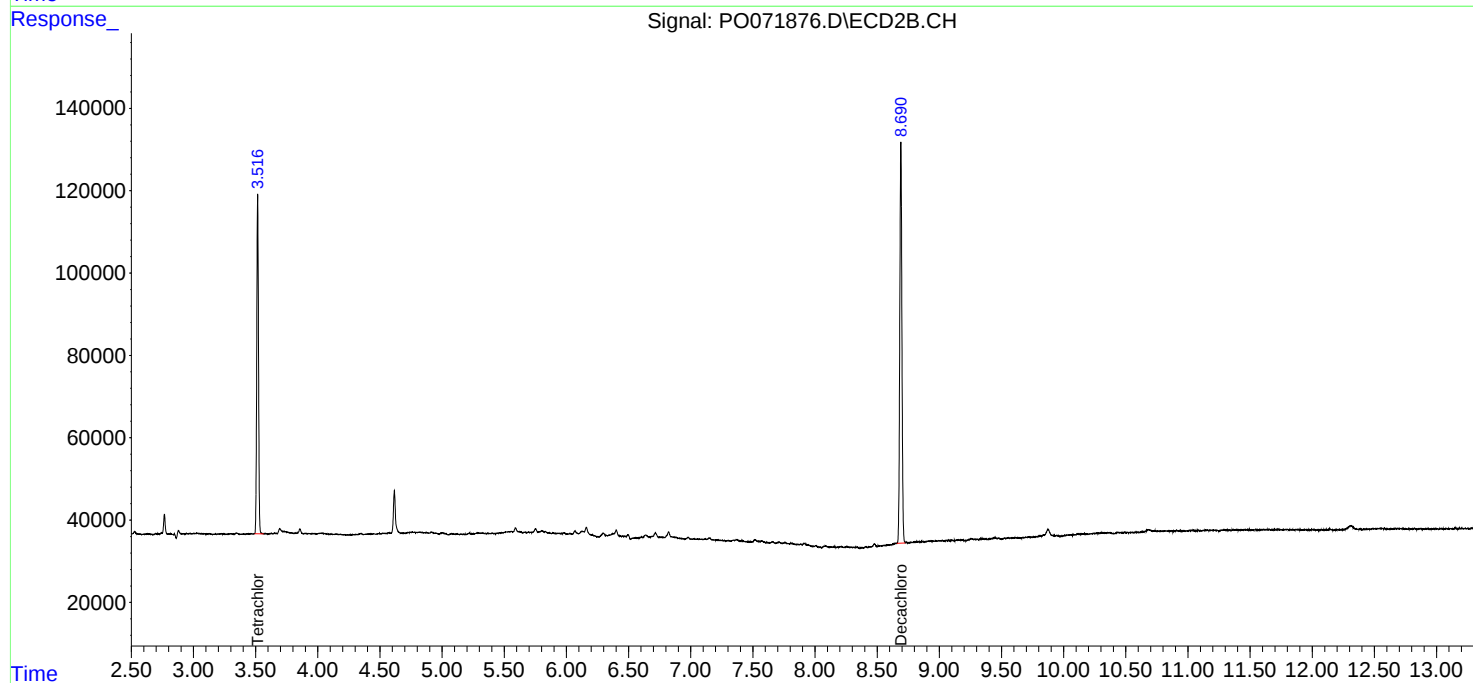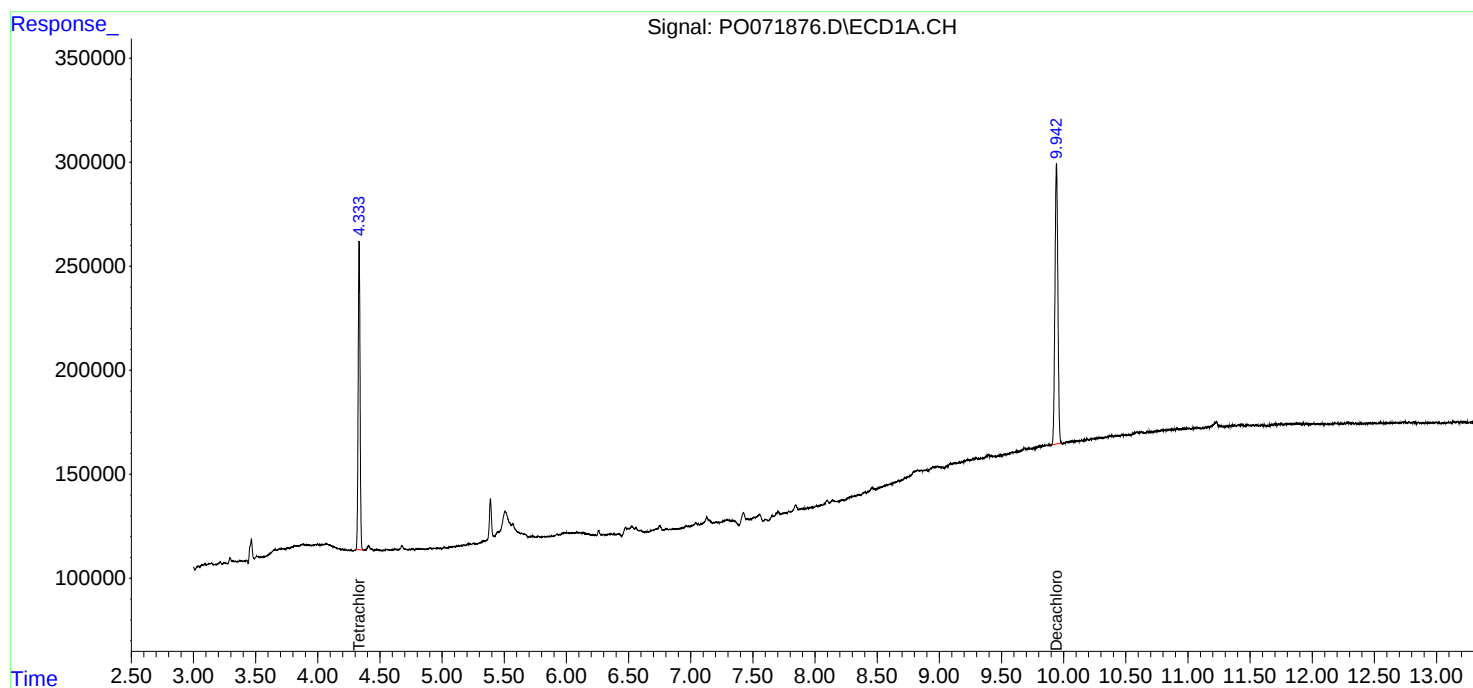


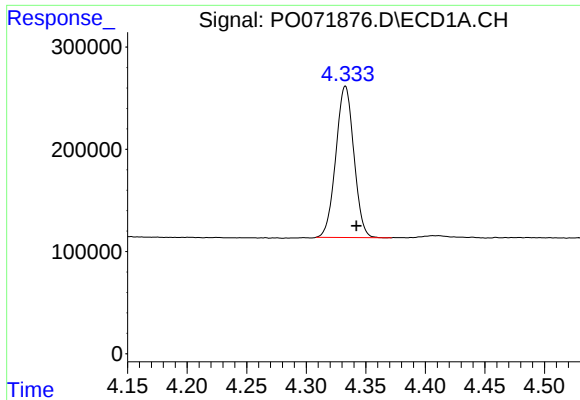

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: -0.009 min
Response: 1558083
Conc: 18.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FB-02-(20201001)

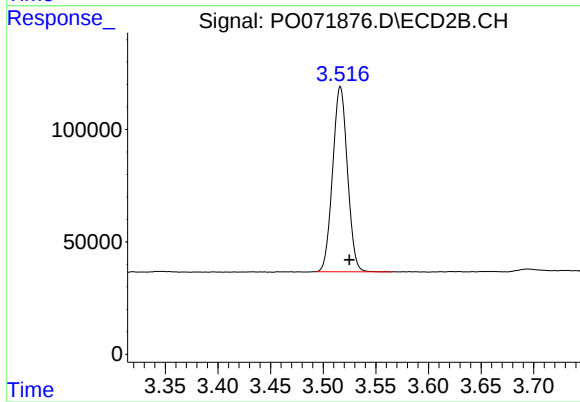


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: -0.009 min
Response: 806612
Conc: 19.58 ng/ml

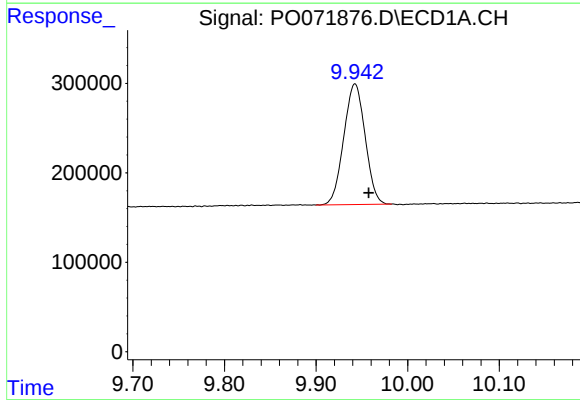

#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: -0.015 min
Response: 2187631
Conc: 19.04 ng/ml

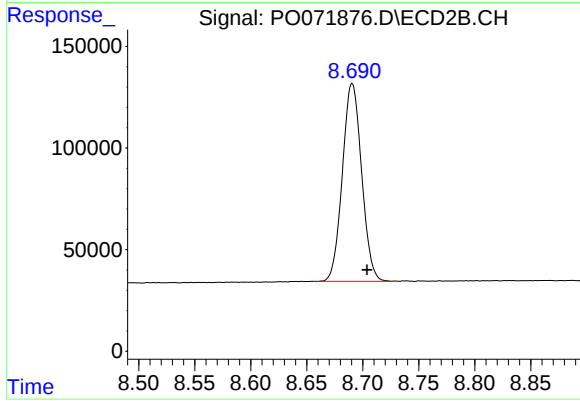

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: -0.013 min
Response: 1163715
Conc: 19.14 ng/ml