

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100121\
 Data File : P0081711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Oct 2021 14:29
 Operator : AJ\MA
 Sample : M4017-05 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HED184-J(1-1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 02:38:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	3.985	142229	35933	1.595	1.349
2)	SA Decachlor...	10.878	9.328	120407	46742	1.616	2.013

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100121\
Data File : PO081711.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Oct 2021 14:29
Operator : AJ\MA
Sample : M4017-05 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HED184-J(1-1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 02:38:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

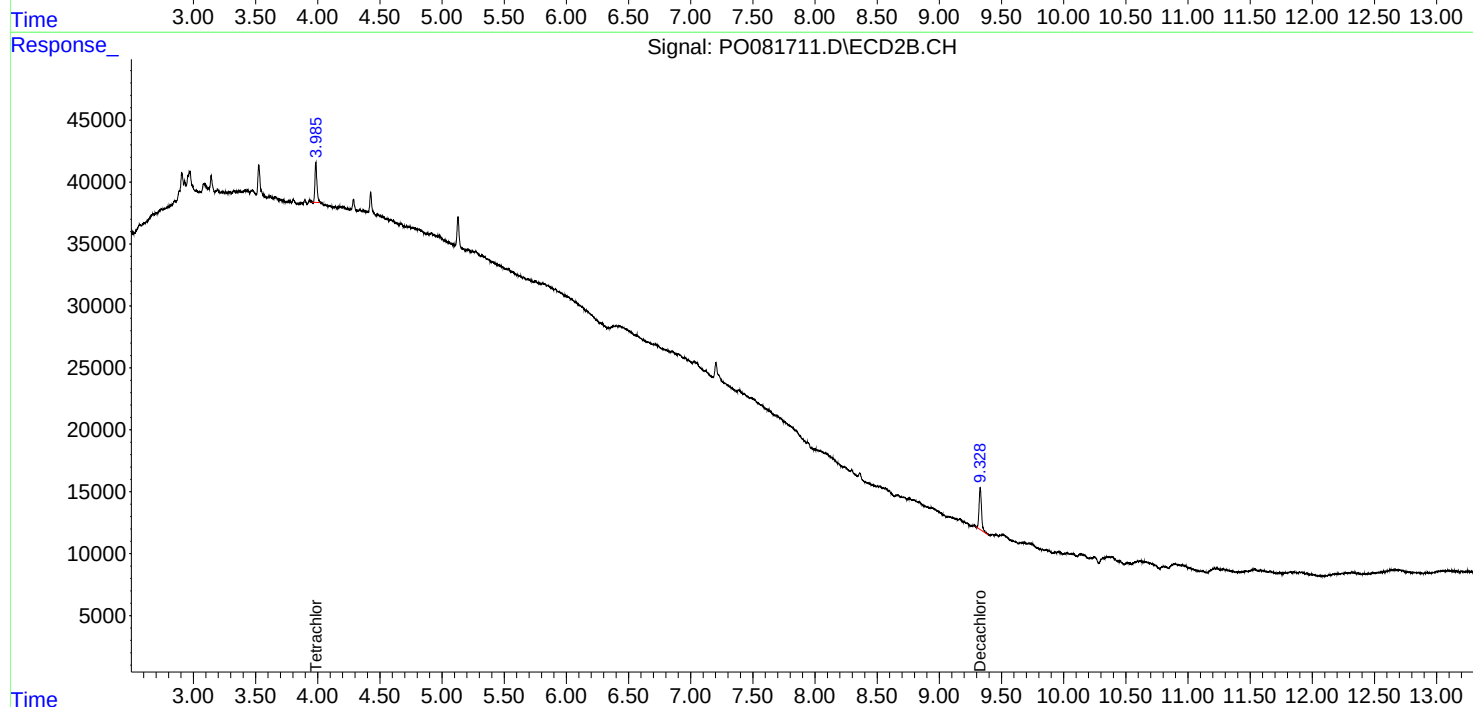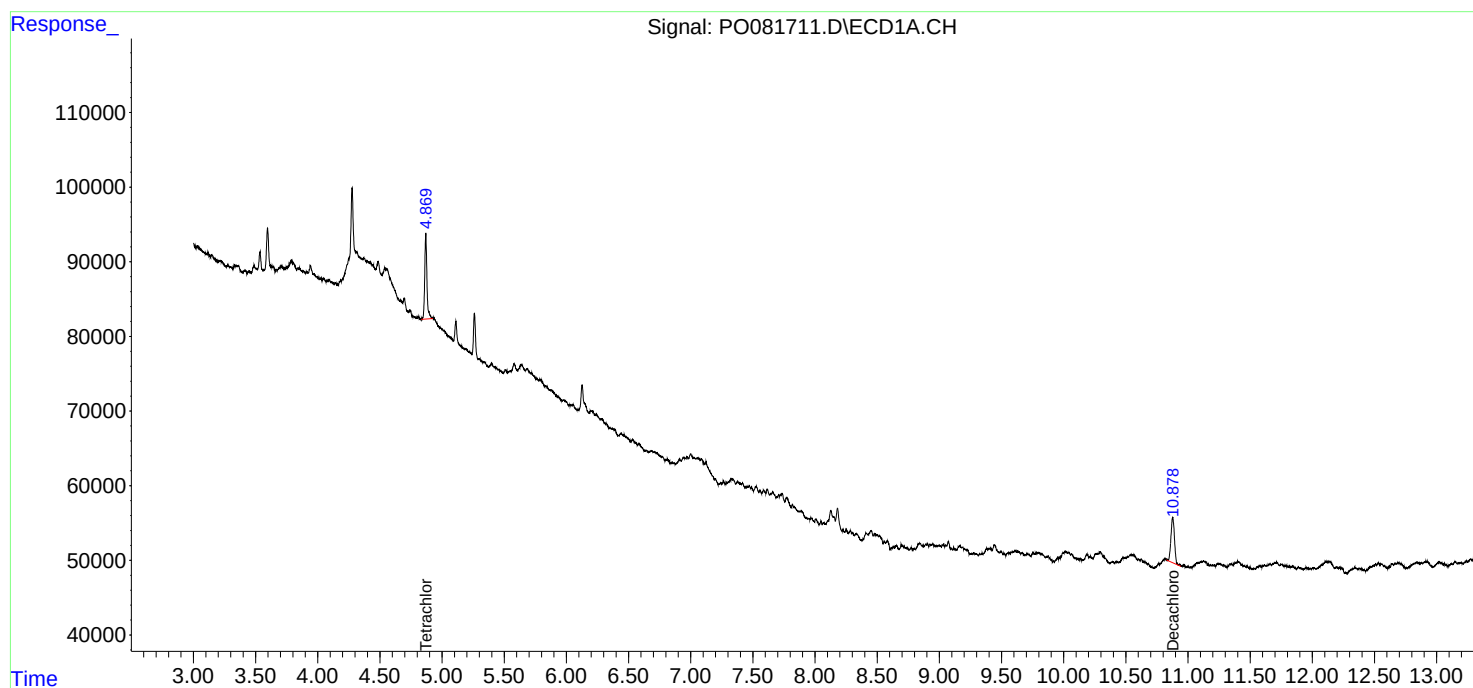


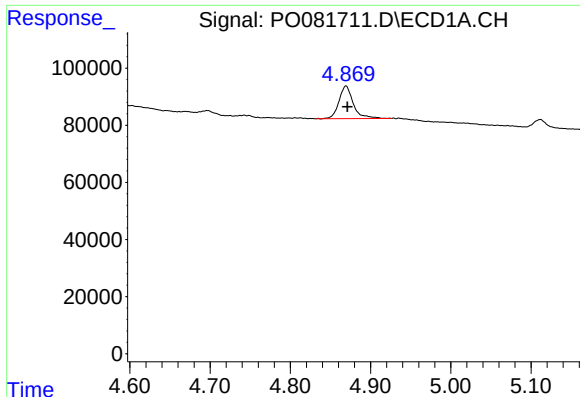

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 142229
Conc: 1.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
HED184-J(1-1)

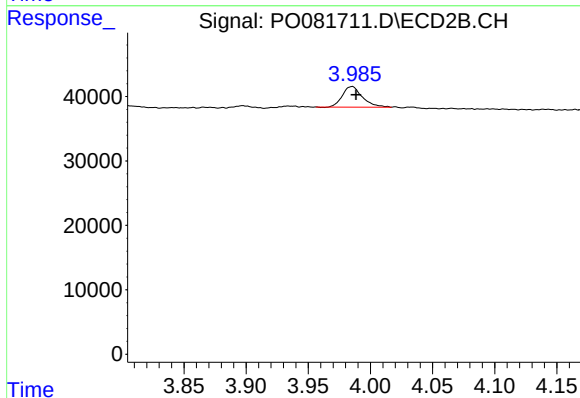


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: -0.003 min
Response: 35933
Conc: 1.35 ng/ml

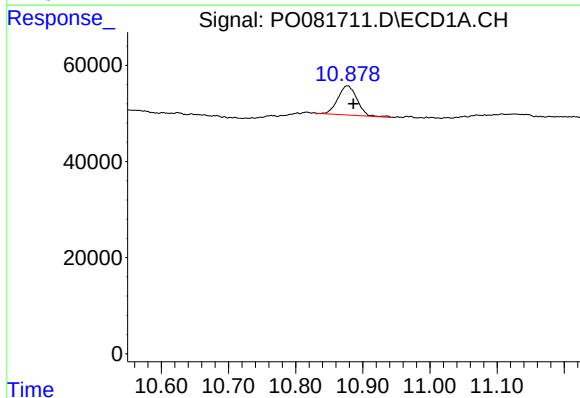

#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.008 min
Response: 120407
Conc: 1.62 ng/ml

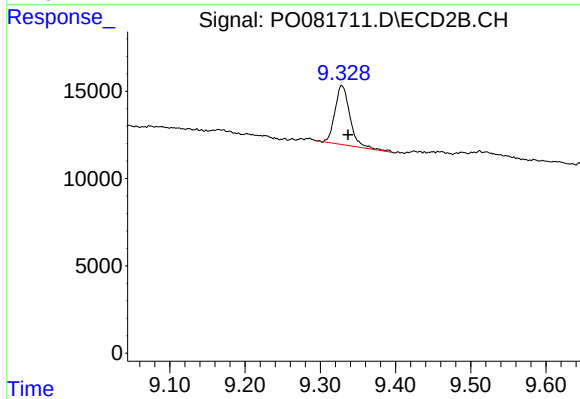

#2 Decachlorobiphenyl

R.T.: 9.328 min
Delta R.T.: -0.009 min
Response: 46742
Conc: 2.01 ng/ml