

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100218\
 Data File : PO049560.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2018 16:10
 Operator : SM/SJ
 Sample : J5153-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 4-NW-CARDBOARD-COIL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 09:11:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.540	3376405	1563626	9.561	4.597 #
2) SA Decachlor...	10.096	8.447	2338624	1209455	4.935	3.959

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100218\
Data File : P0049560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2018 16:10
Operator : SM/SJ
Sample : J5153-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
4-NW-CARDBOARD-COIL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 09:11:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

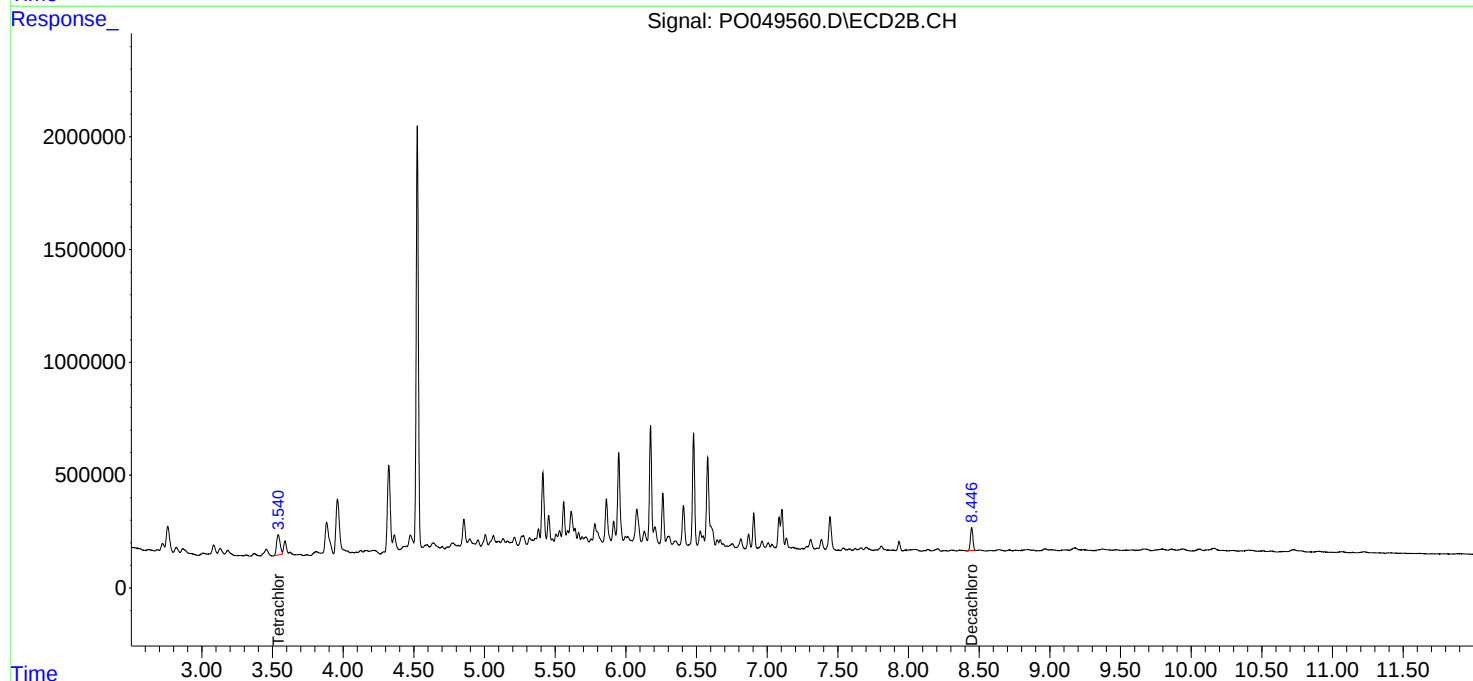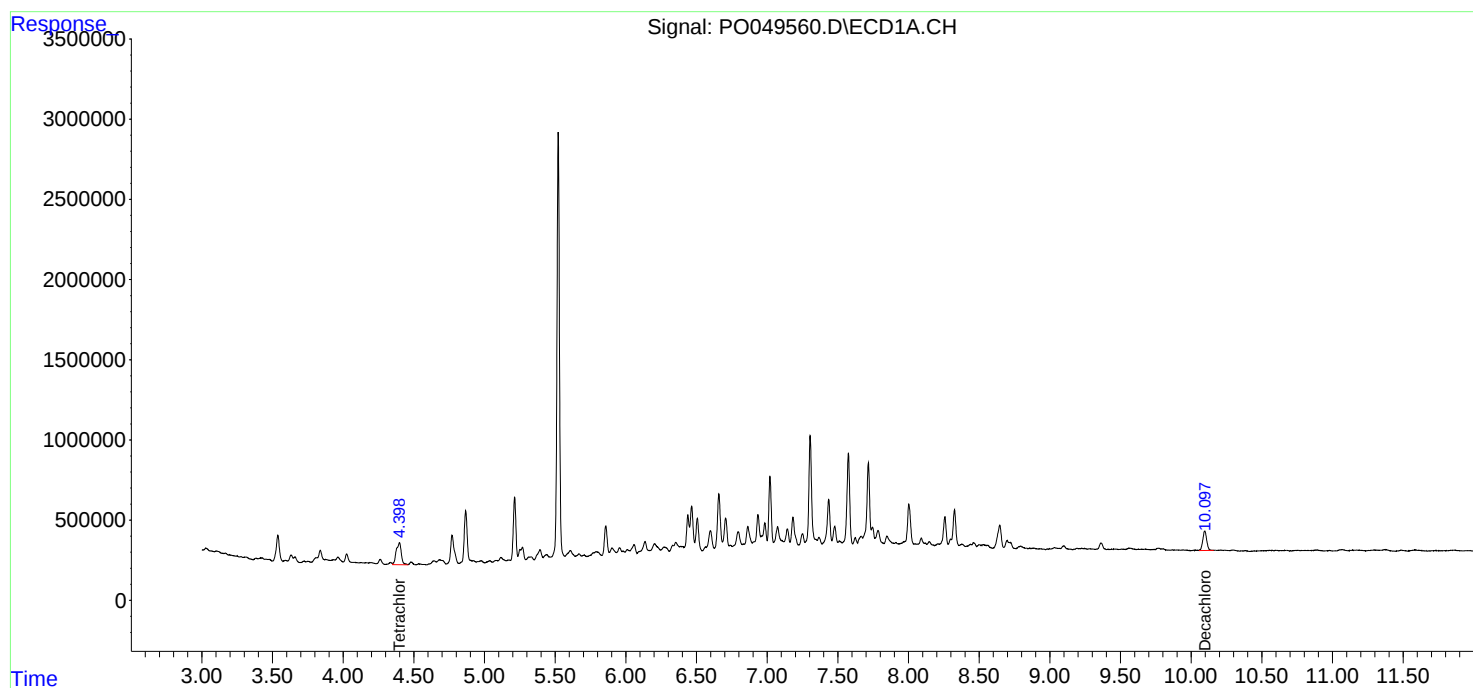


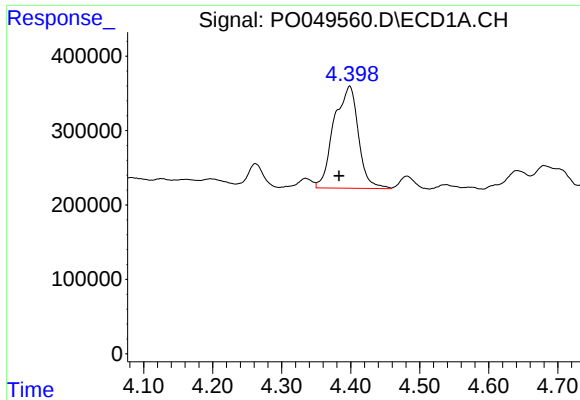

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: 0.016 min
Response: 3376405
Conc: 9.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
4-NW-CARDBOARD-COIL

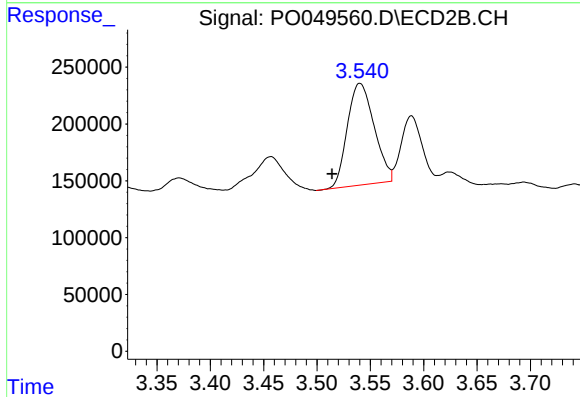


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.026 min
Response: 1563626
Conc: 4.60 ng/ml

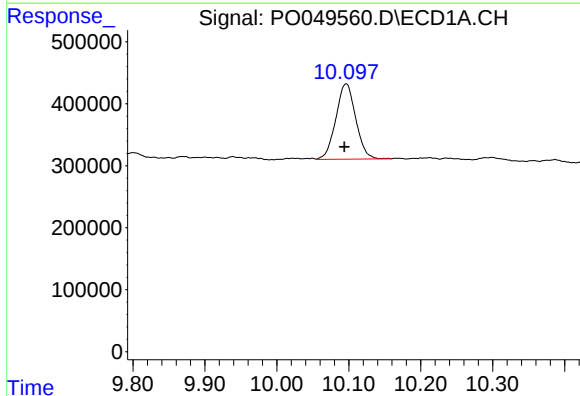

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.002 min
Response: 2338624
Conc: 4.94 ng/ml

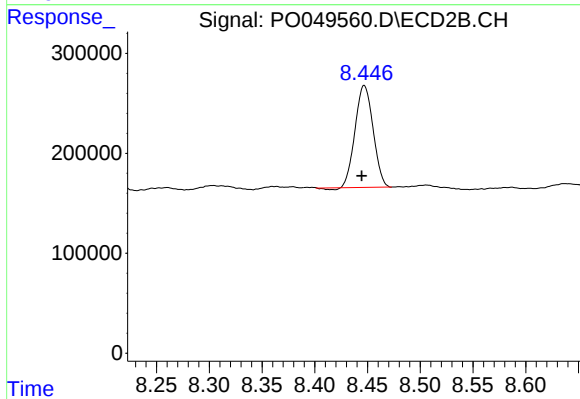

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: 0.002 min
Response: 1209455
Conc: 3.96 ng/ml