

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100220\
 Data File : P0071914.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2020 14:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 15:21:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.514	1706823	885336	19.890	21.496
2)	SA Decachlor...	9.940	8.689	2352225	1226265	20.474	20.174
Target Compounds							
20)	L4 AR-1242-5	6.607	5.610	22441	59198	9.789	47.277 #
24)	L5 AR-1248-4	6.568	0.000	65469	0	16.923	N.D. #
25)	L5 AR-1248-5	6.607	0.000	22441	0	6.226	N.D. #
26)	L6 AR-1254-1	6.537	5.610	474474	59198	129.568	24.996 #
28)	L6 AR-1254-3	7.157f	0.000	58100	0	9.177	N.D. #
29)	L6 AR-1254-4	7.442	0.000	14442	0	2.344	N.D. #
30)	L6 AR-1254-5	7.838f	0.000	34210	0	5.756	N.D. #
43)	L9 AR-1268-3	8.972f	0.000	131619	0	9.990	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100220\
Data File : PO071914.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 14:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 15:21:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

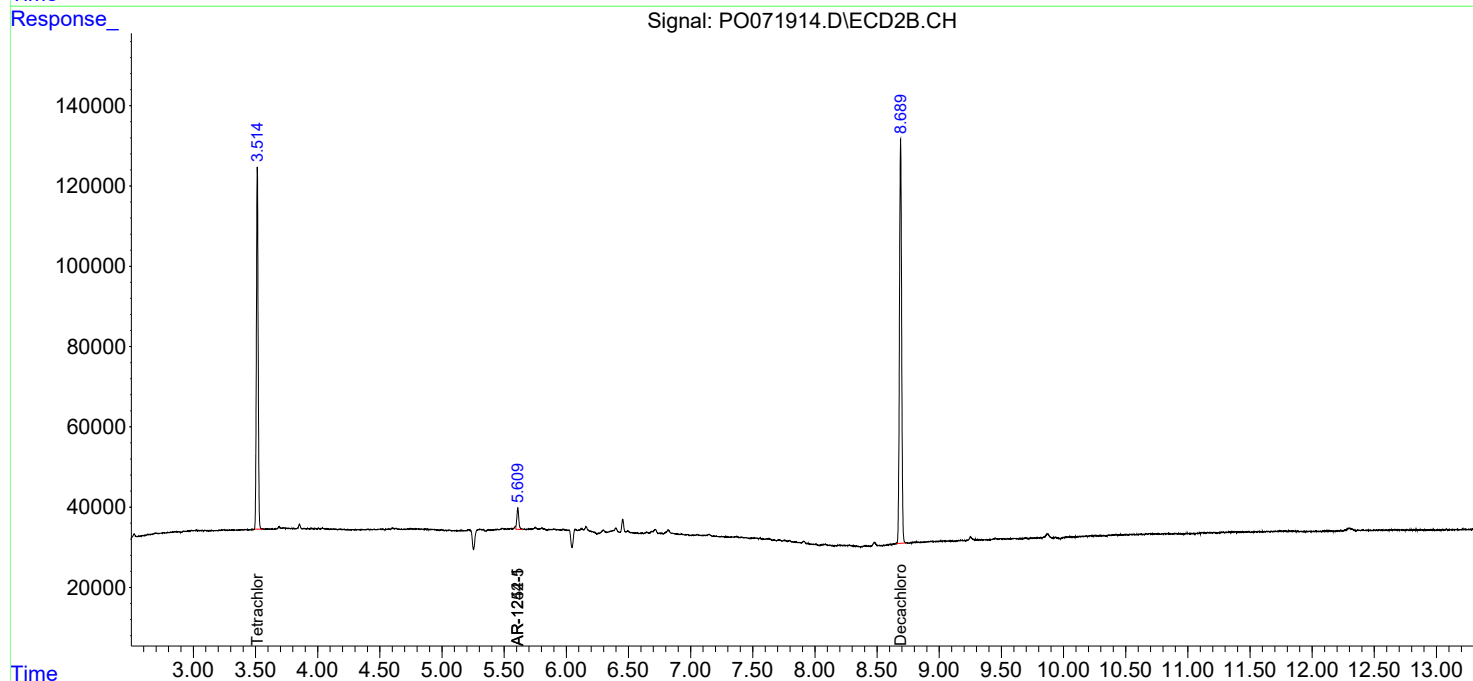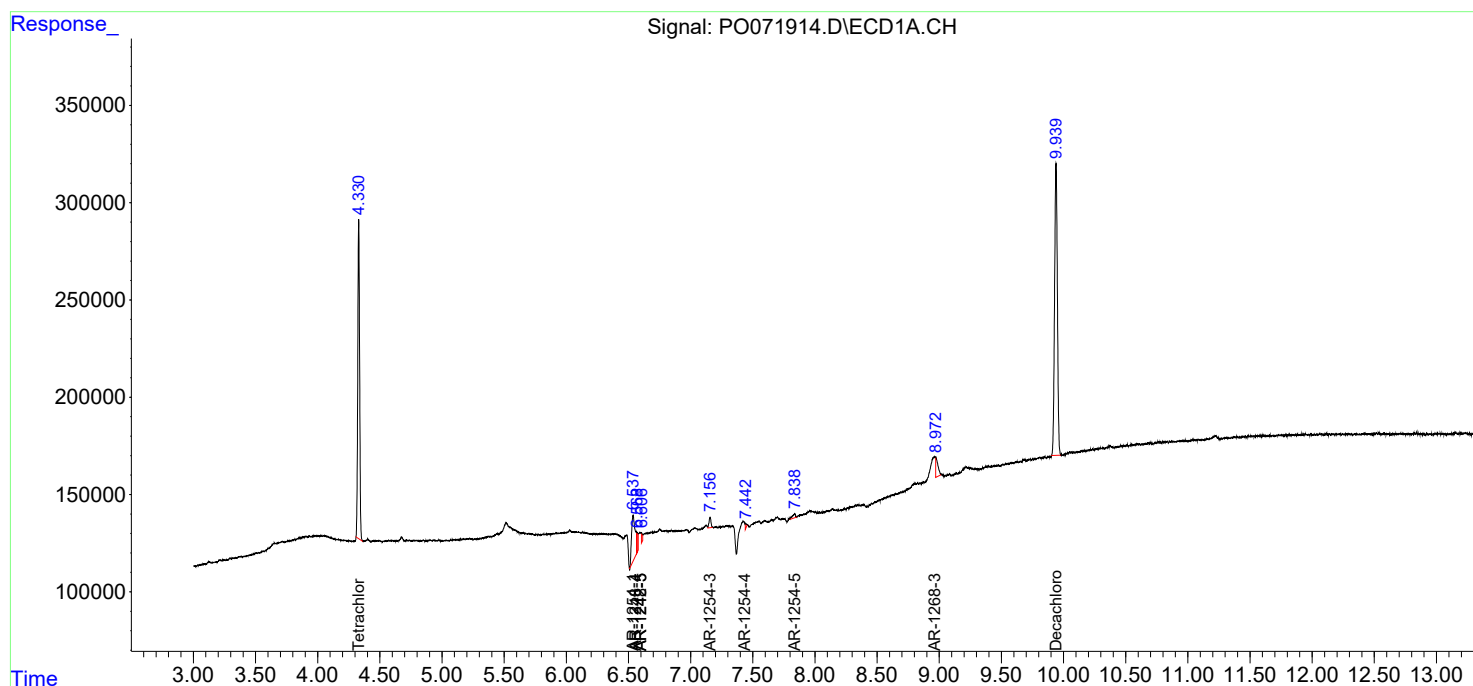


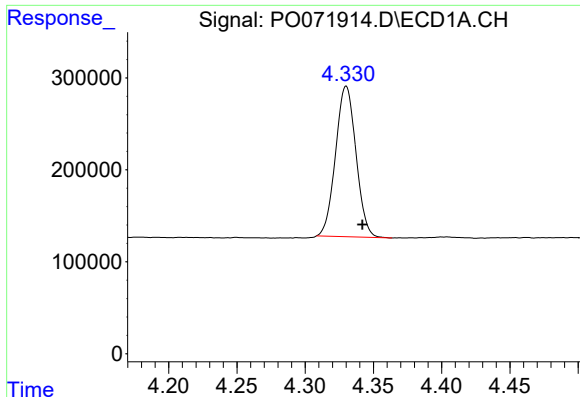

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.012 min
Response: 1706823
Conc: 19.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

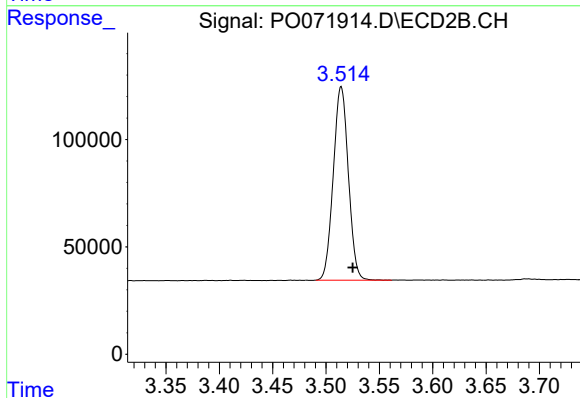


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 885336
Conc: 21.50 ng/ml

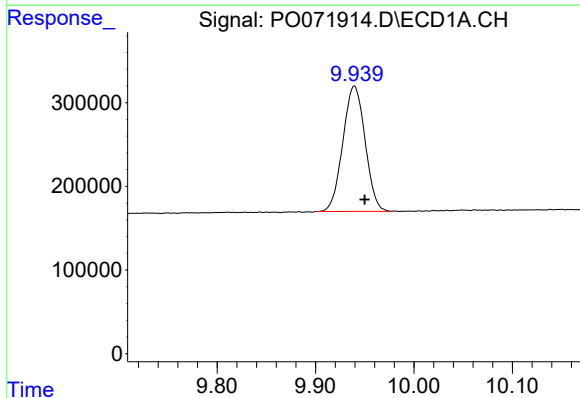


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: -0.010 min
Response: 2352225
Conc: 20.47 ng/ml

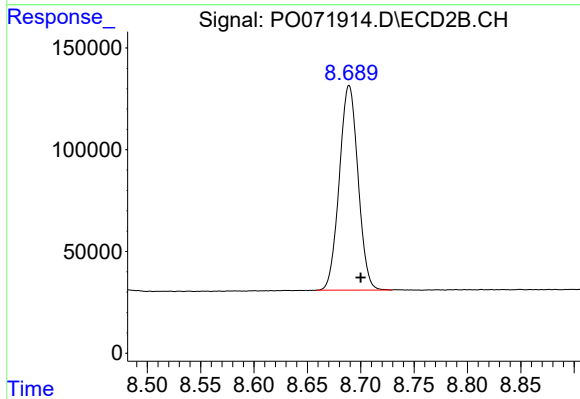

#2 Decachlorobiphenyl


R.T.: 8.689 min
Delta R.T.: -0.011 min
Response: 1226265
Conc: 20.17 ng/ml

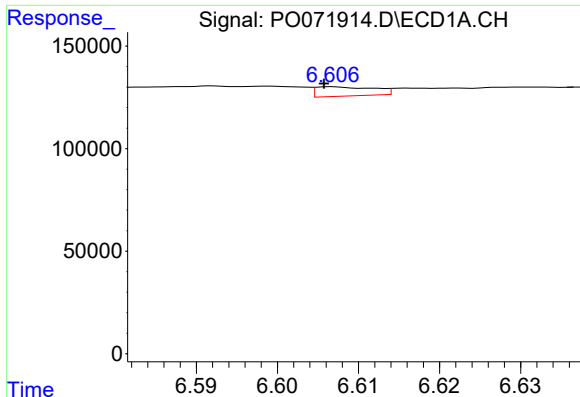

#20 AR-1242-5


R.T.: 6.607 min
Delta R.T.: 0.001 min
Response: 22441
Conc: 9.79 ng/ml

Instrument :
ECD_O
ClientSampleId :

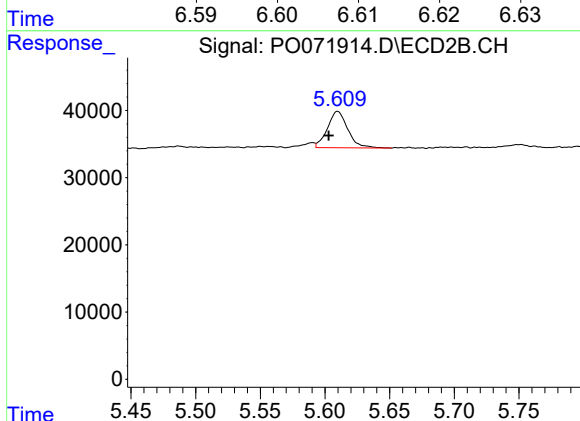


#20 AR-1242-5

R.T.: 5.610 min
Delta R.T.: 0.007 min
Response: 59198
Conc: 47.28 ng/ml

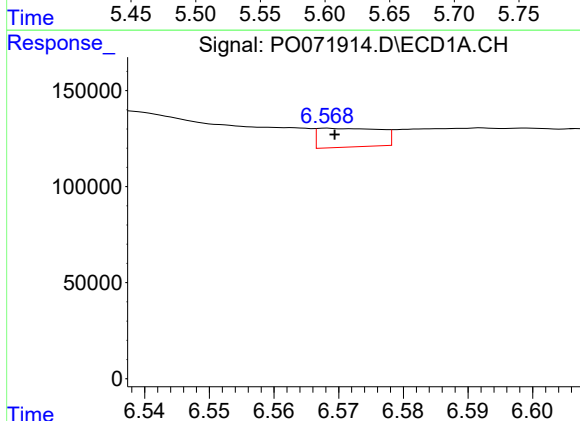


#24 AR-1248-4

R.T.: 6.568 min
Delta R.T.: -0.001 min
Response: 65469
Conc: 16.92 ng/ml

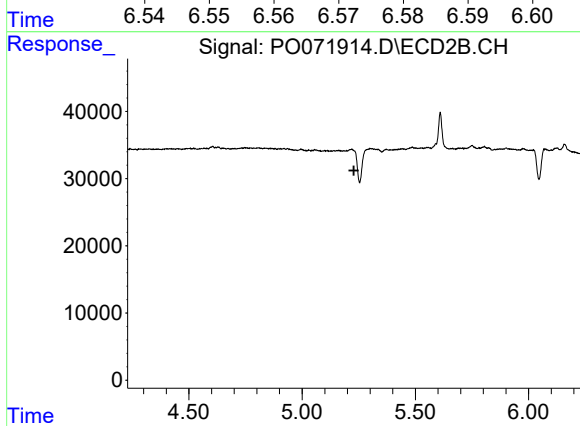

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.228 min
Response: 0
Conc: N.D.

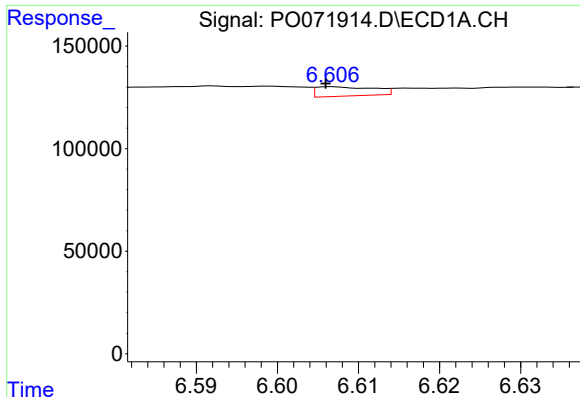

#25 AR-1248-5


R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 22441
Conc: 6.23 ng/ml

Instrument :
ECD_O
ClientSampleId :

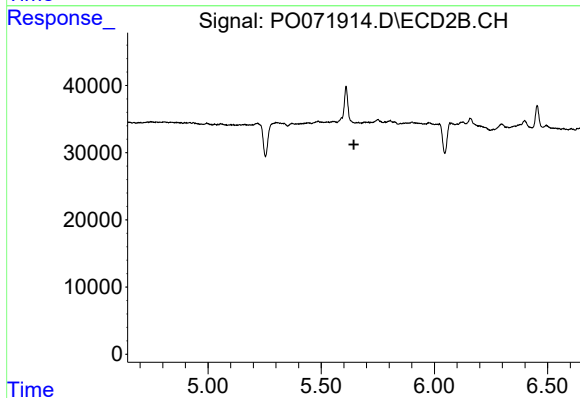


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

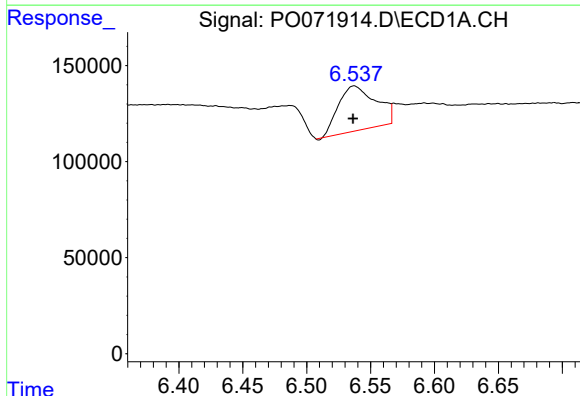


#26 AR-1254-1

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 474474
Conc: 129.57 ng/ml

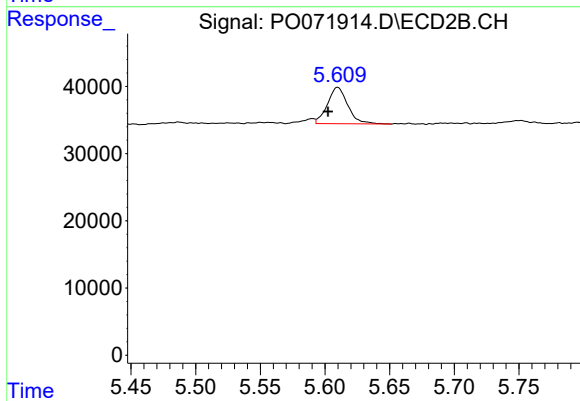

#26 AR-1254-1


R.T.: 5.610 min
Delta R.T.: 0.007 min
Response: 59198
Conc: 25.00 ng/ml

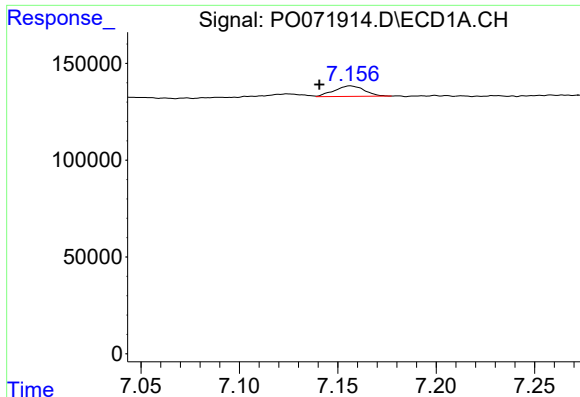

#28 AR-1254-3


R.T.: 7.157 min
Delta R.T.: 0.016 min
Response: 58100
Conc: 9.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

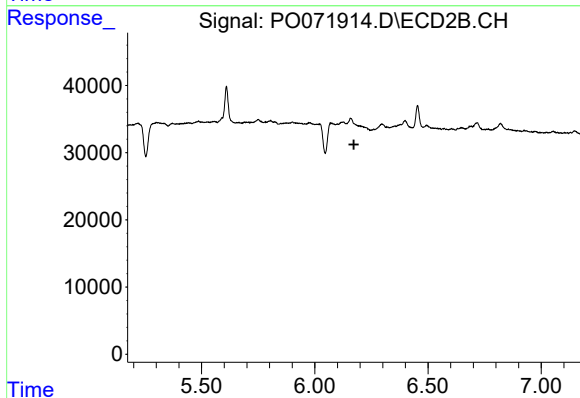


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.173 min
Response: 0
Conc: N.D.

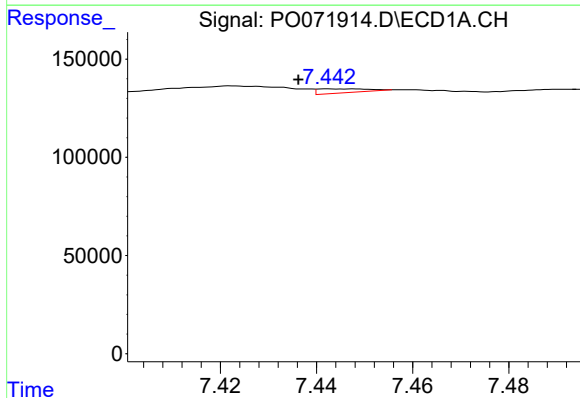


#29 AR-1254-4

R.T.: 7.442 min
Delta R.T.: 0.006 min
Response: 14442
Conc: 2.34 ng/ml

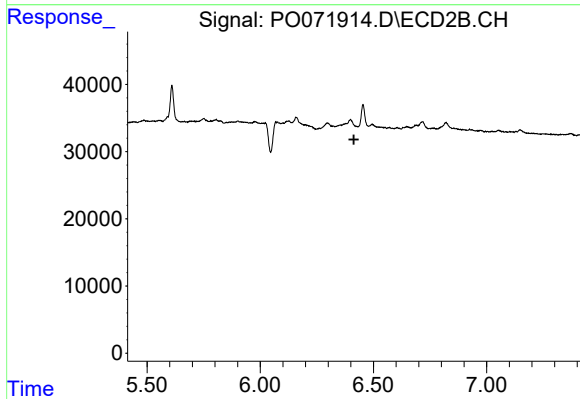

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

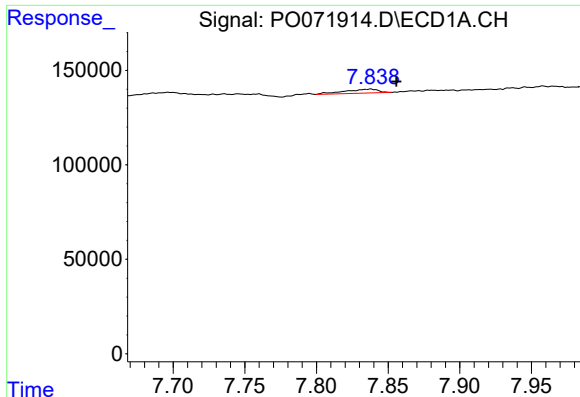

#30 AR-1254-5


R.T.: 7.838 min
Delta R.T.: -0.018 min
Response: 34210
Conc: 5.76 ng/ml

Instrument :
ECD_O
ClientSampleId :

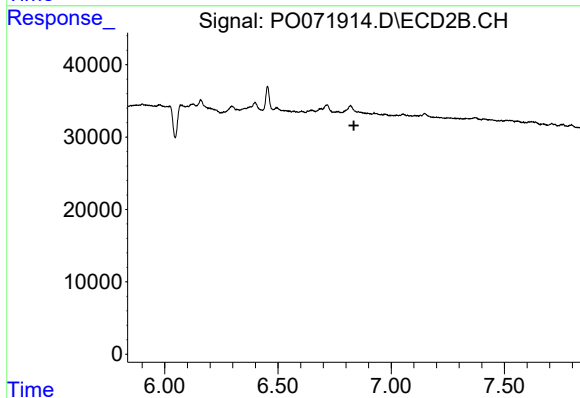


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

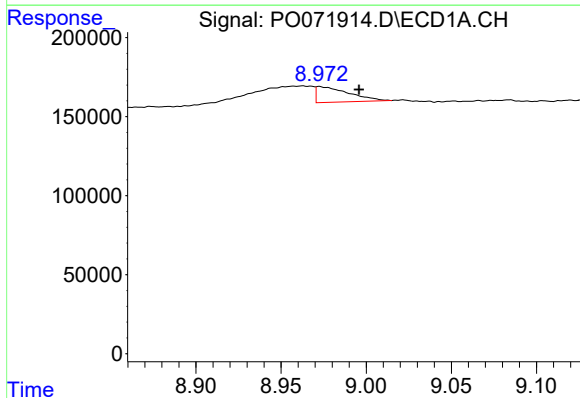

#43 AR-1268-3

R.T.: 8.972 min
Delta R.T.: -0.023 min
Response: 131619
Conc: 9.99 ng/ml

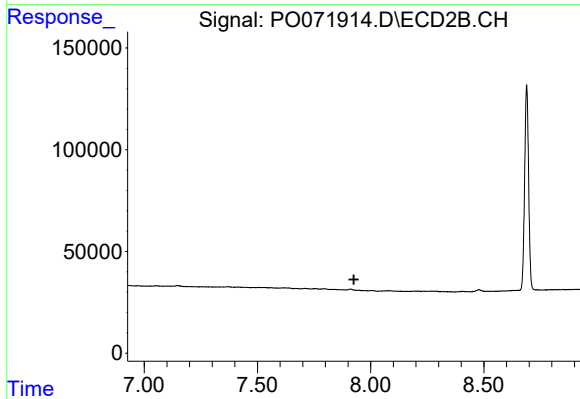

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.926 min
Response: 0
Conc: N.D.