

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100220\
 Data File : PO071913.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2020 14:28
 Operator : DD\AJ
 Sample : L4190-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAV-B18-092920-10-20

Manual Integrations
 APPROVED

Ankita

10/2/2020 5:01:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 02 15:21:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.514	1968022	988881	22.934m	24.010
2) SA Decachlor...	9.940	8.690	2323559	1190329	20.225	19.583

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100220\
Data File : P0071913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 14:28
Operator : DD\AJ
Sample : L4190-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PAV-B18-092920-10-20



Manual Integrations
APPROVED


Ankita

10/2/2020 5:01:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 02 15:21:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

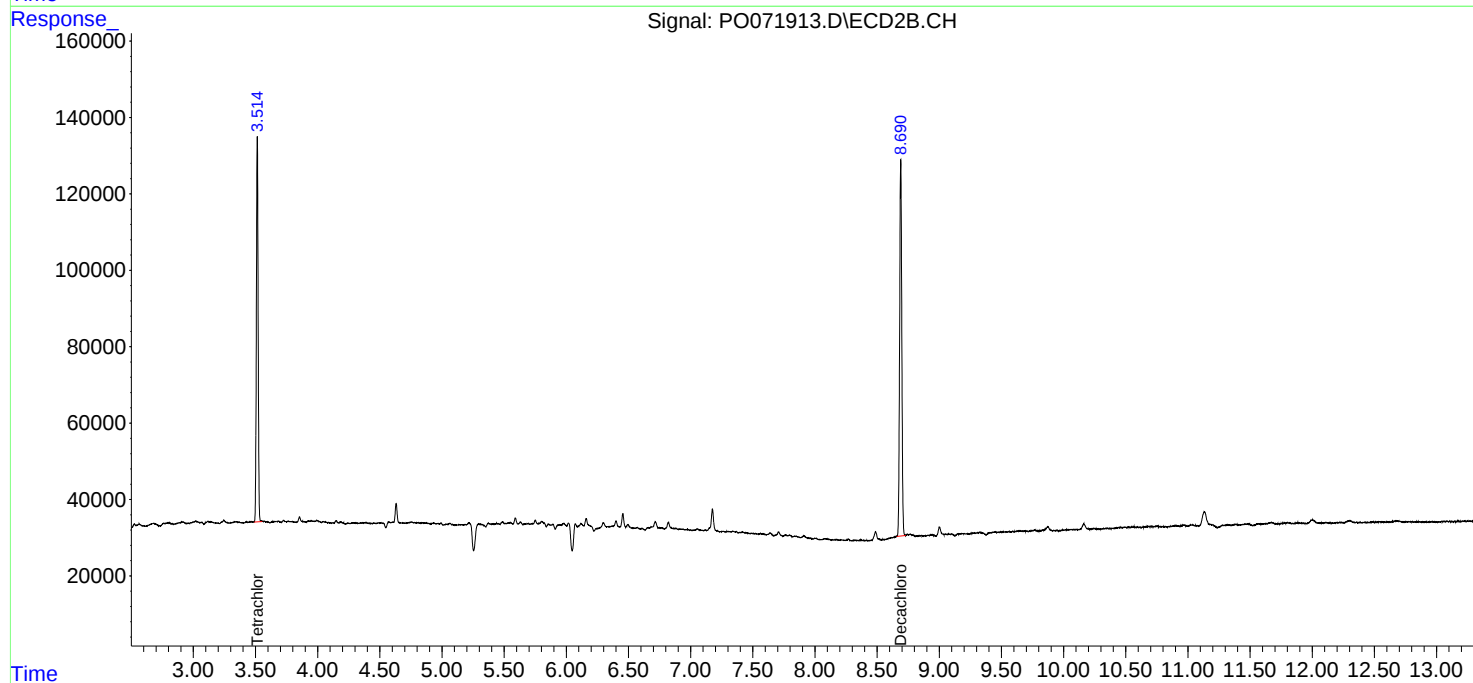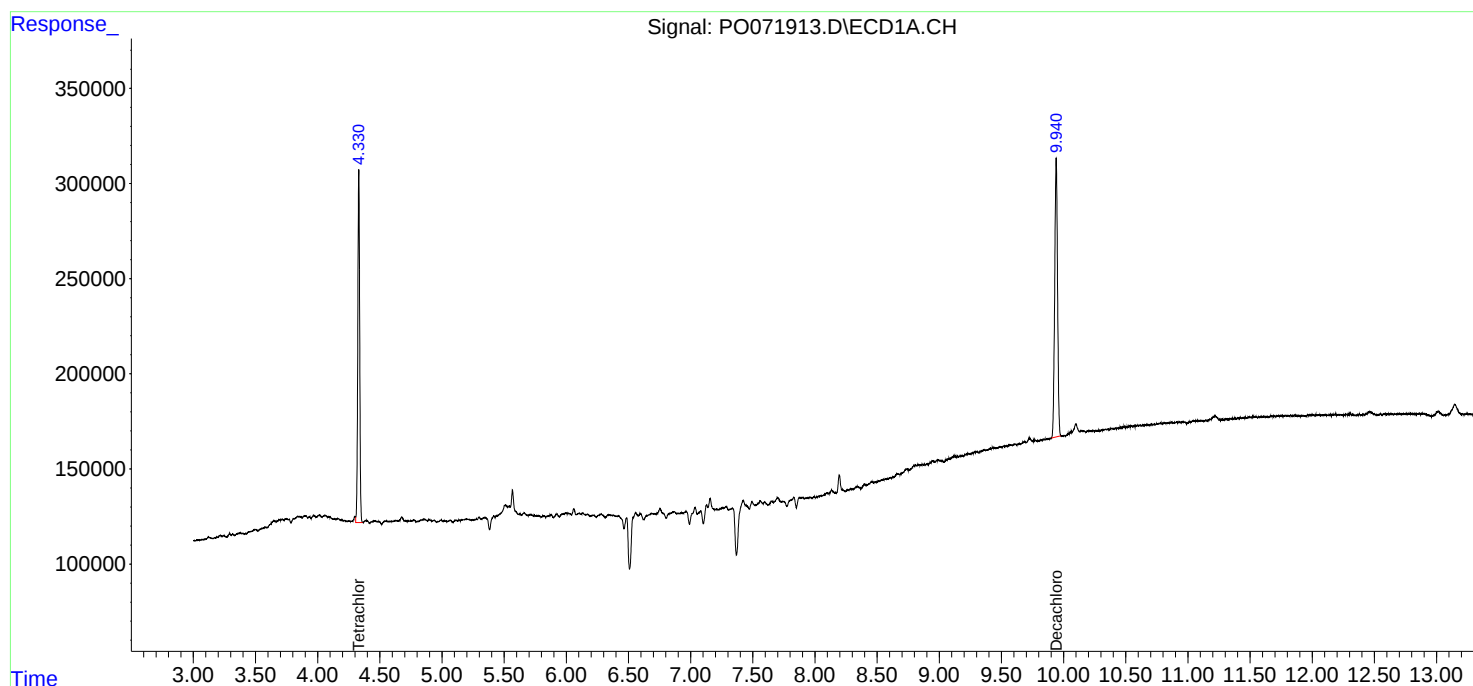

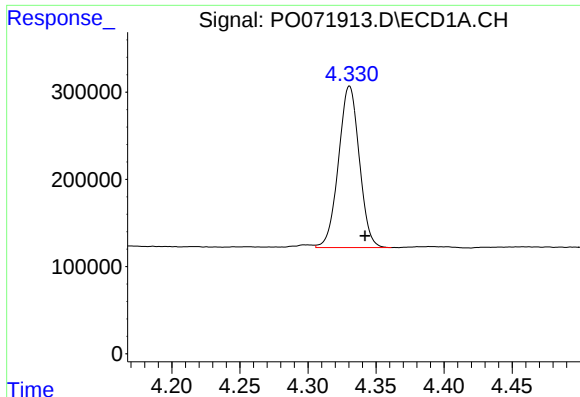

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.012 min
Response: 1968022
Conc: 22.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAV-B18-092920-10-20

Manual Integrations
APPROVED


Ankita

10/2/2020 5:01:25 PM

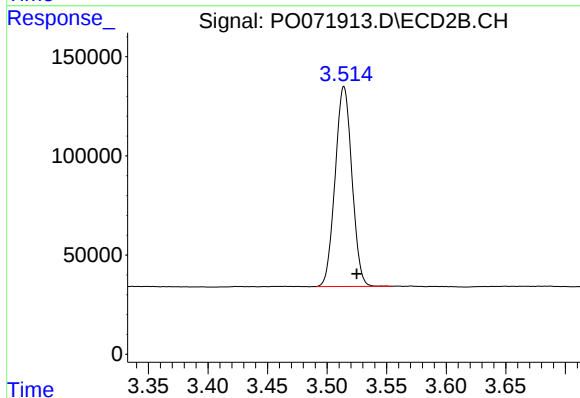


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 988881
Conc: 24.01 ng/ml

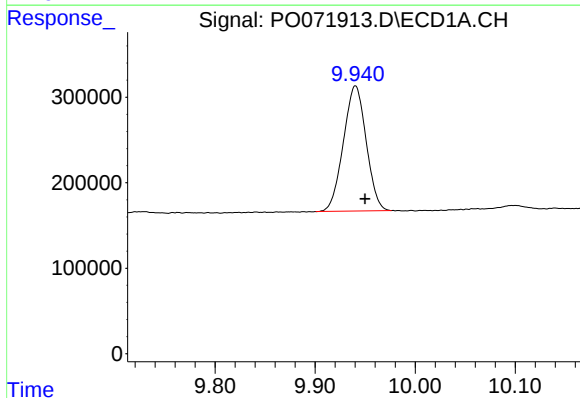

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: -0.010 min
Response: 2323559
Conc: 20.22 ng/ml

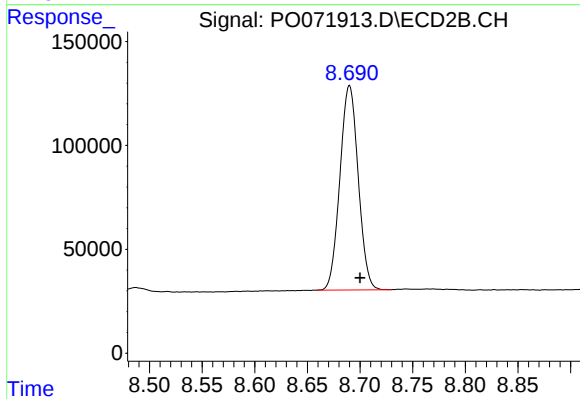

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.010 min
Response: 1190329
Conc: 19.58 ng/ml