

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
 Data File : PO071935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Oct 2020 22:32
 Operator : DD\AJ
 Sample : L3865-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-08-093020

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:35:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:22:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 03 04:09:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.511	1564410	823406	21.781	21.983
2) SA Decachlor...	9.933	8.685	2004186	1016414	18.202	17.870

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : PO071935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 22:32
Operator : DD\AJ
Sample : L3865-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-08-093020


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:22:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

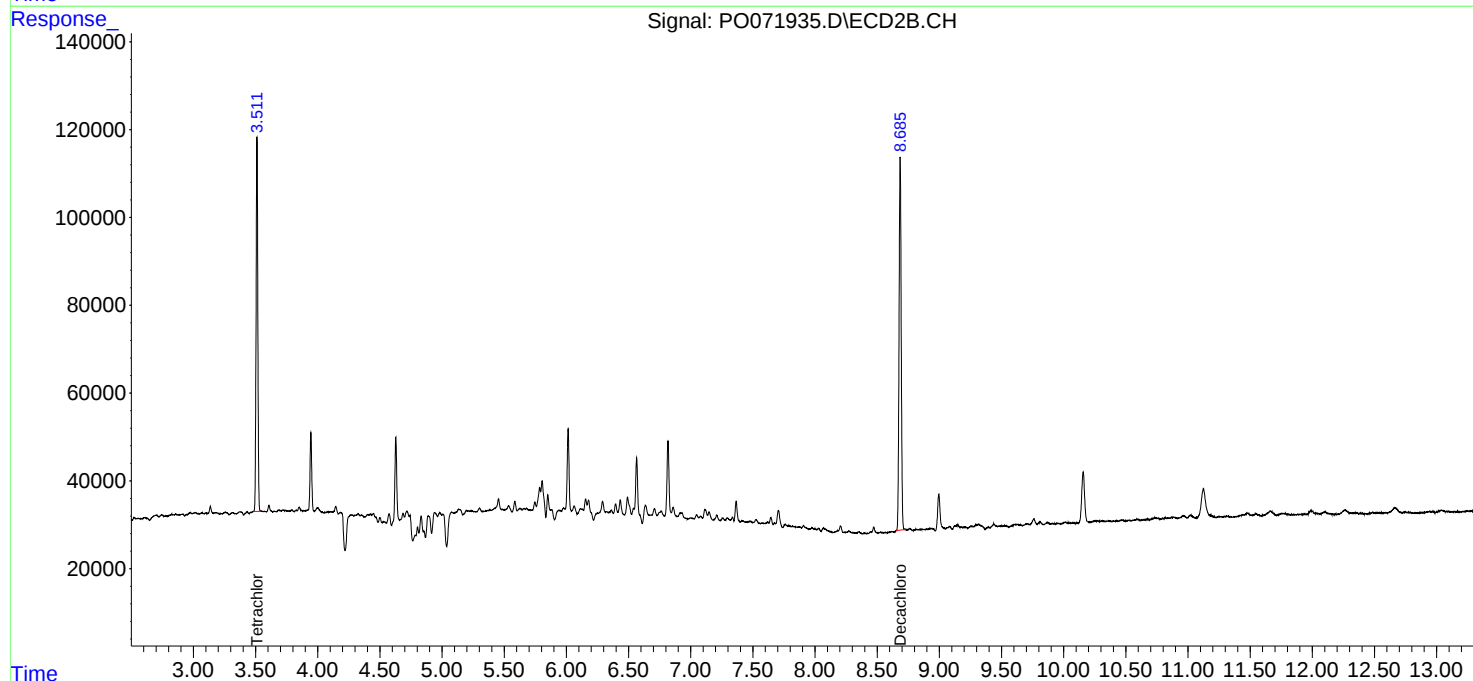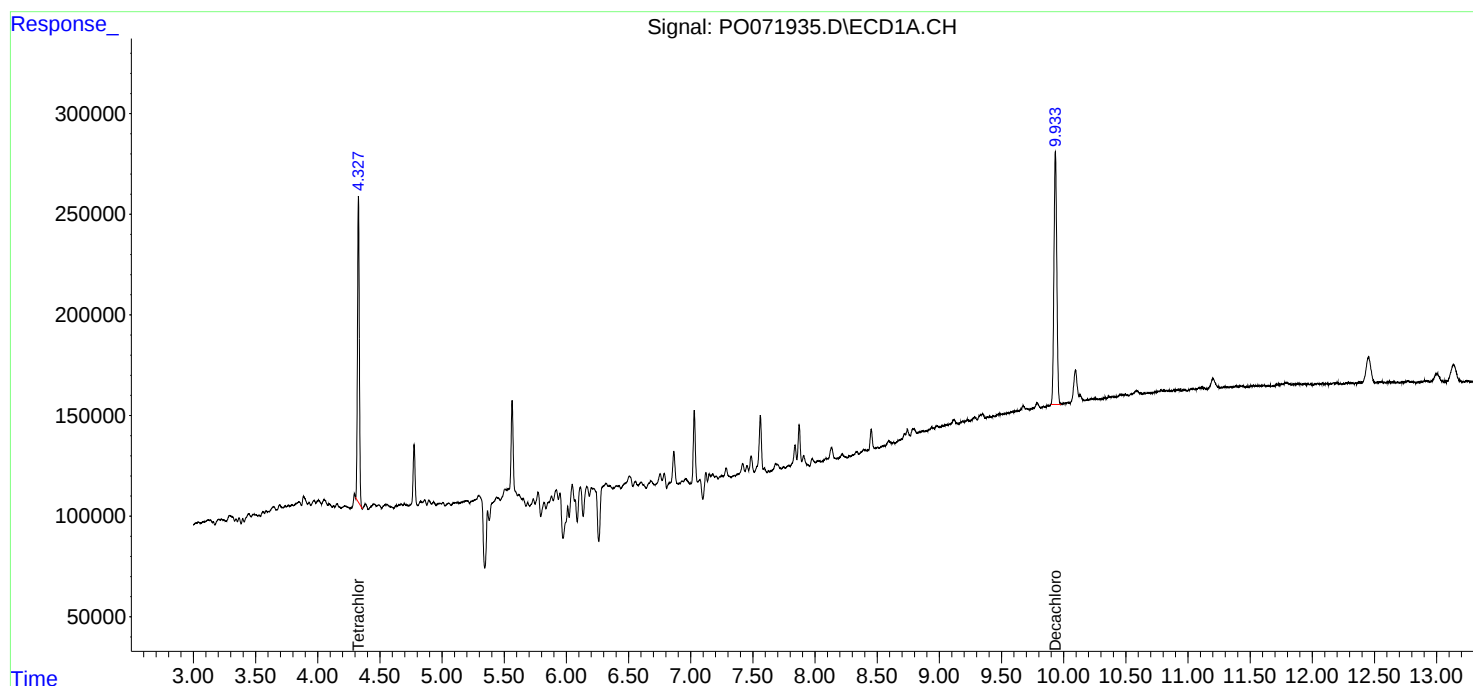

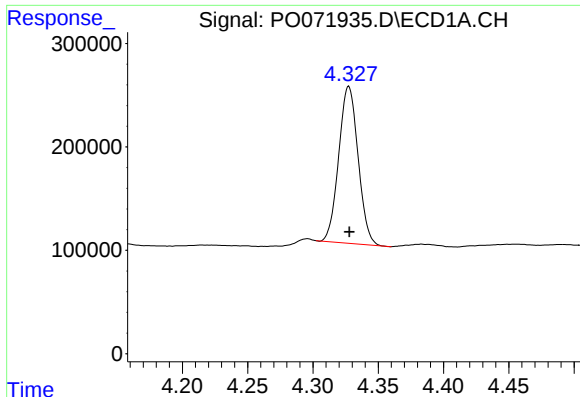


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 1564410
Conc: 21.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-08-093020


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:18 PM

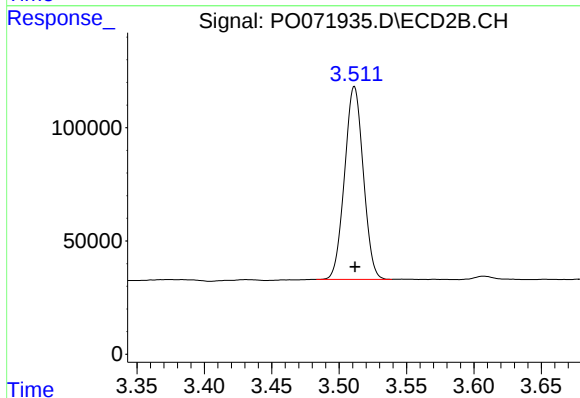


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 823406
Conc: 21.98 ng/ml

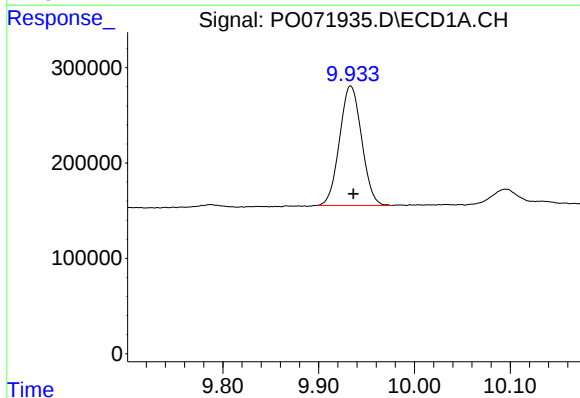

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.003 min
Response: 2004186
Conc: 18.20 ng/ml

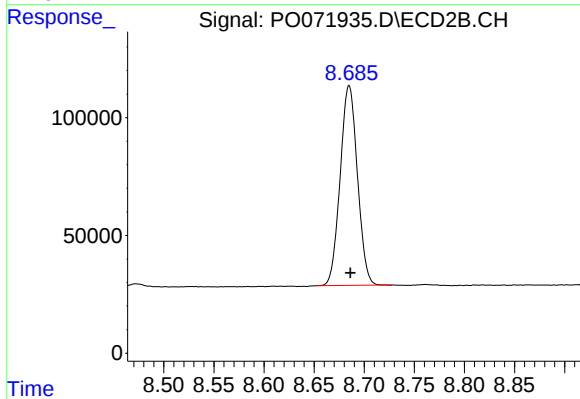

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.001 min
Response: 1016414
Conc: 17.87 ng/ml