

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : PO071936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 22:49
Operator : DD\AJ
Sample : L3865-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NB-07-093020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:22:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.511	1611865	847092	22.441	22.616
2) SA Decachlor...	9.935	8.686	1875831	940653	17.036	16.538

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : P0071936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Oct 2020 22:49
Operator : DD\AJ
Sample : L3865-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NB-07-093020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:22:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

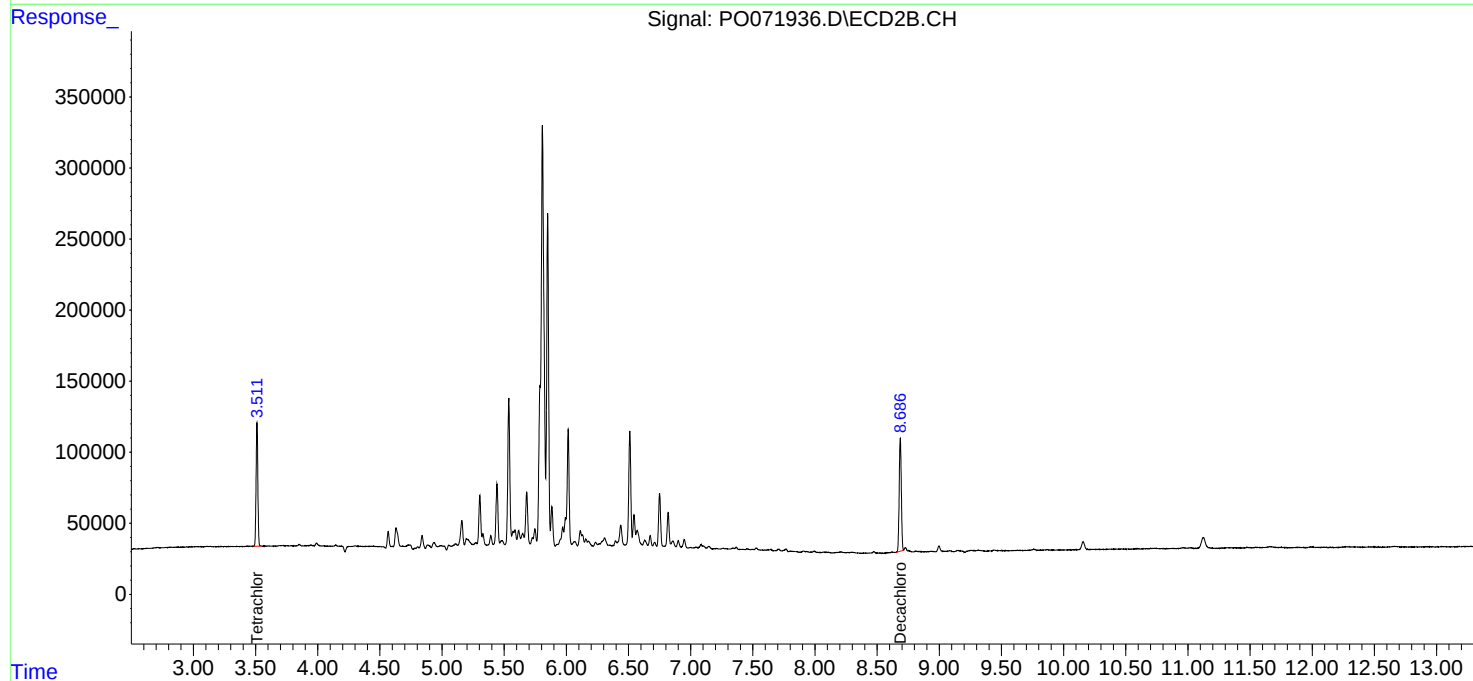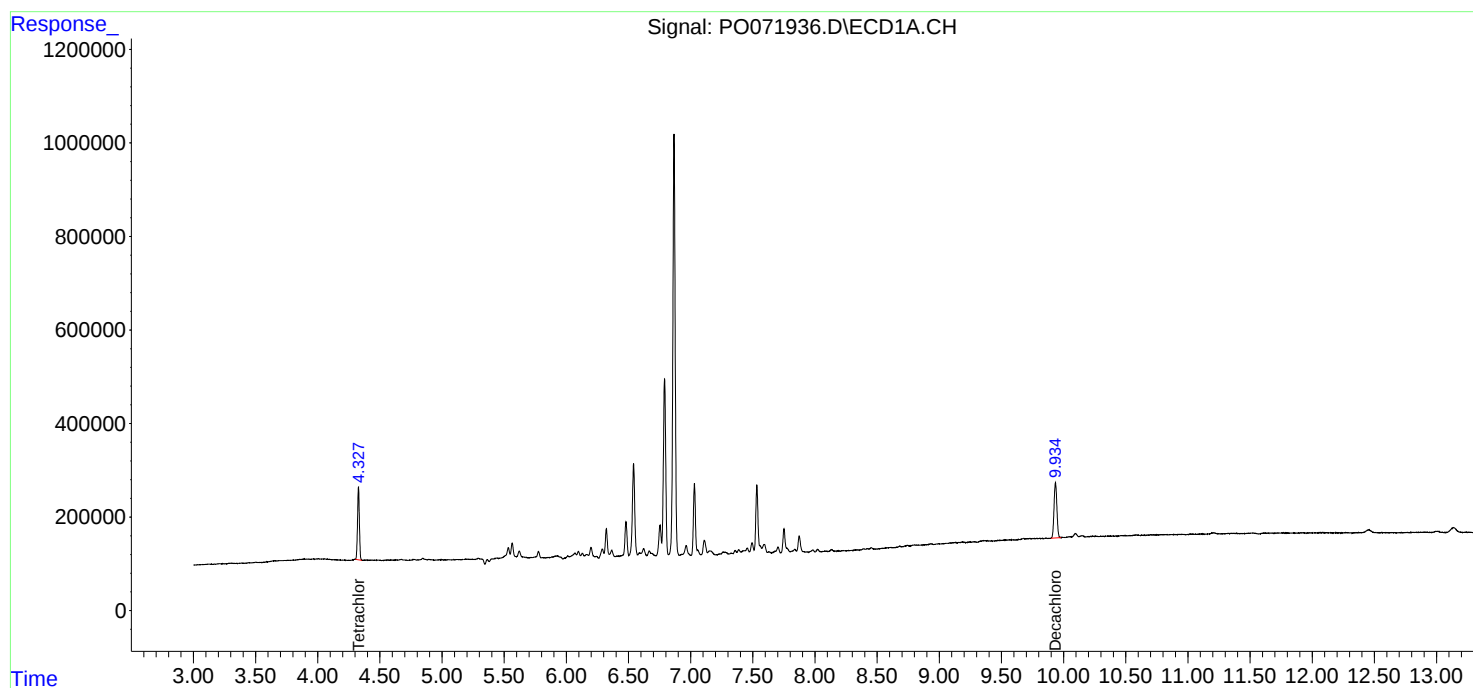


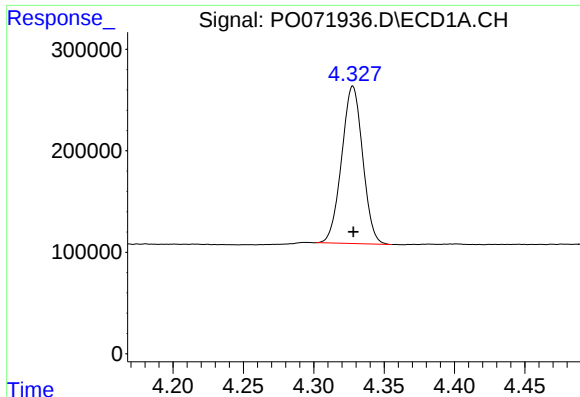

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 1611865
Conc: 22.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-07-093020

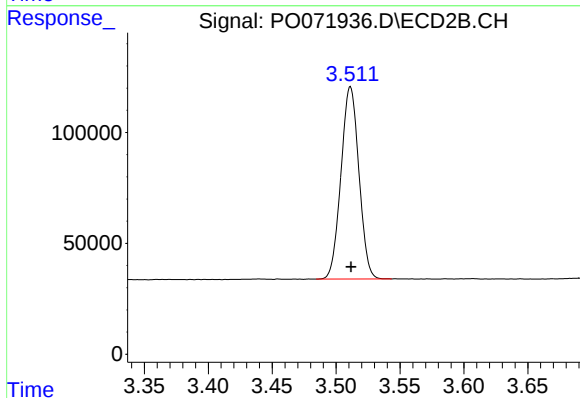


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 847092
Conc: 22.62 ng/ml

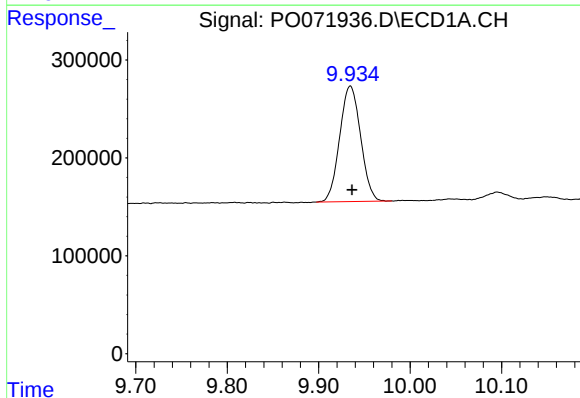

#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.002 min
Response: 1875831
Conc: 17.04 ng/ml

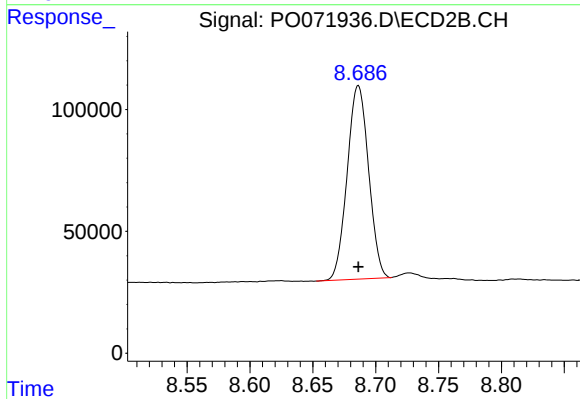

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 940653
Conc: 16.54 ng/ml