

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
 Data File : PO071942.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2020 00:32
 Operator : DD\AJ
 Sample : L4219-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-100120

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:35:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:25:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 03 04:09:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.511	1740318	800645	24.230m	21.376
2) SA Decachlor...	9.933	8.684	2121645	1024677	19.269	18.015
Target Compounds						
26) L6 AR-1254-1	6.520	5.585	571546	431918	177.035m	191.424m
27) L6 AR-1254-2	6.749	5.747	1161194	408577	218.621m	204.589m
28) L6 AR-1254-3	7.126	6.156	1287874	691131	229.436m	214.462
29) L6 AR-1254-4	7.420	6.396	1284136	550416	237.429m	240.149
30) L6 AR-1254-5	7.841	6.817	1151399	790925	217.109m	247.561

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : PO071942.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2020 00:32
Operator : DD\AJ
Sample : L4219-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:25:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

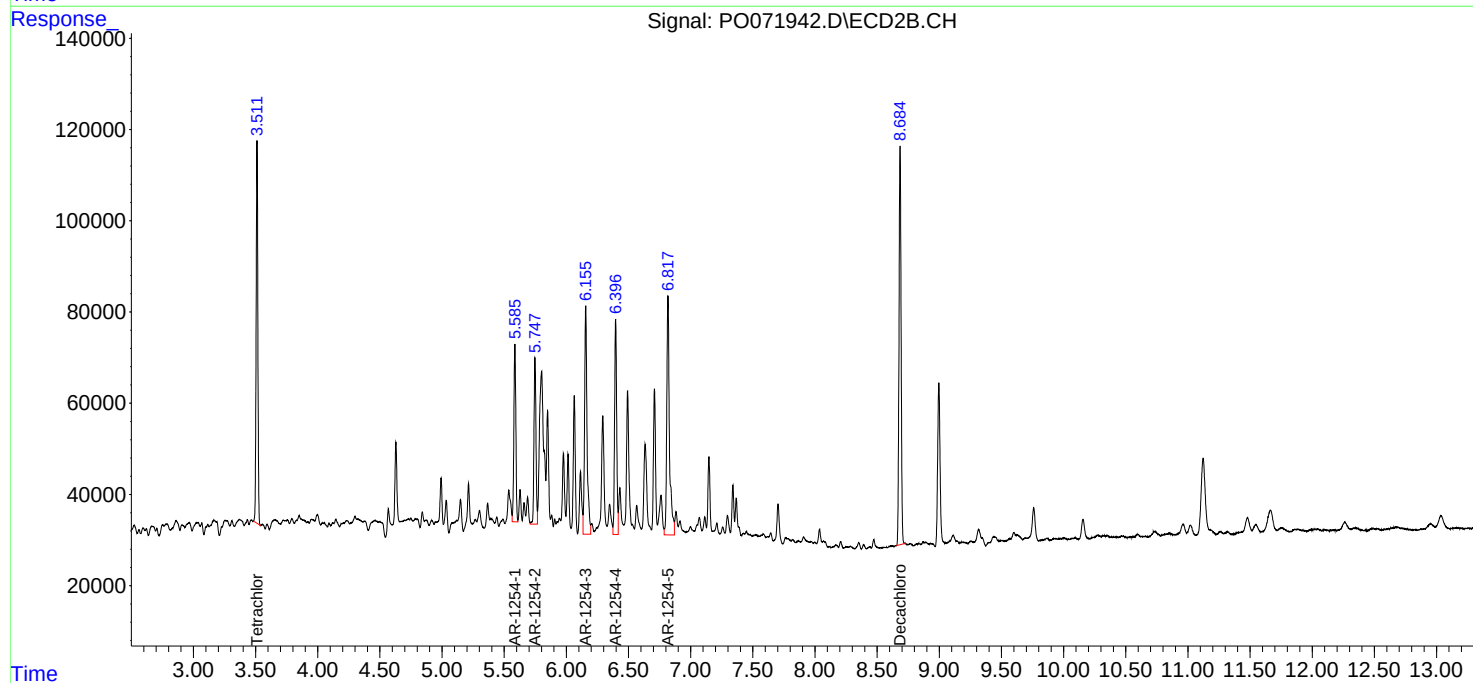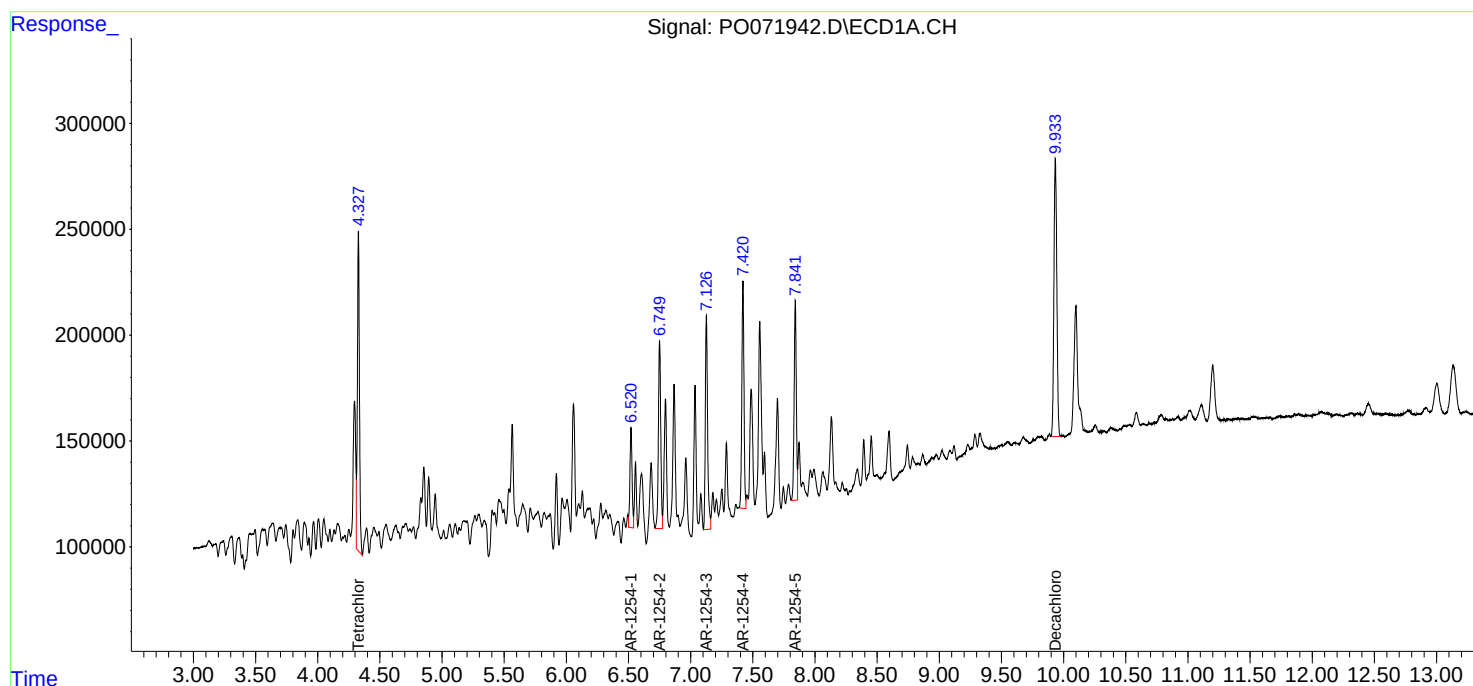

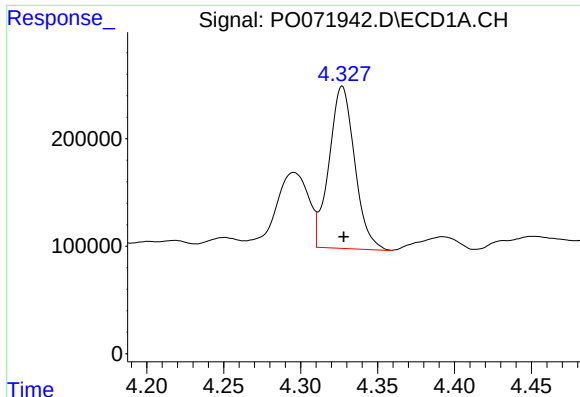


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: -0.001 min
Response: 1740318
Conc: 24.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:24 PM

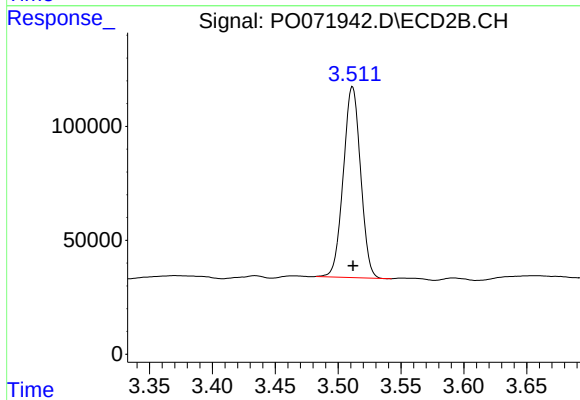


#1 Tetrachloro-m-xylene

R.T.: 3.511 min
Delta R.T.: 0.000 min
Response: 800645
Conc: 21.38 ng/ml

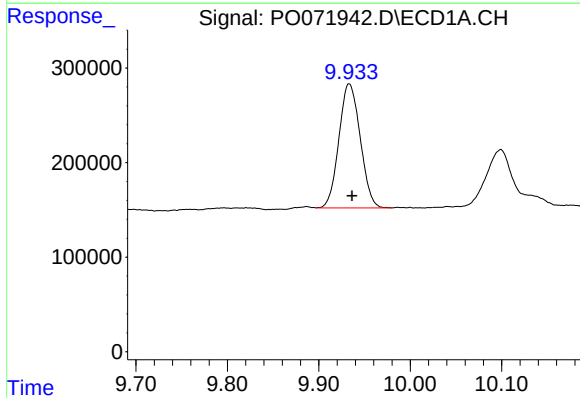


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.003 min
Response: 2121645
Conc: 19.27 ng/ml

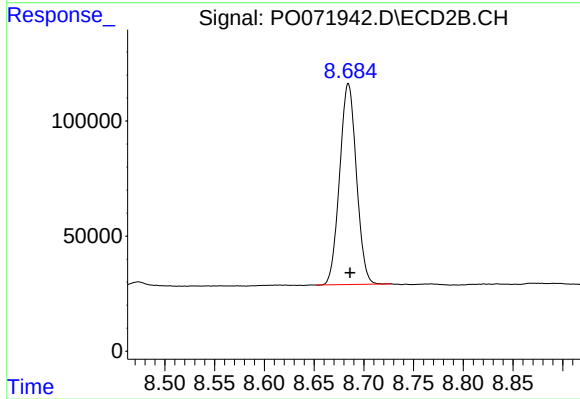

#2 Decachlorobiphenyl

R.T.: 8.684 min
Delta R.T.: -0.002 min
Response: 1024677
Conc: 18.01 ng/ml

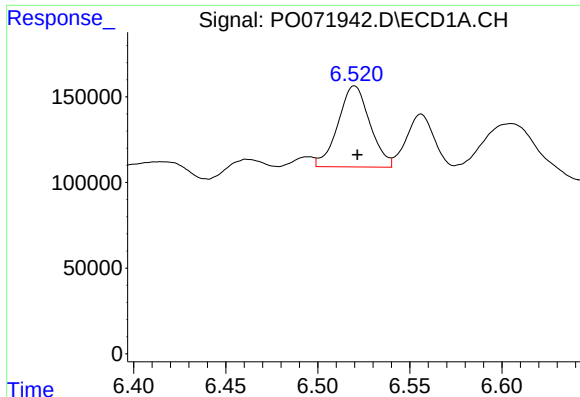


#26 AR-1254-1

R.T.: 6.520 min
Delta R.T.: -0.002 min
Response: 571546
Conc: 177.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:24 PM

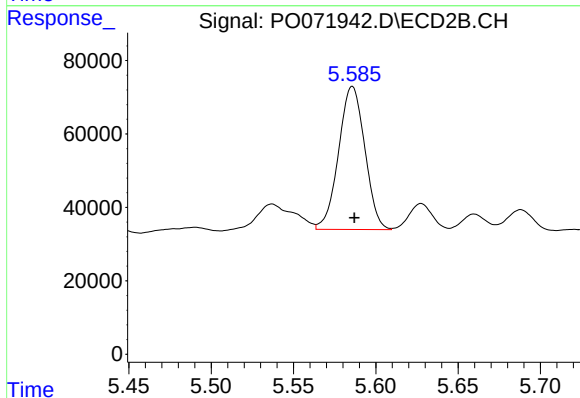


#26 AR-1254-1

R.T.: 5.585 min
Delta R.T.: -0.002 min
Response: 431918
Conc: 191.42 ng/ml m

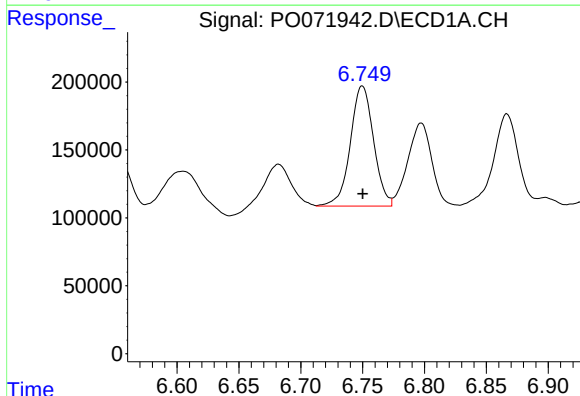


#27 AR-1254-2

R.T.: 6.749 min
Delta R.T.: 0.000 min
Response: 1161194
Conc: 218.62 ng/ml m

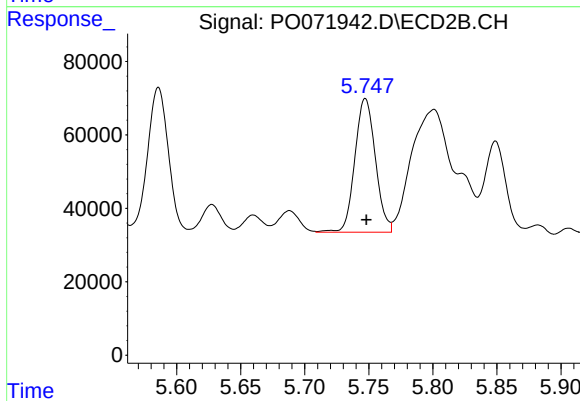

#27 AR-1254-2

R.T.: 5.747 min
Delta R.T.: -0.001 min
Response: 408577
Conc: 204.59 ng/ml m

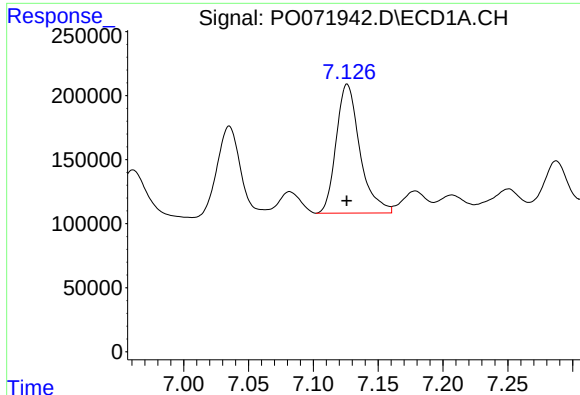


#28 AR-1254-3

R.T.: 7.126 min
Delta R.T.: 0.000 min
Response: 1287874
Conc: 229.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:24 PM

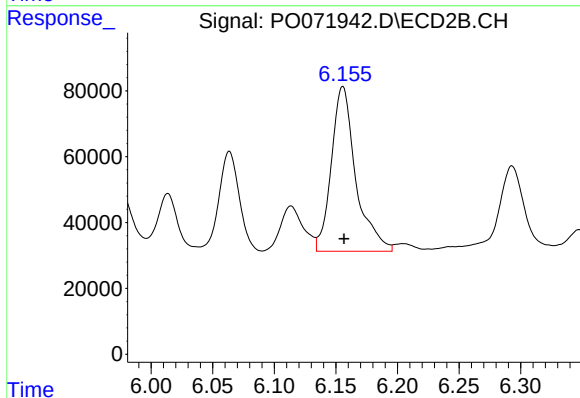


#28 AR-1254-3

R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 691131
Conc: 214.46 ng/ml

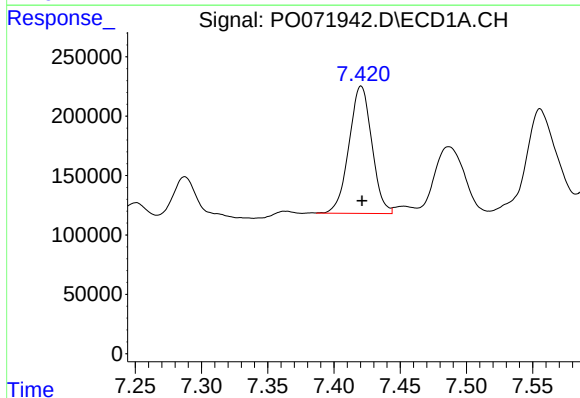


#29 AR-1254-4

R.T.: 7.420 min
Delta R.T.: -0.001 min
Response: 1284136
Conc: 237.43 ng/ml m

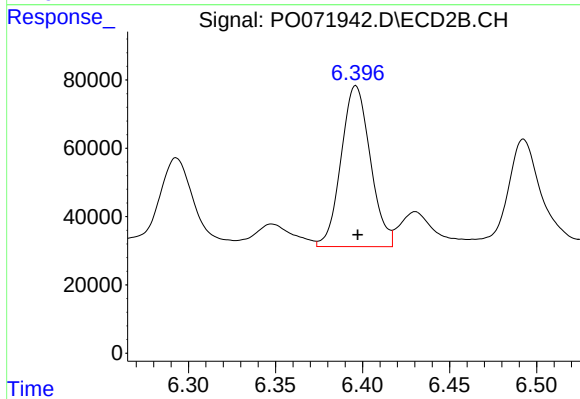

#29 AR-1254-4

R.T.: 6.396 min
Delta R.T.: -0.001 min
Response: 550416
Conc: 240.15 ng/ml

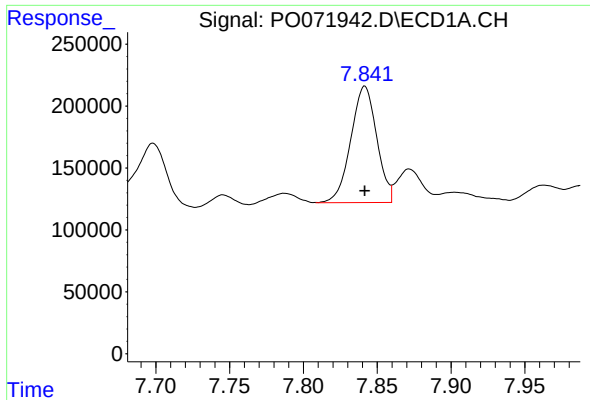


#30 AR-1254-5

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 1151399
Conc: 217.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-100120

Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:24 PM

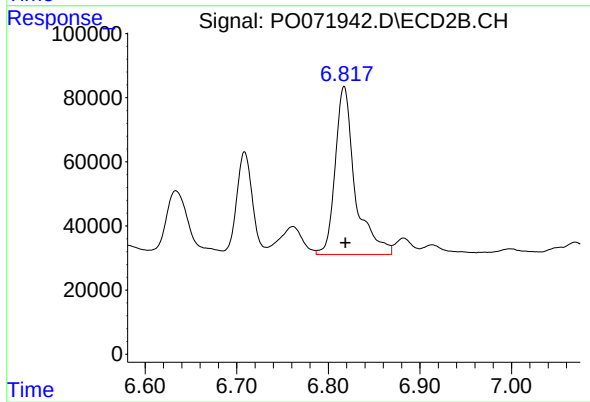

#30 AR-1254-5

R.T.: 6.817 min
Delta R.T.: -0.001 min
Response: 790925
Conc: 247.56 ng/ml