

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
 Data File : PO071943.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2020 00:49
 Operator : DD\AJ
 Sample : L4221-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-100120

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:35:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 04:25:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 03 04:09:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.512	1709428	903036	23.800	24.109
2) SA Decachlor...	9.933	8.686	2094293	1005840	19.021	17.684
Target Compounds						
26) L6 AR-1254-1	6.521	5.586	49195	47641	15.238m	21.114 #
27) L6 AR-1254-2	6.752	5.748	98989	35478	18.637	17.765
28) L6 AR-1254-3	7.126	6.155	145805	63879	25.975	19.822m
29) L6 AR-1254-4	7.422	6.397	122871	31011	22.718	13.530 #
30) L6 AR-1254-5	7.839	6.817	142605	100307	26.890	31.396

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : PO071943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2020 00:49
Operator : DD\AJ
Sample : L4221-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 04:25:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

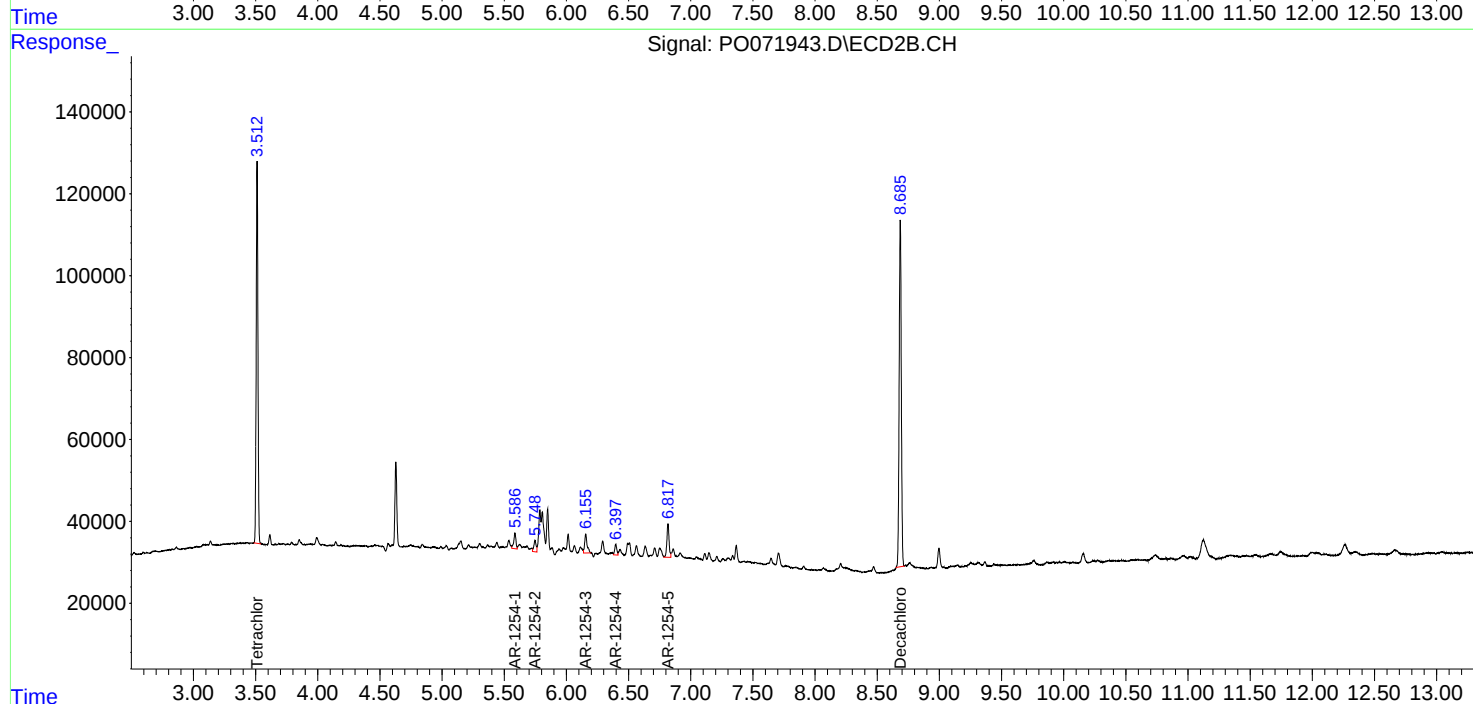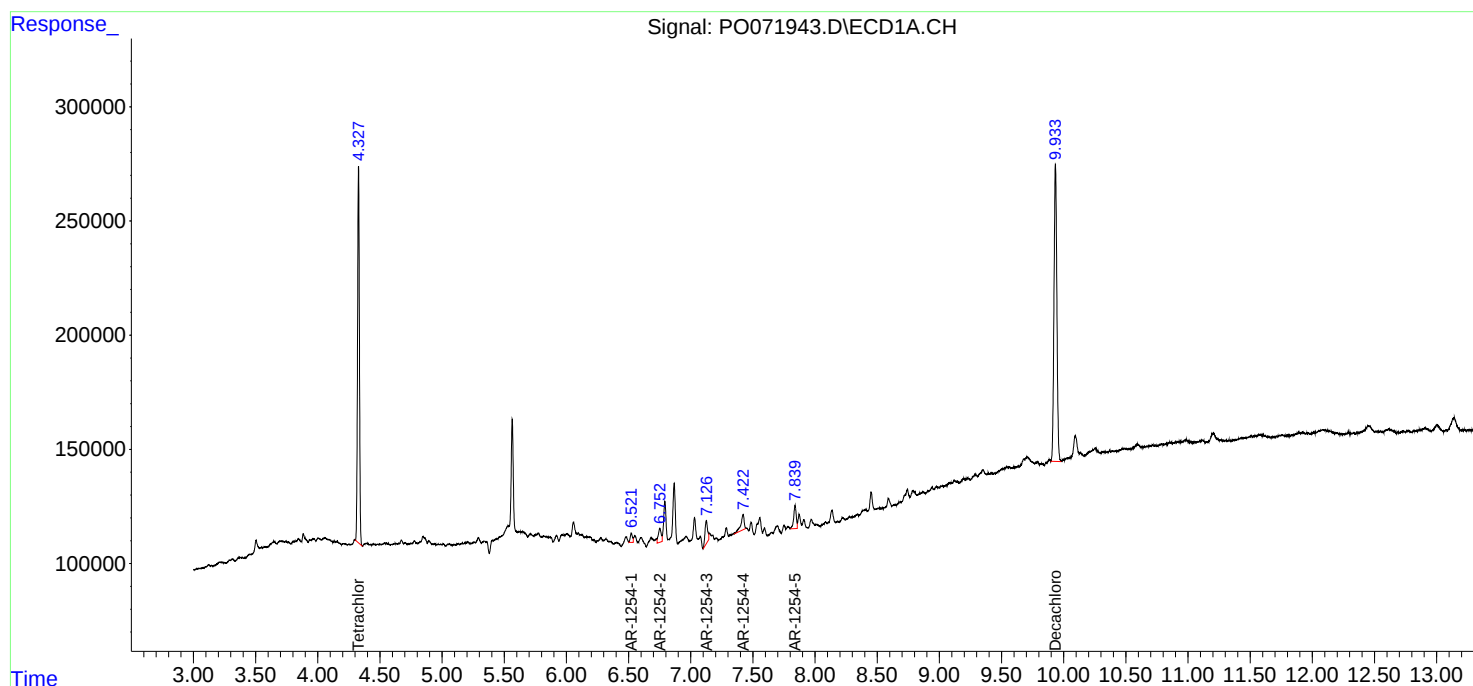

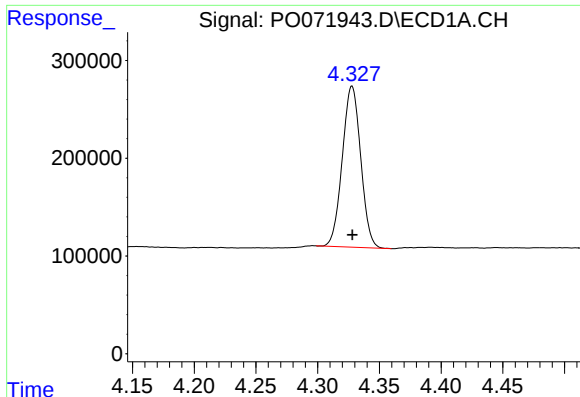


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 1709428
Conc: 23.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:26 PM

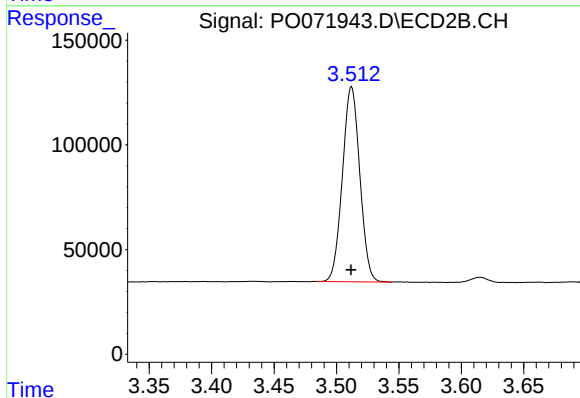


#1 Tetrachloro-m-xylene

R.T.: 3.512 min
Delta R.T.: 0.000 min
Response: 903036
Conc: 24.11 ng/ml

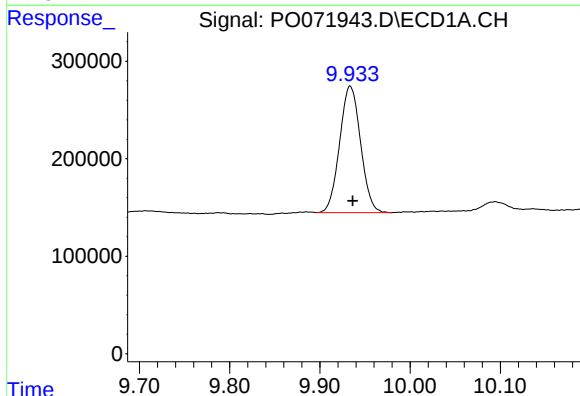


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.003 min
Response: 2094293
Conc: 19.02 ng/ml

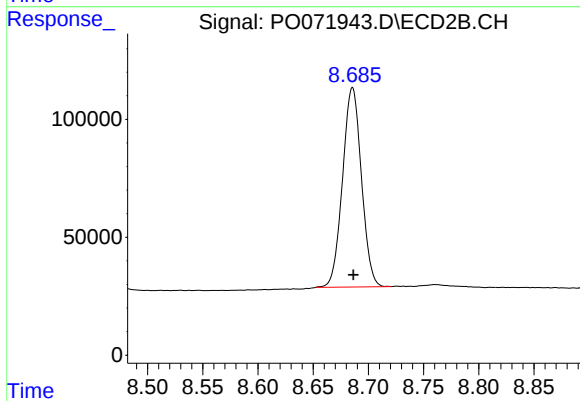

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 1005840
Conc: 17.68 ng/ml

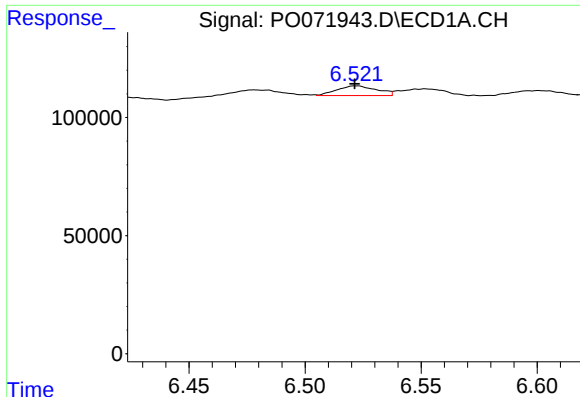


#26 AR-1254-1

R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 49195
Conc: 15.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-02-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:26 PM

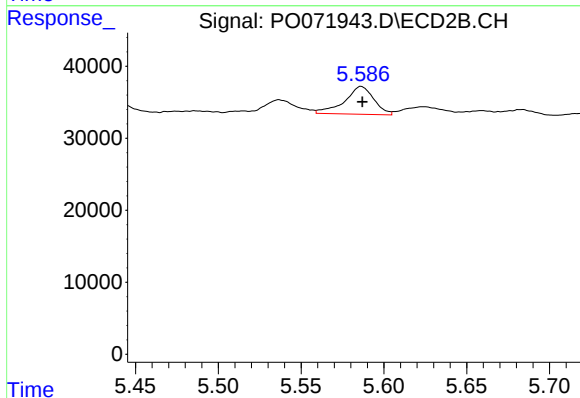


#26 AR-1254-1

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 47641
Conc: 21.11 ng/ml

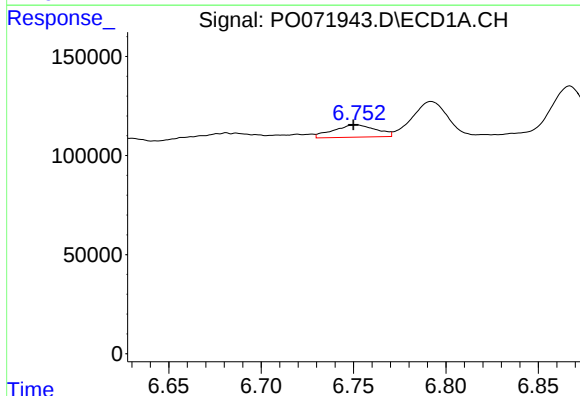


#27 AR-1254-2

R.T.: 6.752 min
Delta R.T.: 0.002 min
Response: 98989
Conc: 18.64 ng/ml

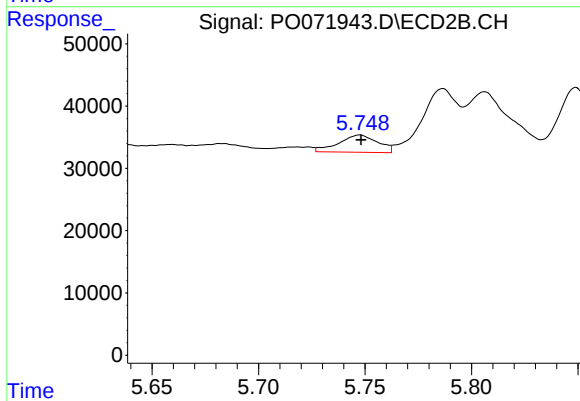

#27 AR-1254-2

R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 35478
Conc: 17.76 ng/ml

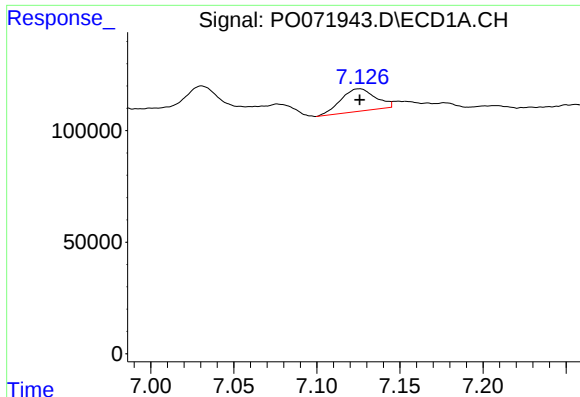


#28 AR-1254-3

R.T.: 7.126 min
Delta R.T.: 0.000 min
Response: 145805
Conc: 25.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-100120


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:26 PM

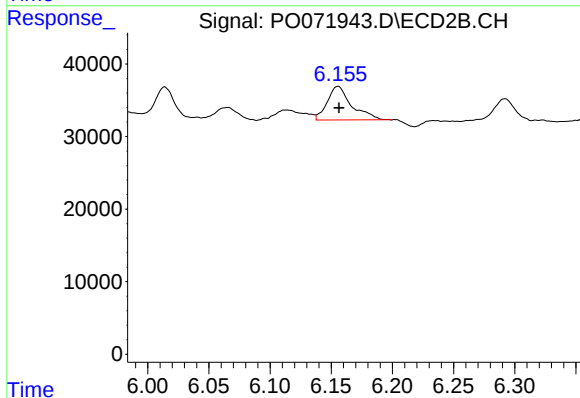


#28 AR-1254-3

R.T.: 6.155 min
Delta R.T.: -0.001 min
Response: 63879
Conc: 19.82 ng/ml m

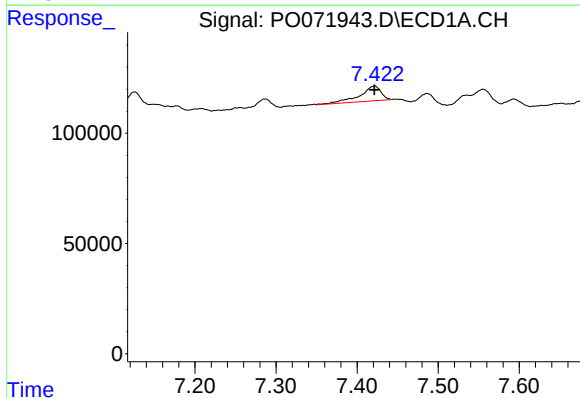


#29 AR-1254-4

R.T.: 7.422 min
Delta R.T.: 0.001 min
Response: 122871
Conc: 22.72 ng/ml

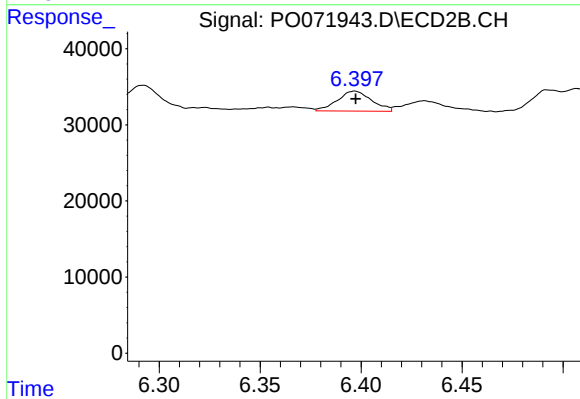

#29 AR-1254-4

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 31011
Conc: 13.53 ng/ml

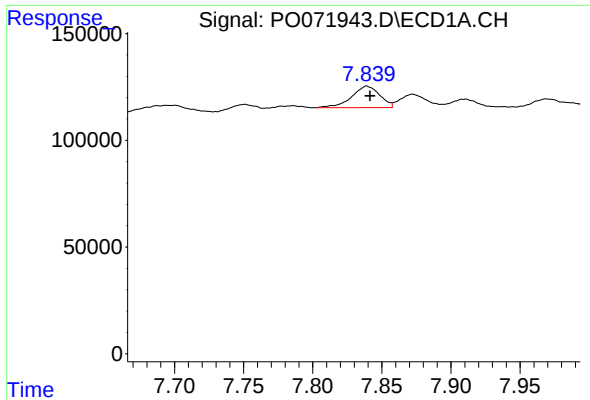


#30 AR-1254-5

R.T.: 7.839 min
Delta R.T.: -0.002 min
Response: 142605
Conc: 26.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-100120

Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:26 PM

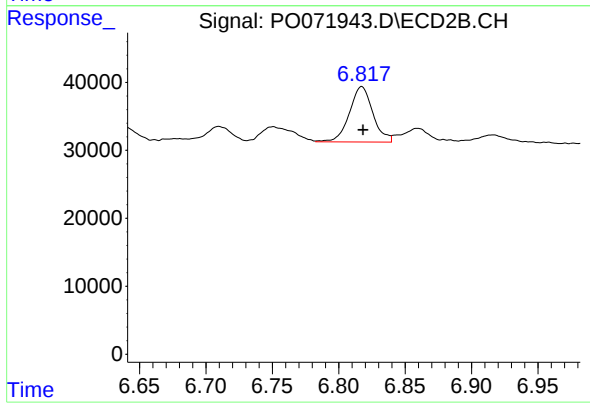

#30 AR-1254-5

R.T.: 6.817 min
Delta R.T.: -0.001 min
Response: 100307
Conc: 31.40 ng/ml