

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
 Data File : PO071956.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Oct 2020 6:14
 Operator : DD\AJ
 Sample : L4246-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 108885

Manual Integrations
 APPROVED

Ankita
 10/5/2020 3:35:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 07:38:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 03 04:09:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347f	3.542f	2325430	873301	32.376m	23.315m#
2) SA Decachlor...	9.938	8.689	2038297	928598	18.512	16.326

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100320\
Data File : P0071956.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Oct 2020 6:14
Operator : DD\AJ
Sample : L4246-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
108885


Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 07:38:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 03 04:09:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

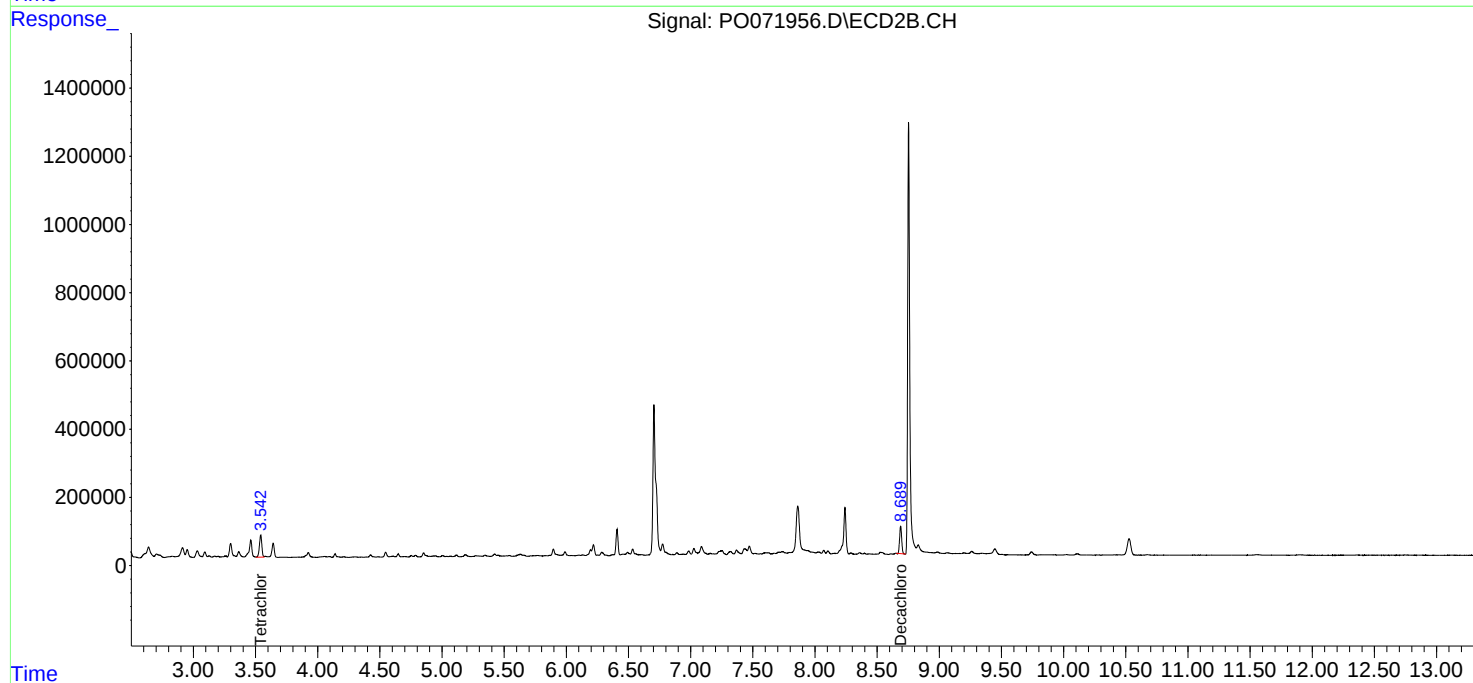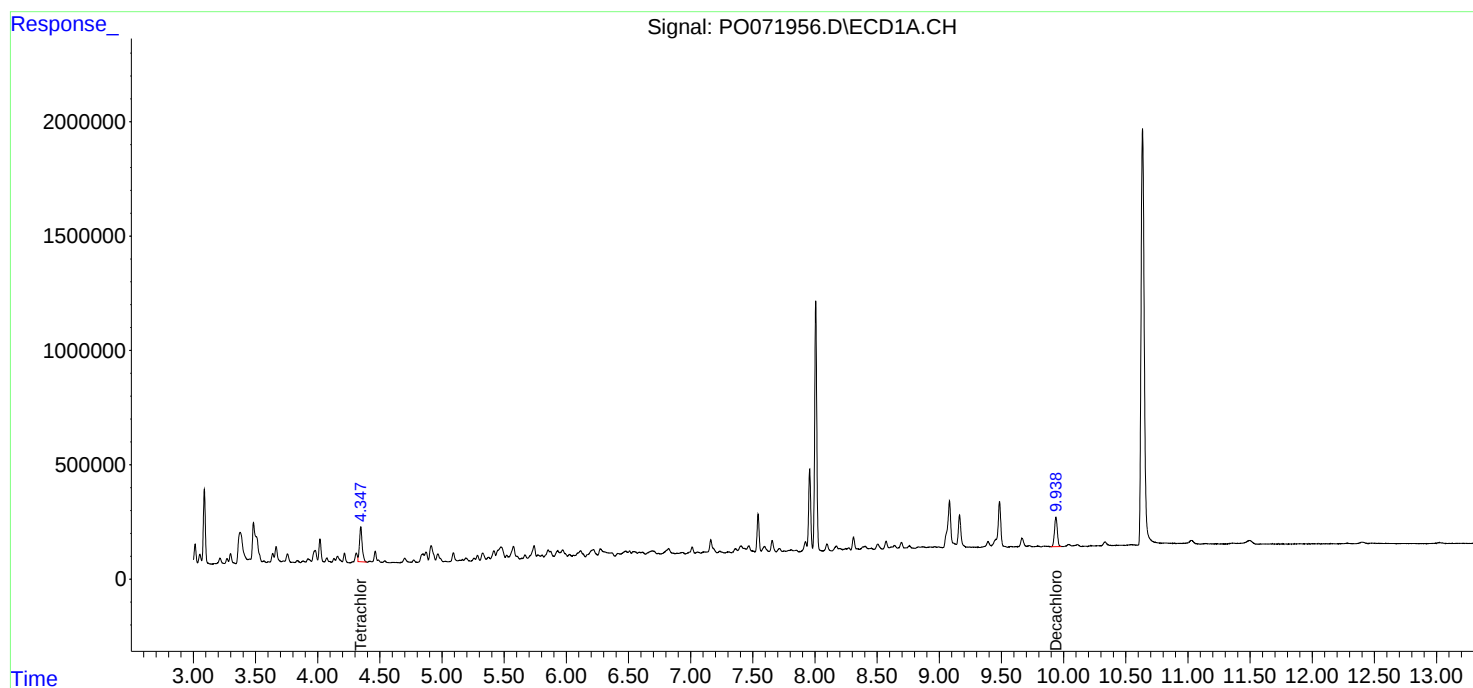

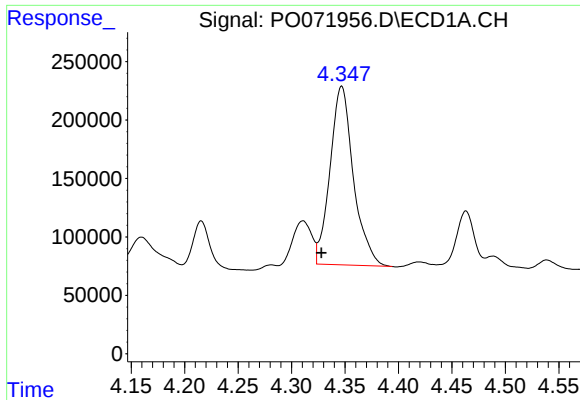

#1 Tetrachloro-m-xylene

R.T.: 4.347 min

Delta R.T.: 0.019 min


Response: 2325430

Conc: 32.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
108885

Manual Integrations
APPROVED

Ankita
10/5/2020 3:35:47 PM

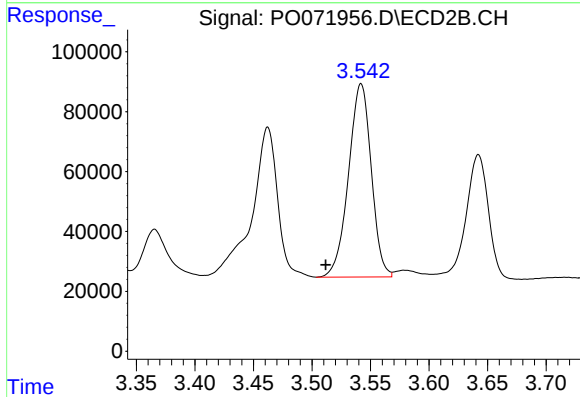


#1 Tetrachloro-m-xylene

R.T.: 3.542 min

Delta R.T.: 0.030 min

Response: 873301

Conc: 23.32 ng/ml m

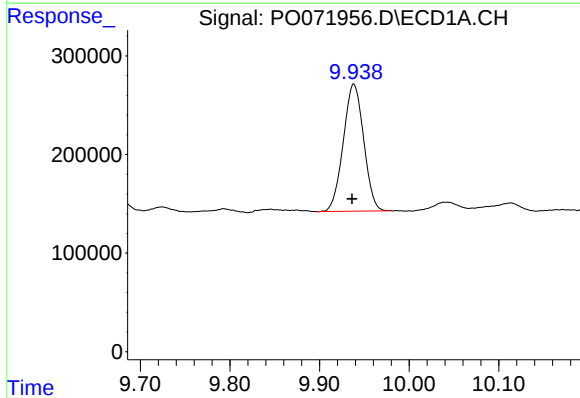


#2 Decachlorobiphenyl

R.T.: 9.938 min

Delta R.T.: 0.002 min

Response: 2038297

Conc: 18.51 ng/ml

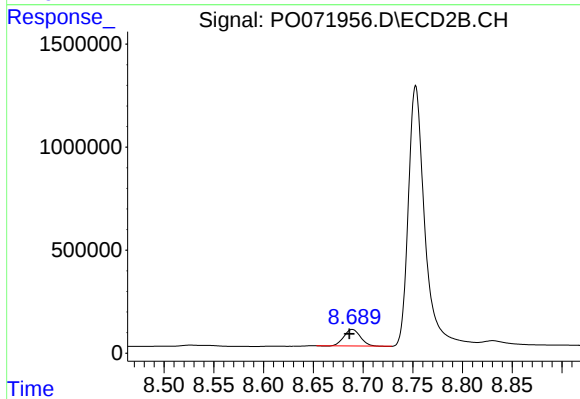

#2 Decachlorobiphenyl

R.T.: 8.689 min

Delta R.T.: 0.003 min

Response: 928598

Conc: 16.33 ng/ml