

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100323\
 Data File : P0098496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 22:28
 Operator : YP/AJ
 Sample : 04695-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P001-CS01-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2023
 Supervised By :mohammad ahmed 10/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 01:36:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.637	35114885	14626284	18.287	18.779
2) SA Decachlor...	10.300	8.643	22553445	10580588	18.580	19.749m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100323\
Data File : PO098496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 22:28
Operator : YP/AJ
Sample : 04695-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P001-CS01-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2023
Supervised By :mohammad ahmed 10/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 01:36:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

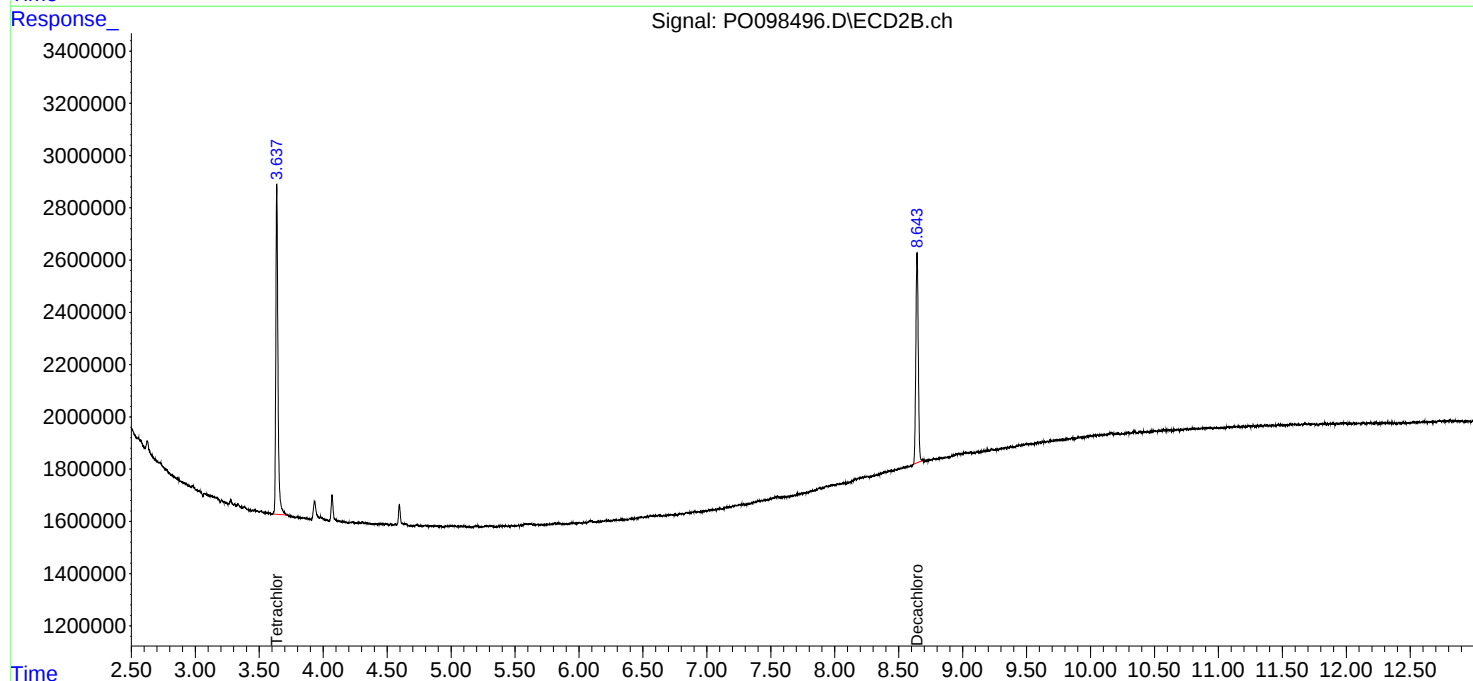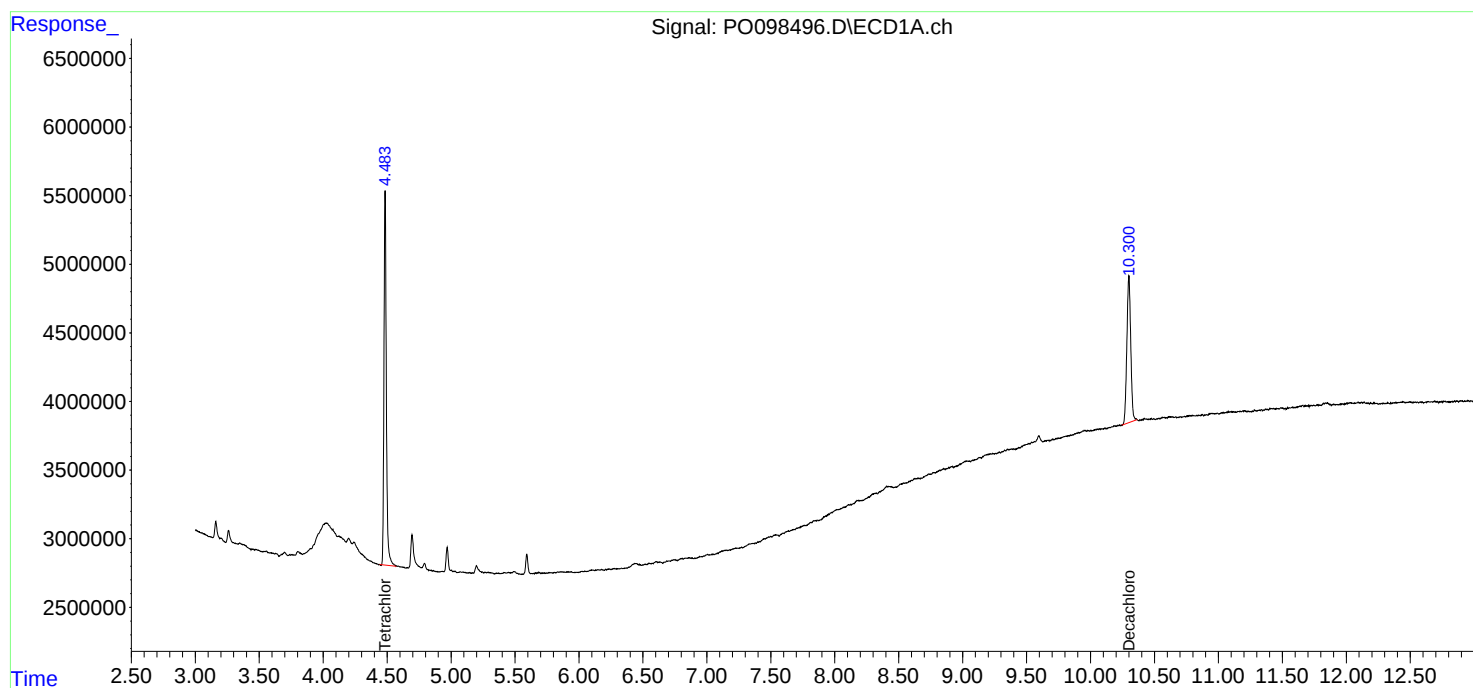

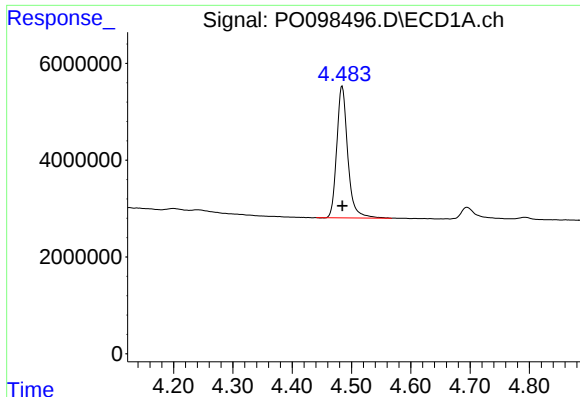


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.000 min
Response: 35114885
Conc: 18.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
P001-CS01-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2023
Supervised By :mohammad ahmed 10/16/2023

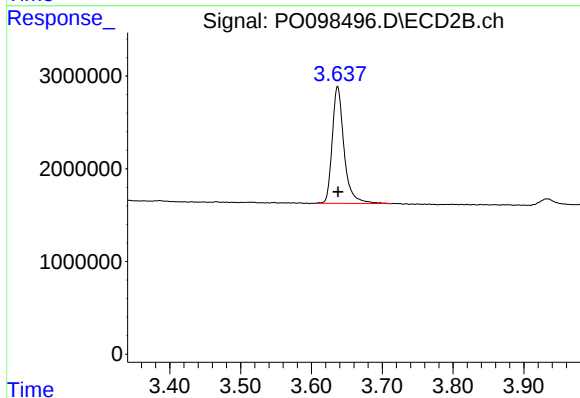


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: 0.000 min
Response: 14626284
Conc: 18.78 ng/ml

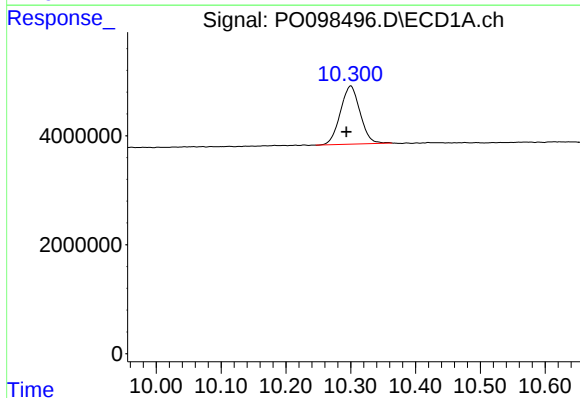

#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: 0.006 min
Response: 22553445
Conc: 18.58 ng/ml

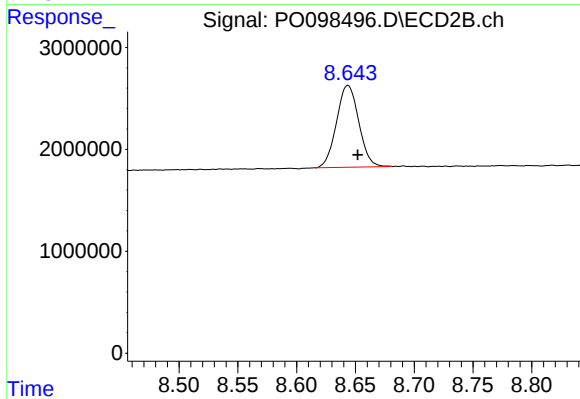

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.009 min
Response: 10580588
Conc: 19.75 ng/ml m