

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100323\
 Data File : P0098507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 02:03
 Operator : YP/AJ
 Sample : 04695-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P001-CS04-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/04/2023
 Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 03:01:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.635	35450789	14606855	18.462	18.754
2) SA Decachlor...	10.294	8.640	15801038	7582751	13.017	14.153m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100323\
Data File : PO098507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 02:03
Operator : YP/AJ
Sample : 04695-13
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P001-CS04-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 03:01:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

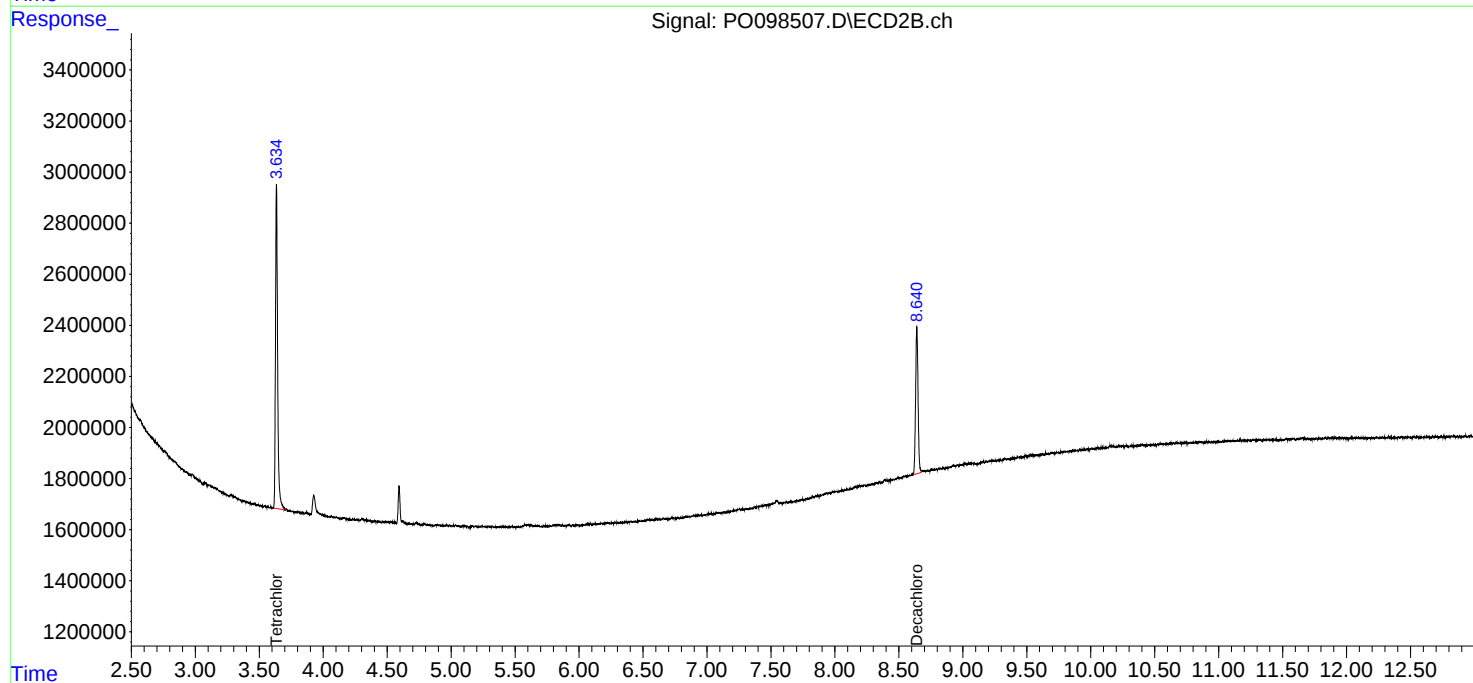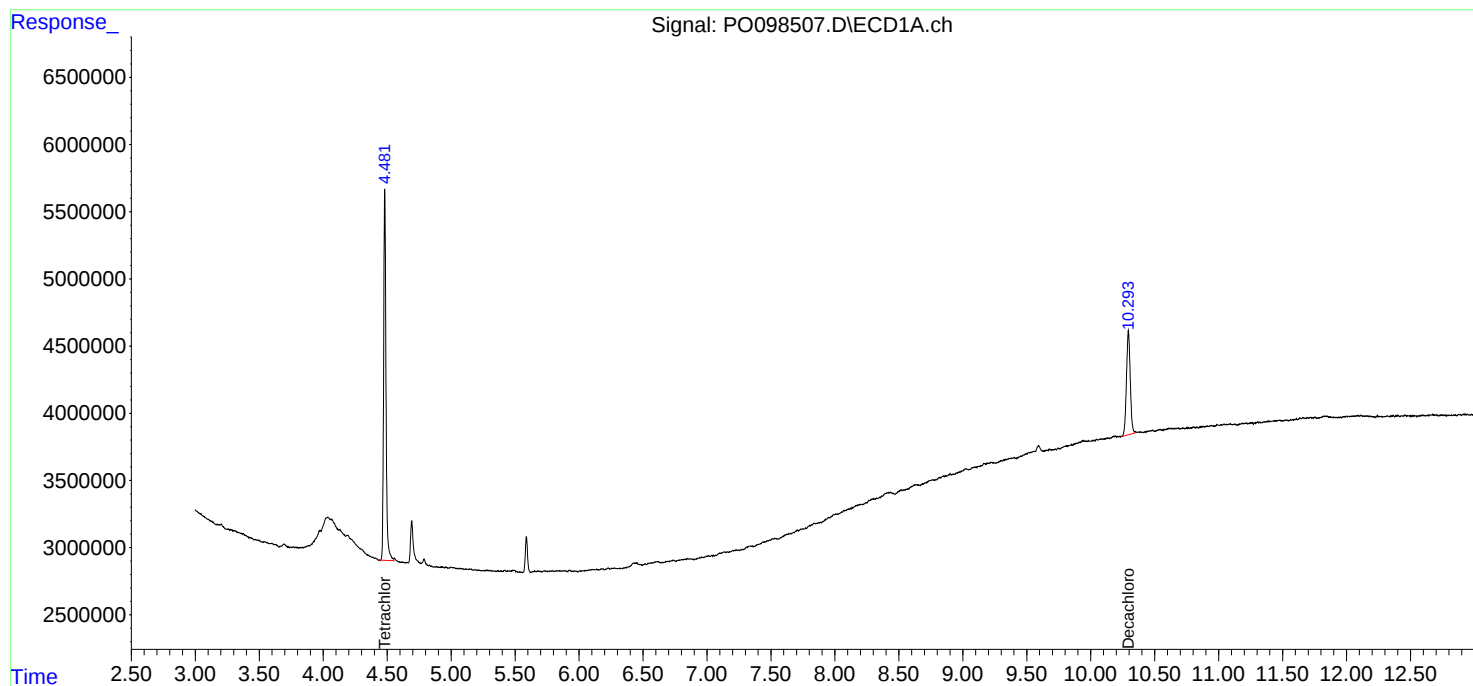

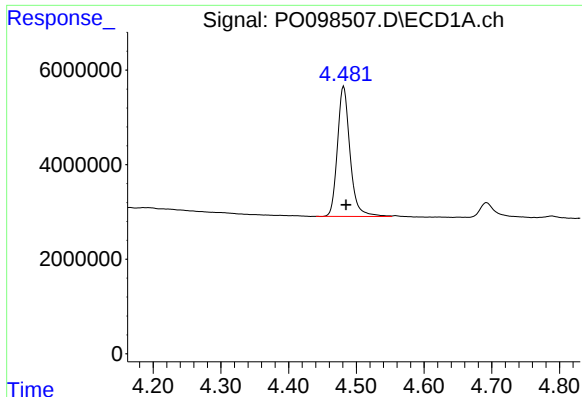


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: -0.004 min
Response: 35450789
Conc: 18.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
P001-CS04-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/04/2023
Supervised By :Ankita Jodhani 10/04/2023

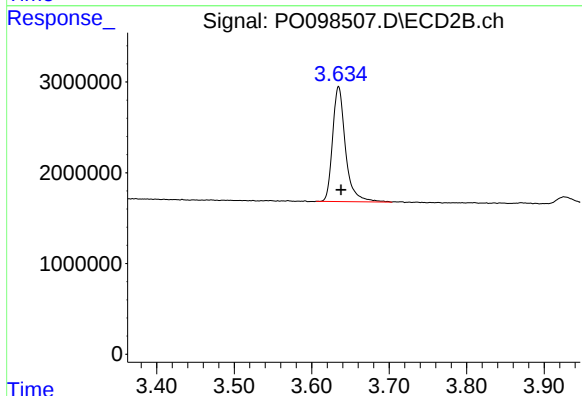


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 14606855
Conc: 18.75 ng/ml

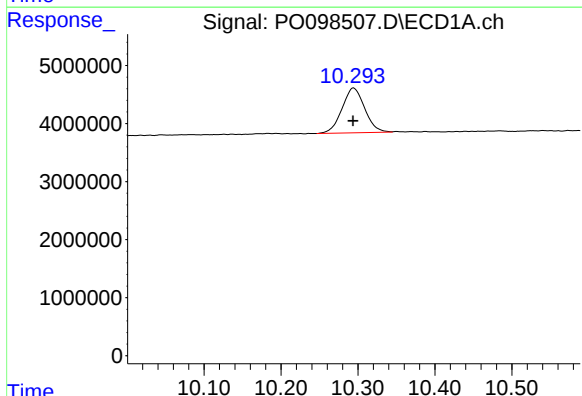

#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: 0.000 min
Response: 15801038
Conc: 13.02 ng/ml

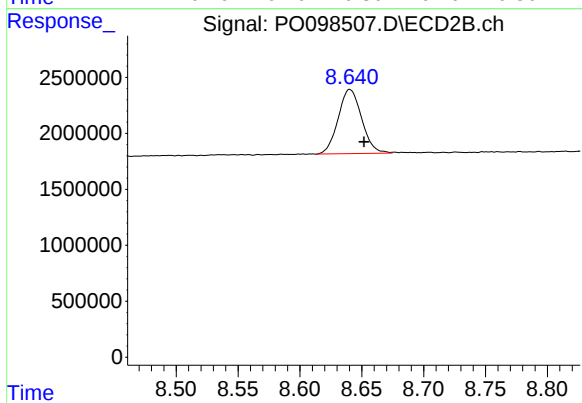

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.012 min
Response: 7582751
Conc: 14.15 ng/ml m