

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
 Data File : PO049621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2018 19:23
 Operator : SM/SJ
 Sample : J5241-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100218-SIDI-E-D-M

Manual Integrations
 APPROVED

Sohil
 10/5/2018 11:05:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 01:01:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.516	4524379	3831741	12.812	11.266m
2) SA Decachlor...	10.096	8.444	4436707	2722603	9.363	8.911

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
Data File : PO049621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2018 19:23
Operator : SM/SJ
Sample : J5241-02
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
100218-SIDI-E-D-M


Manual Integrations
APPROVED

Sohil
10/5/2018 11:05:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 01:01:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

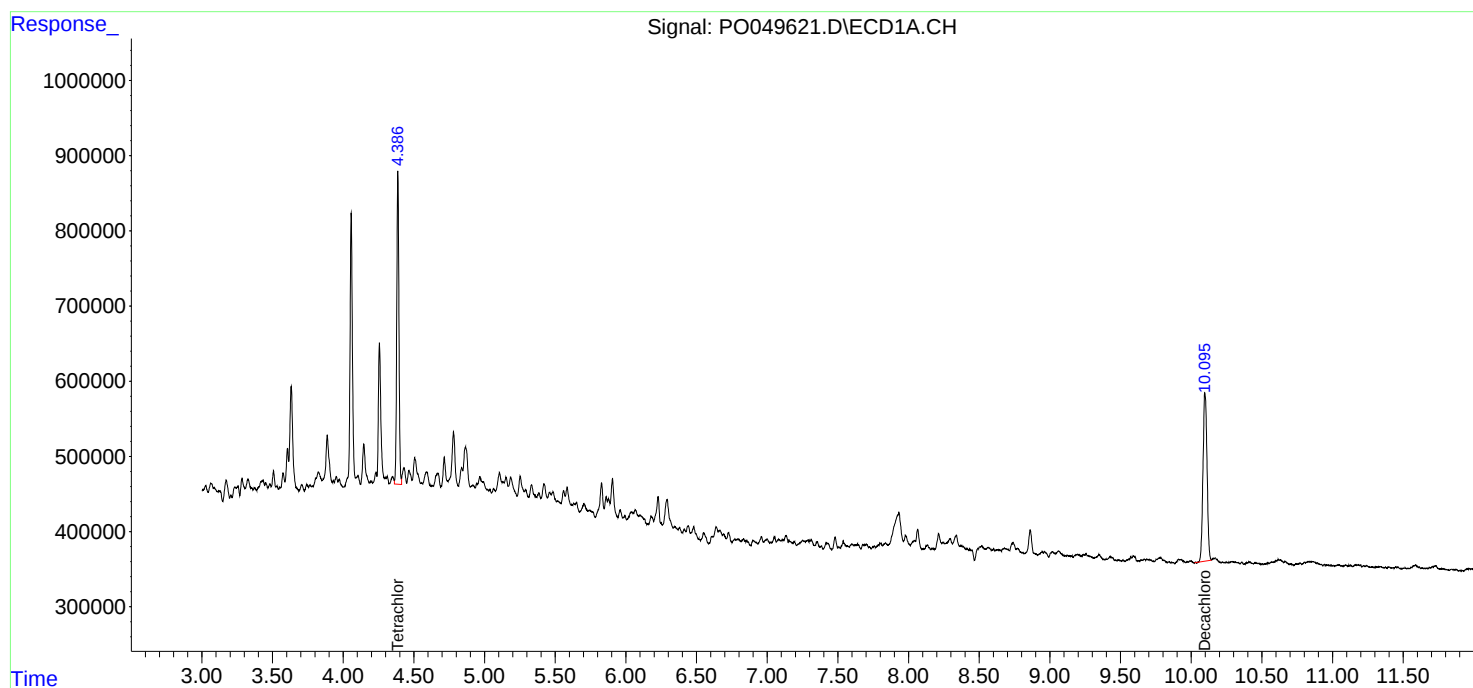

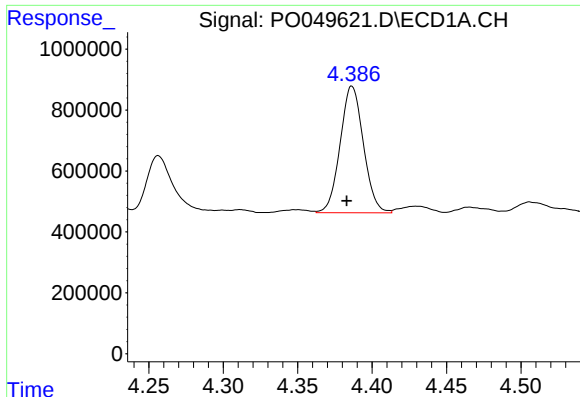


#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: 0.004 min
Response: 4524379
Conc: 12.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
100218-SIDI-E-D-M


Manual Integrations
APPROVED

Sohil
10/5/2018 11:05:59 AM

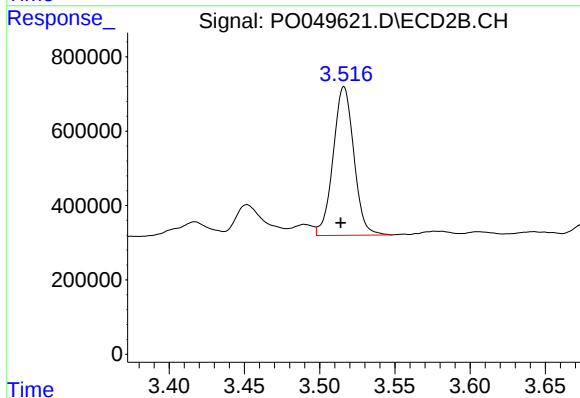


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.002 min
Response: 3831741
Conc: 11.27 ng/ml m

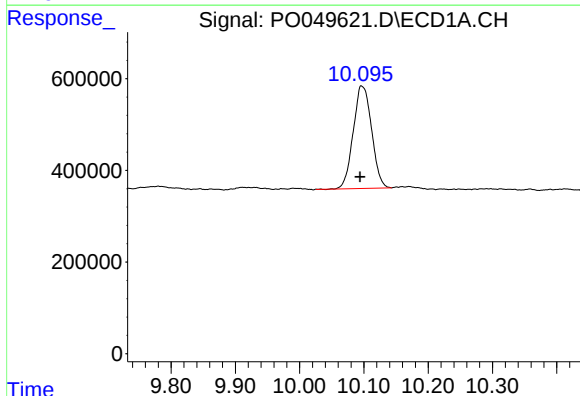

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.002 min
Response: 4436707
Conc: 9.36 ng/ml

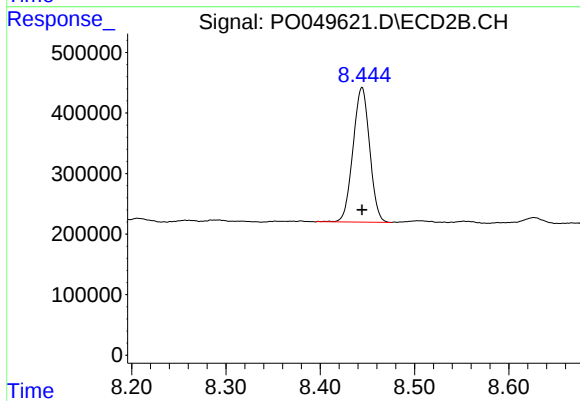

#2 Decachlorobiphenyl

R.T.: 8.444 min
Delta R.T.: 0.000 min
Response: 2722603
Conc: 8.91 ng/ml