

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
 Data File : PO049641.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 00:58
 Operator : SM/SJ
 Sample : J5219-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-E10-F10-E10A-F10A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 02:31:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.515	6647642	6462367	18.825	19.000
2) SA Decachlor...	10.097	8.442	7092465	5111923	14.967	16.731

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
Data File : P0049641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 00:58
Operator : SM/SJ
Sample : J5219-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E10-F10-E10A-F10A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 02:31:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

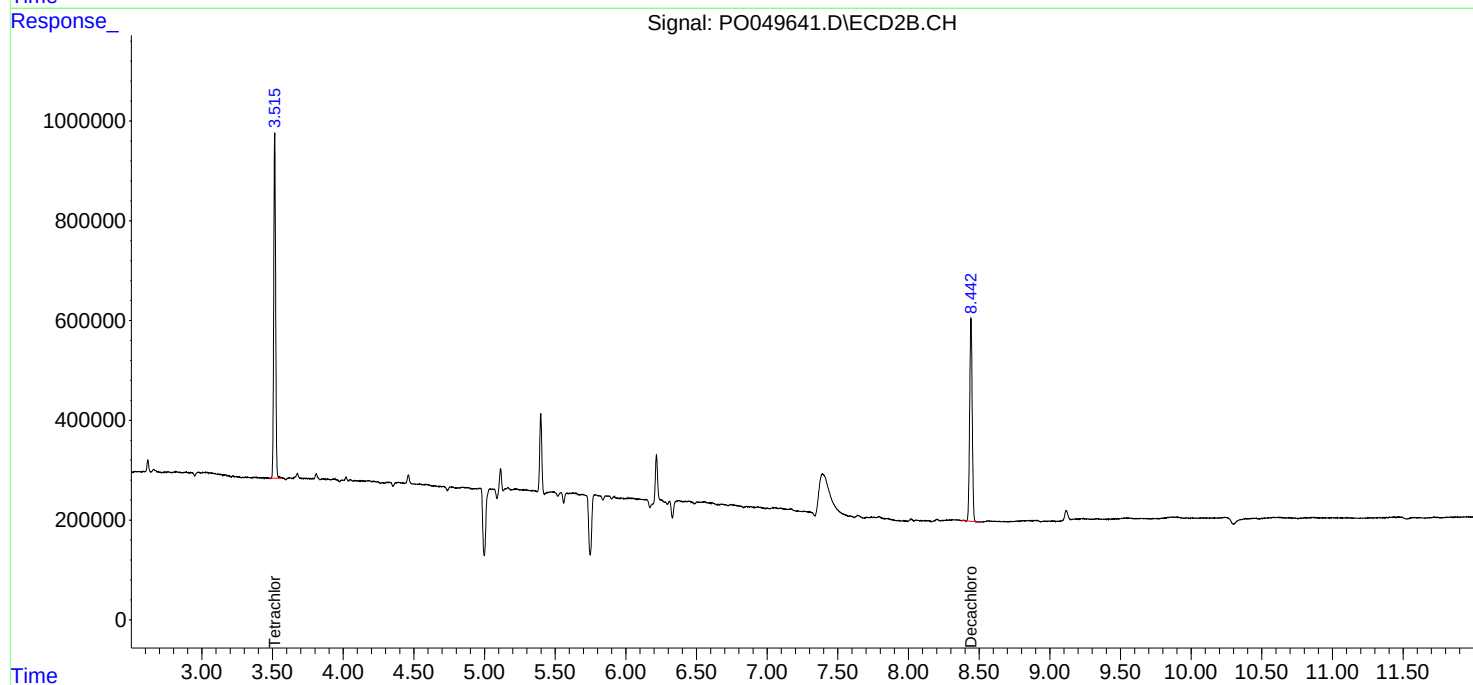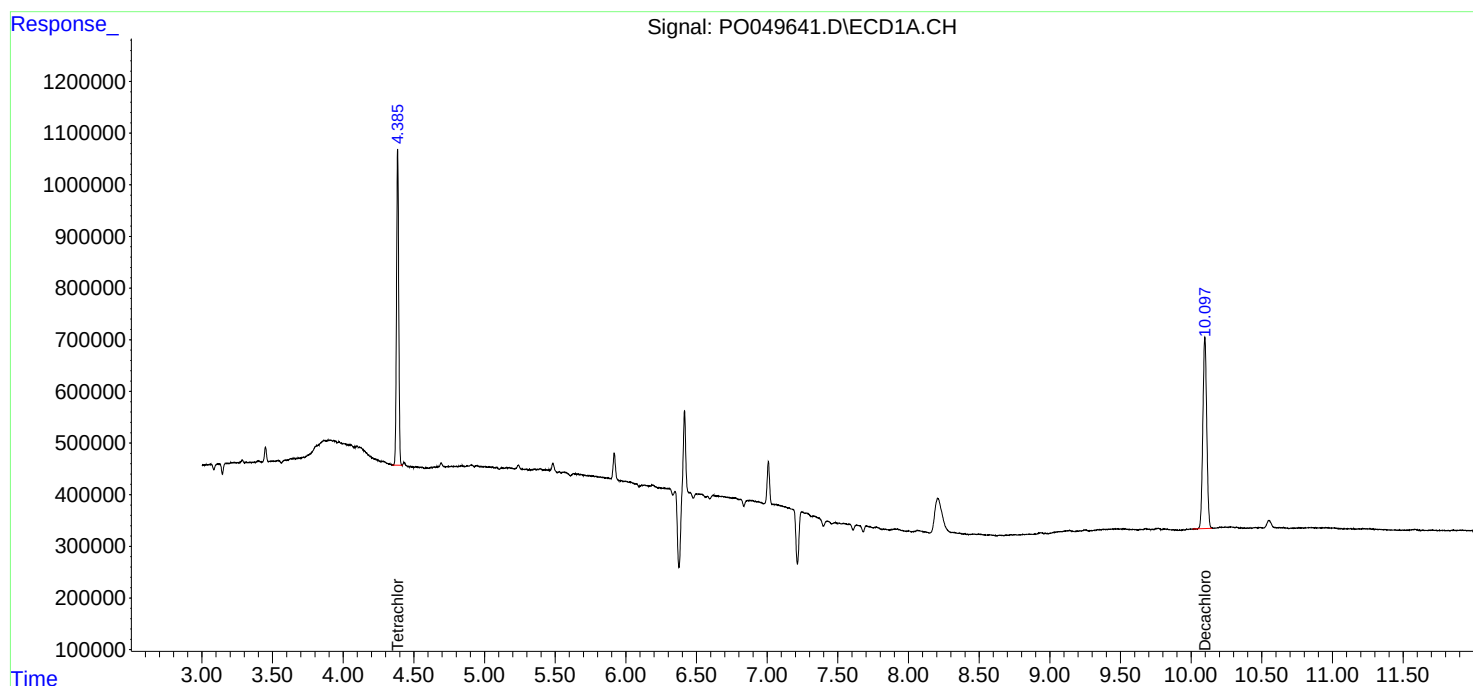


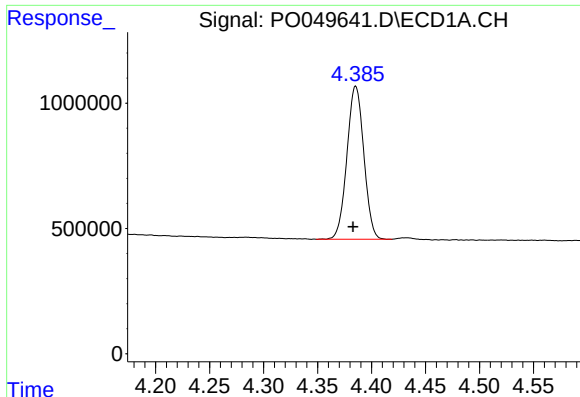

#1 Tetrachloro-m-xylene


R.T.: 4.385 min
Delta R.T.: 0.002 min
Response: 6647642
Conc: 18.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E10-F10-E10A-F10A

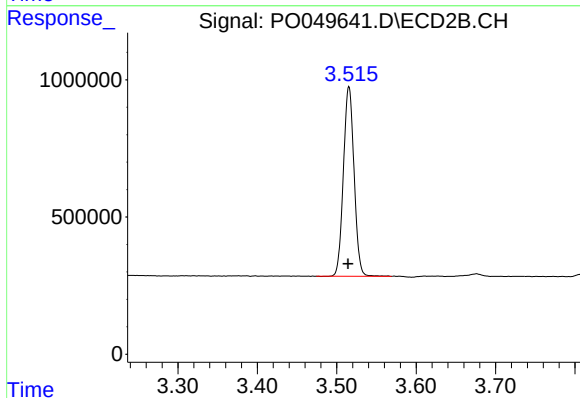


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 6462367
Conc: 19.00 ng/ml

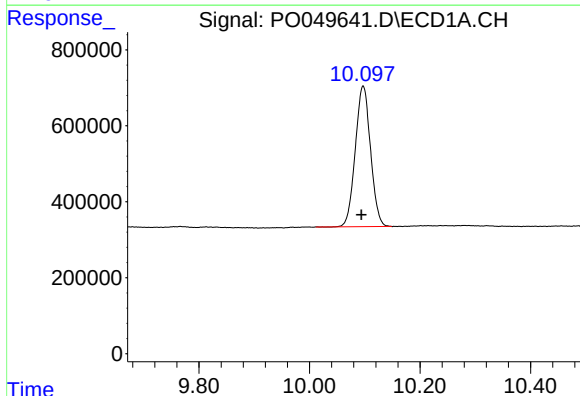

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: 0.003 min
Response: 7092465
Conc: 14.97 ng/ml

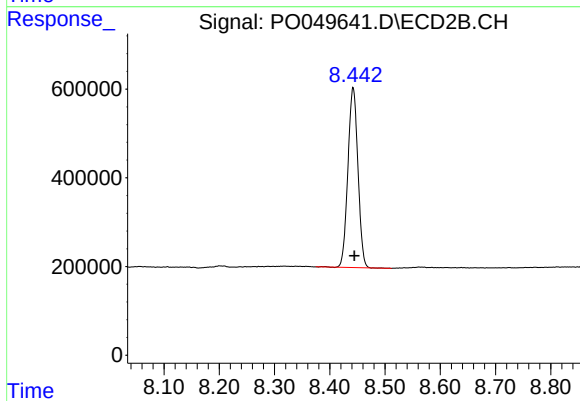

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.002 min
Response: 5111923
Conc: 16.73 ng/ml