

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
 Data File : PO049660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 6:18
 Operator : SM/SJ
 Sample : J5244-04
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER

Manual Integrations
 APPROVED

Sohil
 10/5/2018 11:06:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 06:43:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.515	4596451	4546041	13.016m	13.366m
2) SA Decachlor...	10.094	8.440	4224405	3162625	8.915	10.351

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
Data File : PO049660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 6:18
Operator : SM/SJ
Sample : J5244-04
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Sohil
10/5/2018 11:06:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 06:43:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

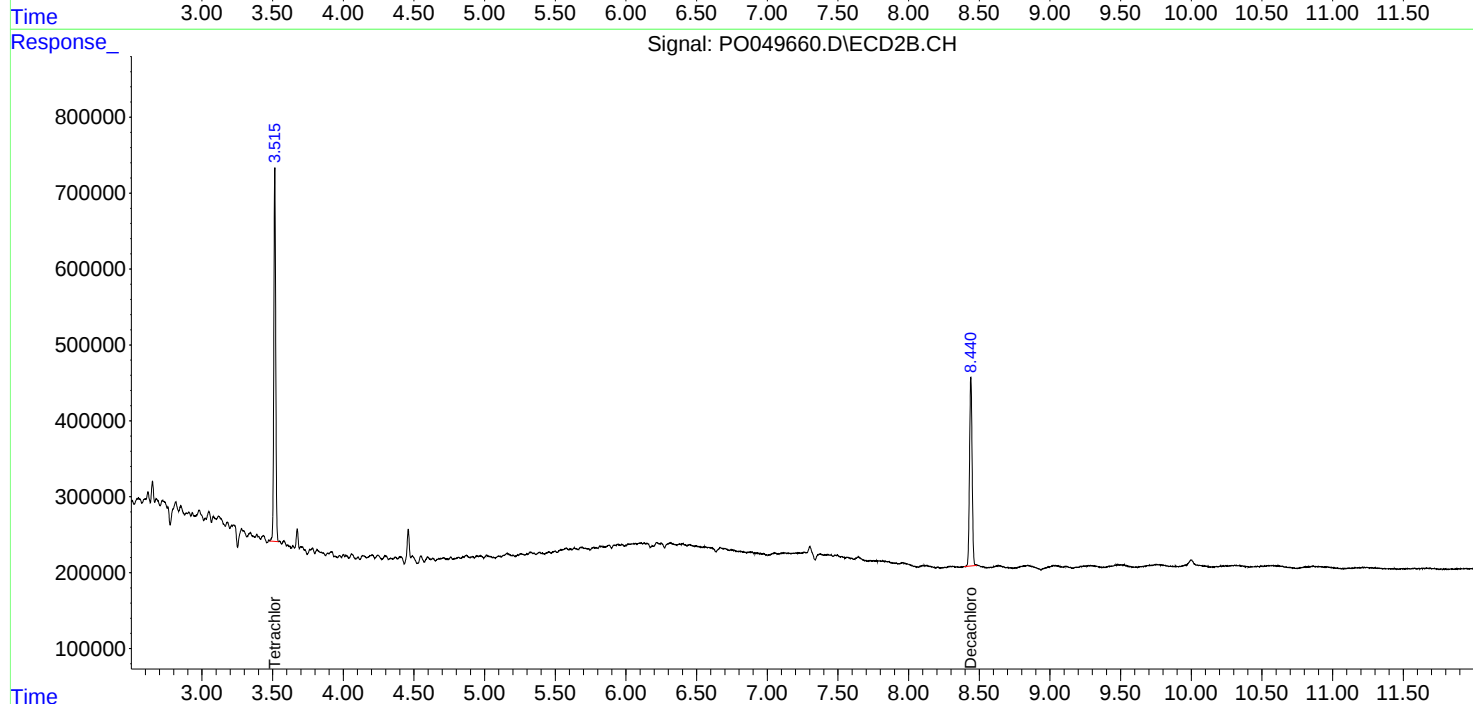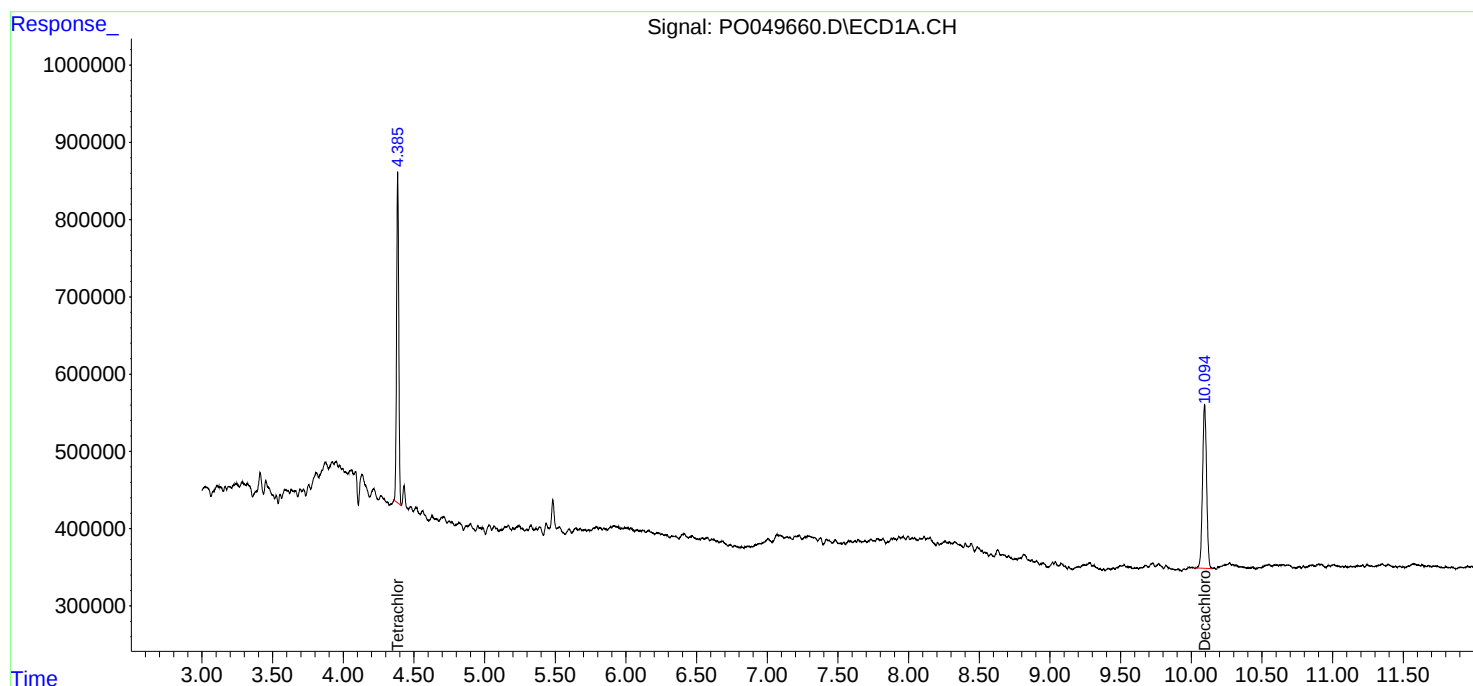

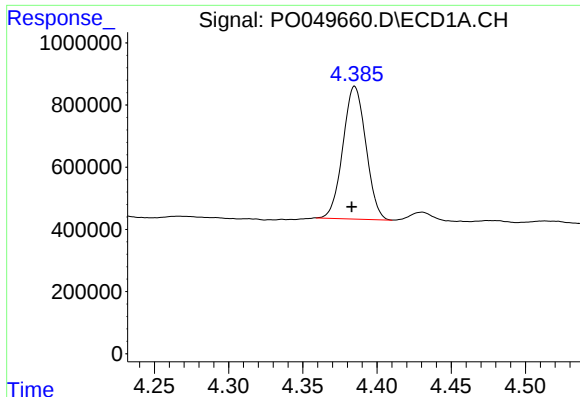


#1 Tetrachloro-m-xylene

R.T.: 4.385 min
Delta R.T.: 0.002 min
Response: 4596451
Conc: 13.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Sohil
10/5/2018 11:06:58 AM

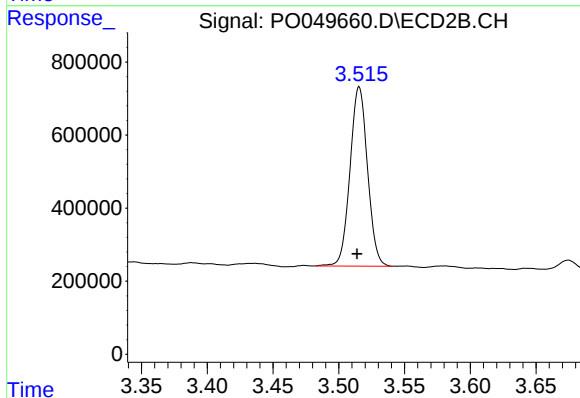


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 4546041
Conc: 13.37 ng/ml m

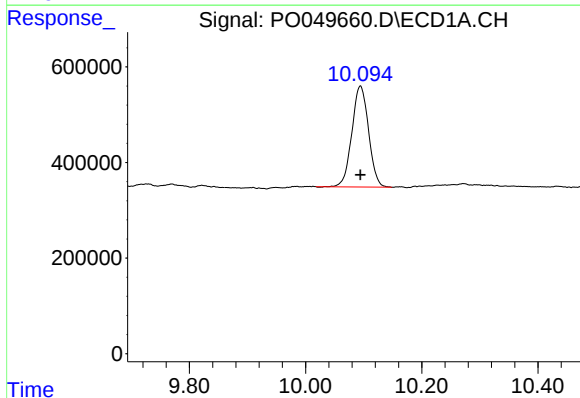

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.000 min
Response: 4224405
Conc: 8.91 ng/ml

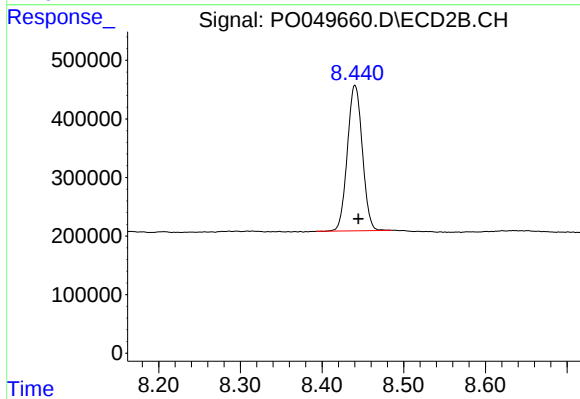

#2 Decachlorobiphenyl

R.T.: 8.440 min
Delta R.T.: -0.004 min
Response: 3162625
Conc: 10.35 ng/ml