

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
 Data File : PO049661.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Oct 2018 6:34
 Operator : SM/SJ
 Sample : J5150-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-0926-S-10B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 07:16:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 02 05:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.386	3.515	8548410	8475854	24.208	24.920
2)	SA Decachlor...	10.094	8.441	7776343	5733120	16.411	18.764

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100418\
Data File : P0049661.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Oct 2018 6:34
Operator : SM/SJ
Sample : J5150-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-0926-S-10B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 07:16:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100118.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 02 05:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

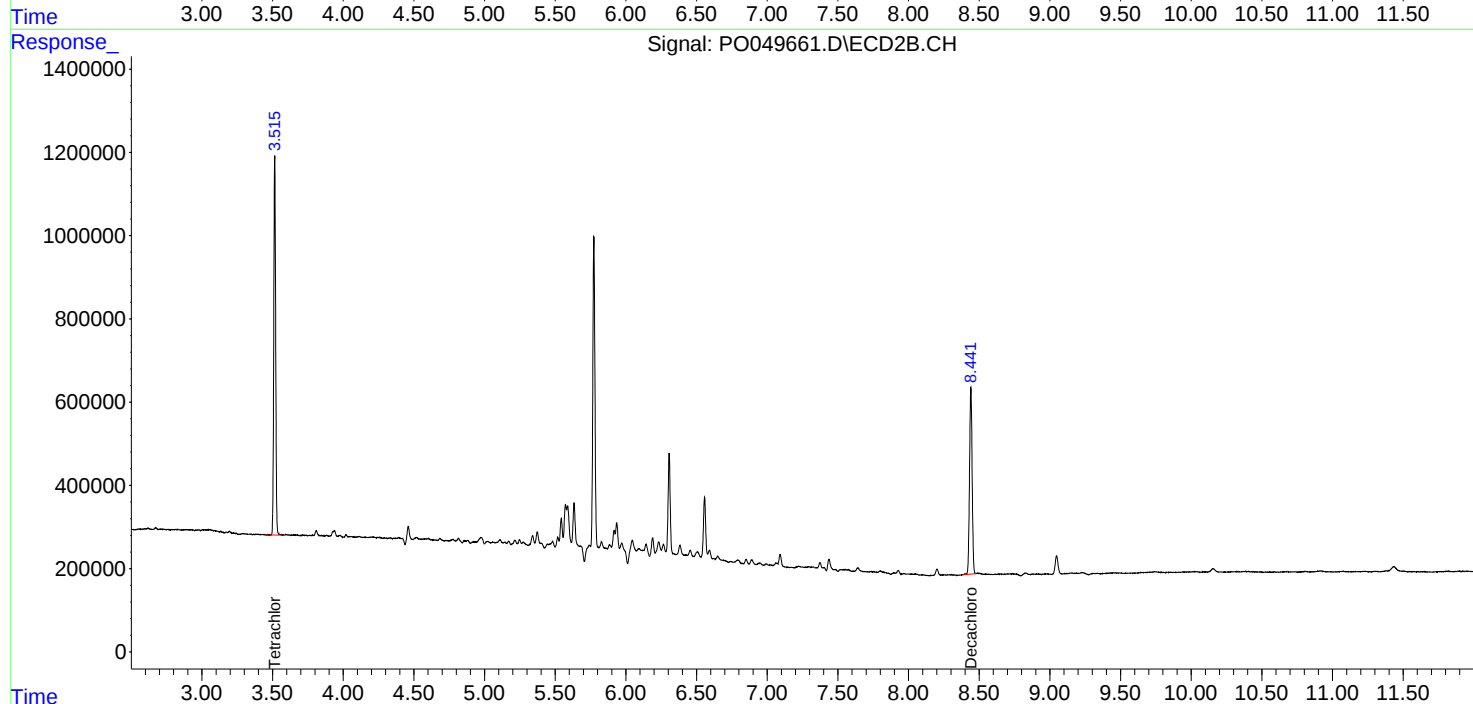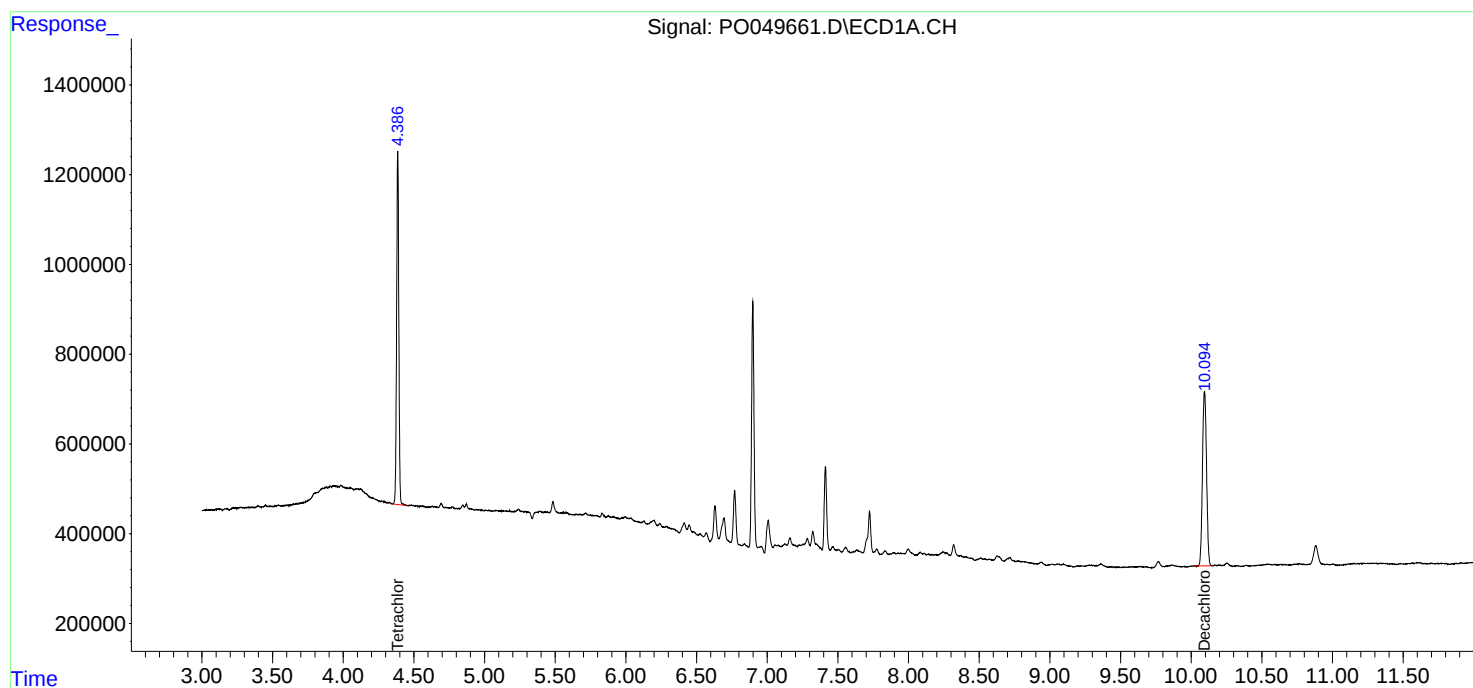


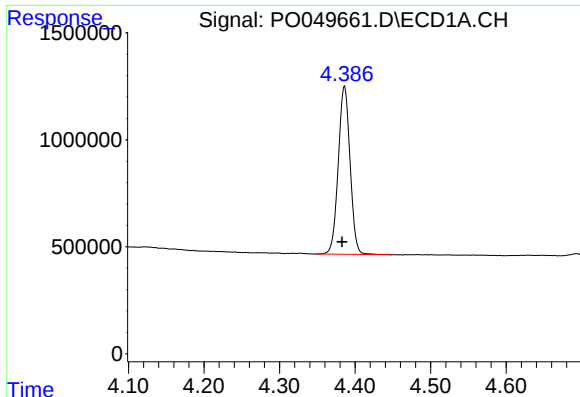

#1 Tetrachloro-m-xylene


R.T.: 4.386 min
Delta R.T.: 0.003 min
Response: 8548410
Conc: 24.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-0926-S-10B

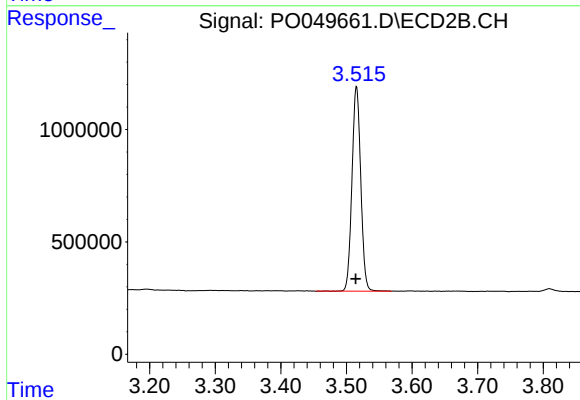


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: 0.001 min
Response: 8475854
Conc: 24.92 ng/ml

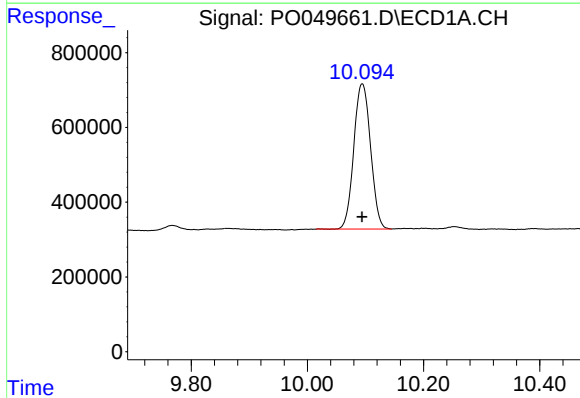

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.000 min
Response: 7776343
Conc: 16.41 ng/ml

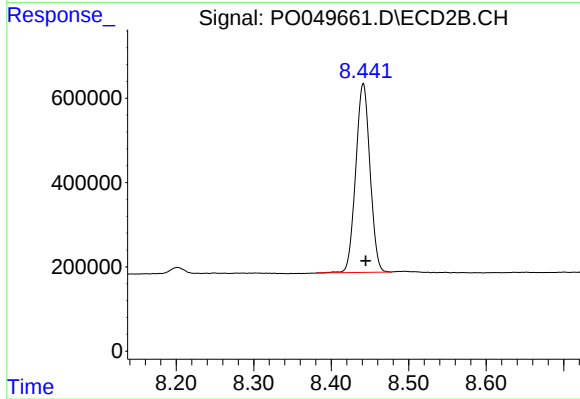

#2 Decachlorobiphenyl

R.T.: 8.441 min
Delta R.T.: -0.003 min
Response: 5733120
Conc: 18.76 ng/ml