

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100421\
 Data File : P0081750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 19:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 01:08:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.868	3.983	1855561	525977	20.808	19.742
2)	SA Decachlor...	10.877	9.327	1651236	512058	22.168	22.050
Target Compounds							
8)	L2 AR-1221-1	5.114	0.000	54217	0	49.545	N.D. #
9)	L2 AR-1221-2	5.220	0.000	27125	0	34.402	N.D. #
10)	L2 AR-1221-3	0.000	4.424	0	10628	N.D.	13.697 #
11)	L3 AR-1232-1	0.000	4.424	0	10628	N.D.	17.725 #
24)	L5 AR-1248-4	7.116f	0.000	24588	0	7.139	N.D. #
26)	L6 AR-1254-1	7.116	0.000	24588	0	6.858	N.D. #
28)	L6 AR-1254-3	7.736	0.000	30704	0	5.442	N.D. #
33)	L7 AR-1260-3	0.000	7.205	0	7268	N.D.	4.371 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100421\
Data File : PO081750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 19:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 01:08:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

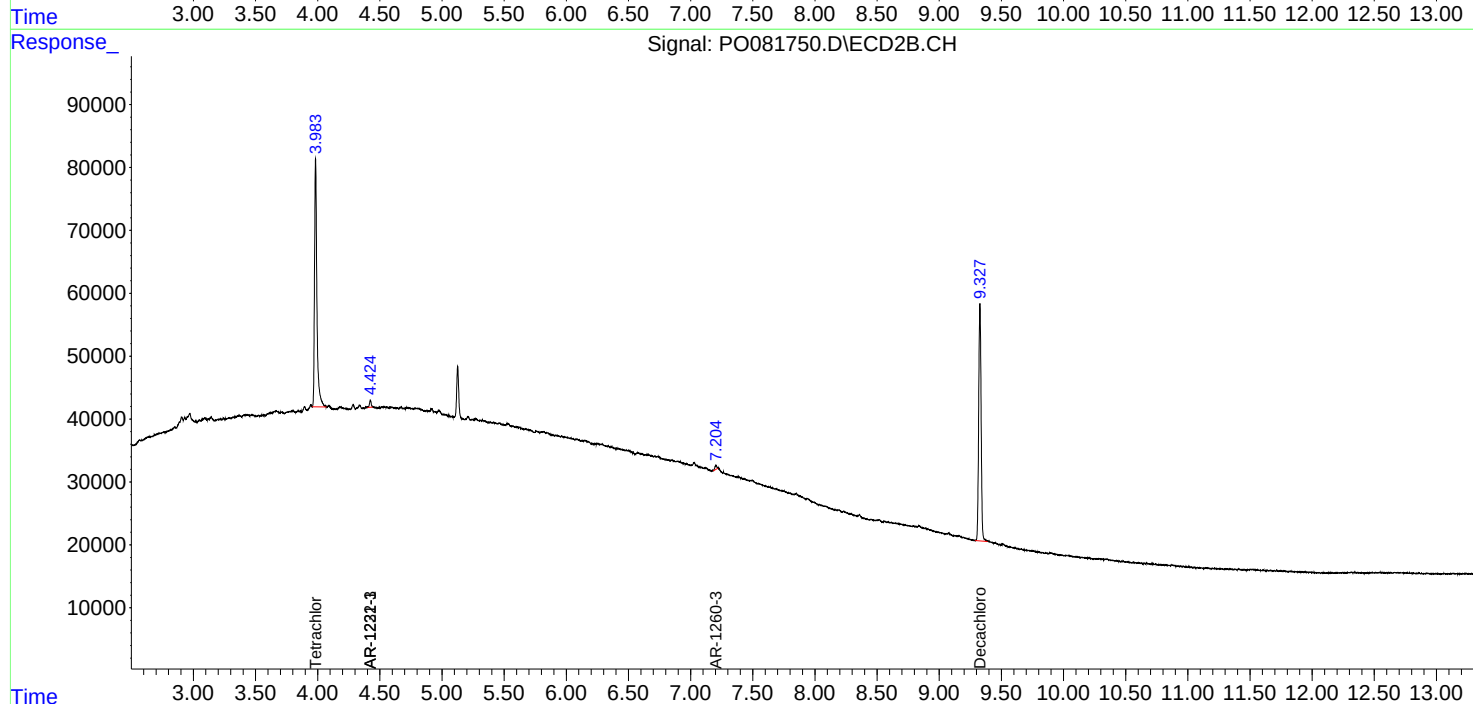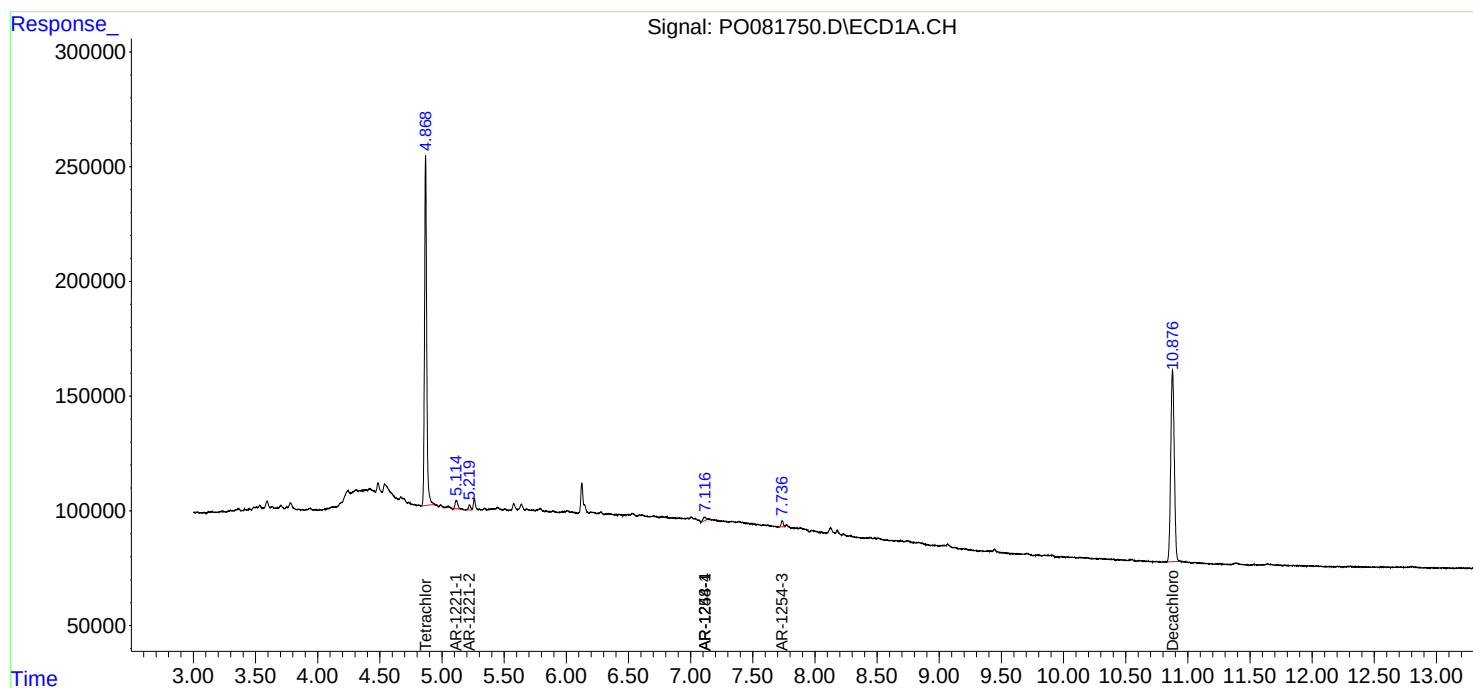


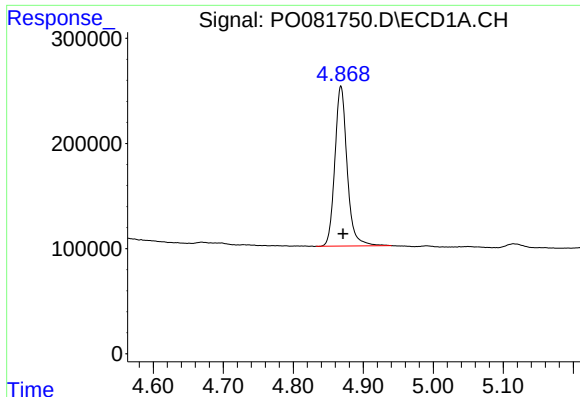

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.003 min
Response: 1855561
Conc: 20.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

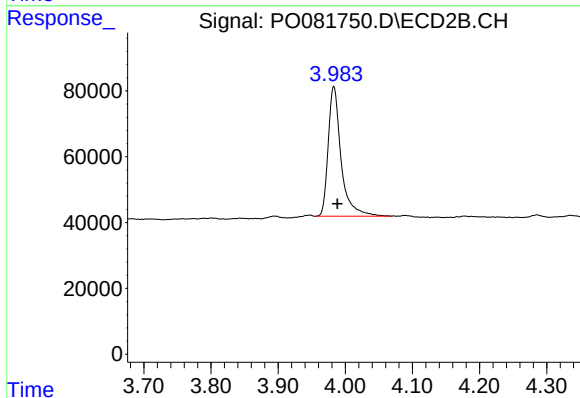


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.005 min
Response: 525977
Conc: 19.74 ng/ml

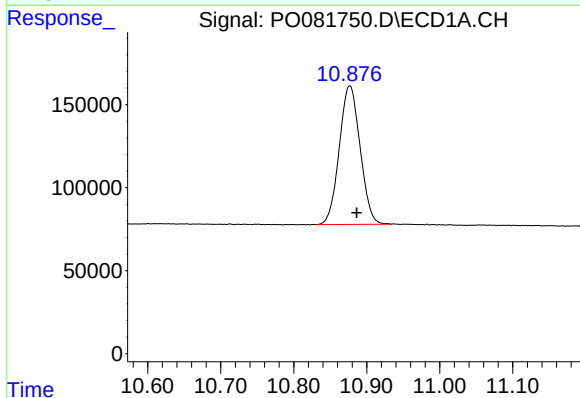


#2 Decachlorobiphenyl

R.T.: 10.877 min
Delta R.T.: -0.009 min
Response: 1651236
Conc: 22.17 ng/ml

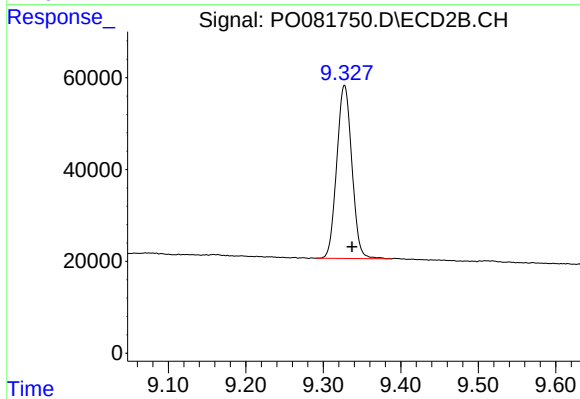

#2 Decachlorobiphenyl


R.T.: 9.327 min
Delta R.T.: -0.009 min
Response: 512058
Conc: 22.05 ng/ml

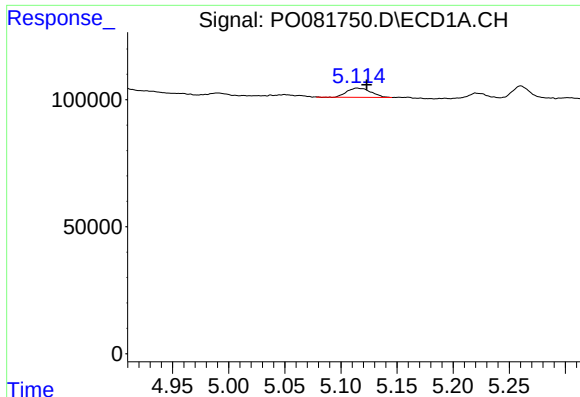

#8 AR-1221-1


R.T.: 5.114 min
Delta R.T.: -0.009 min
Response: 54217
Conc: 49.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

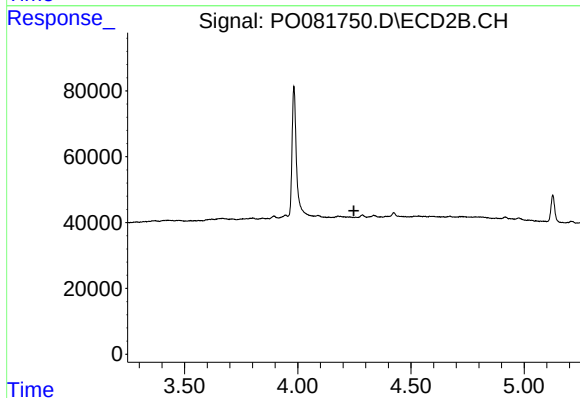


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.248 min
Response: 0
Conc: N.D.

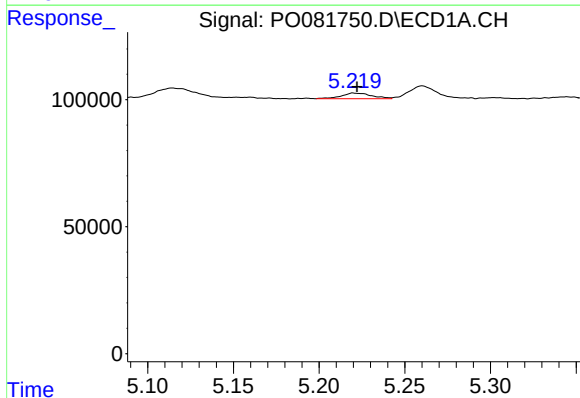


#9 AR-1221-2

R.T.: 5.220 min
Delta R.T.: -0.002 min
Response: 27125
Conc: 34.40 ng/ml

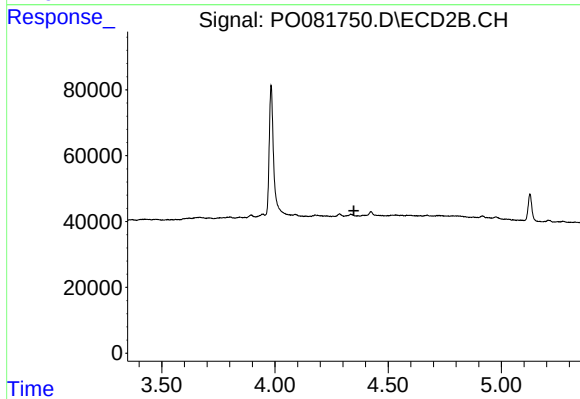

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.348 min
Response: 0
Conc: N.D.

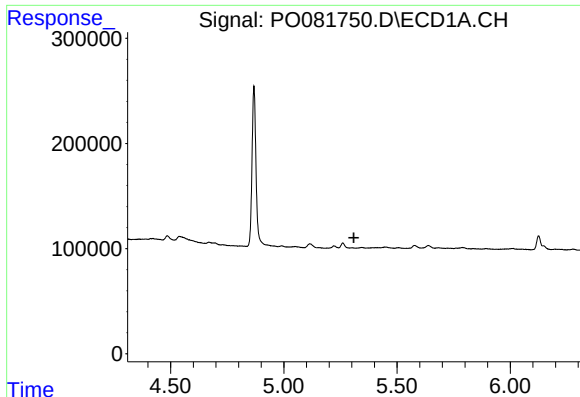

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.310 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

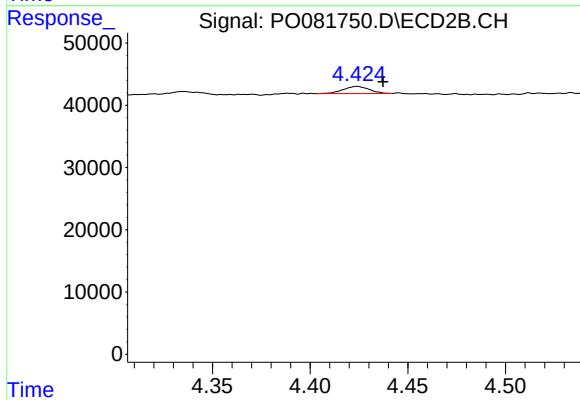


#10 AR-1221-3

R.T.: 4.424 min
Delta R.T.: -0.013 min
Response: 10628
Conc: 13.70 ng/ml

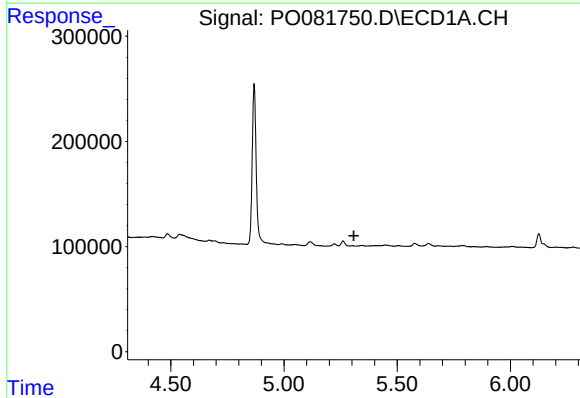


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.309 min
Response: 0
Conc: N.D.

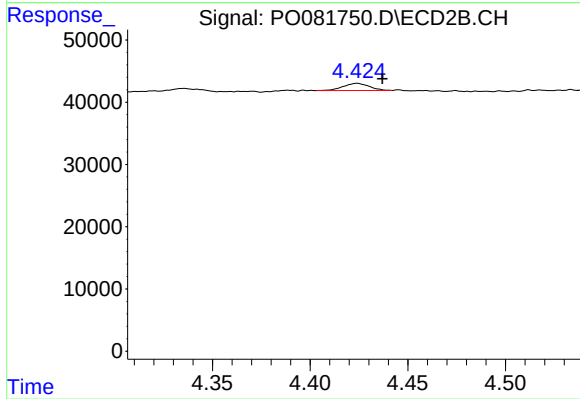

#11 AR-1232-1


R.T.: 4.424 min
Delta R.T.: -0.013 min
Response: 10628
Conc: 17.73 ng/ml

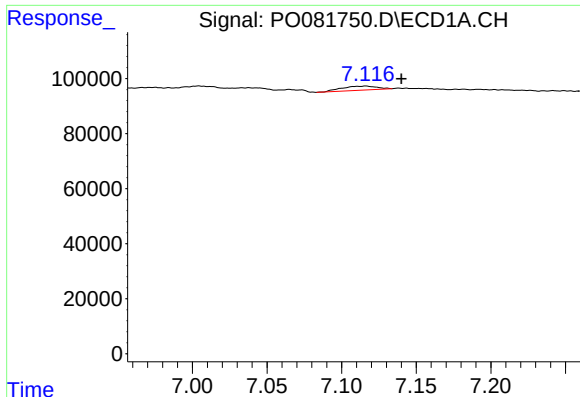

#24 AR-1248-4


R.T.: 7.116 min
Delta R.T.: -0.024 min
Response: 24588
Conc: 7.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

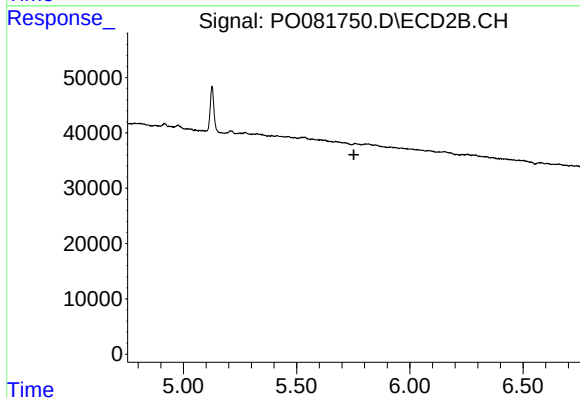


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

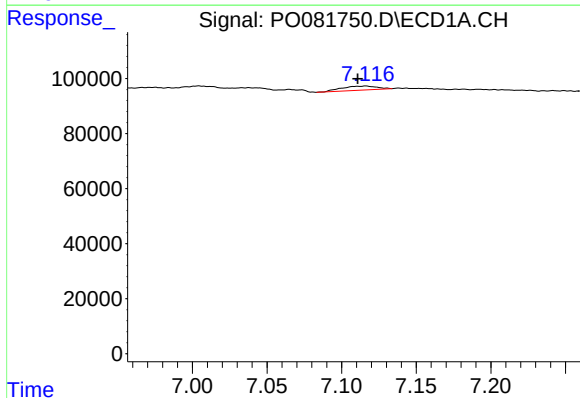


#26 AR-1254-1

R.T.: 7.116 min
Delta R.T.: 0.005 min
Response: 24588
Conc: 6.86 ng/ml

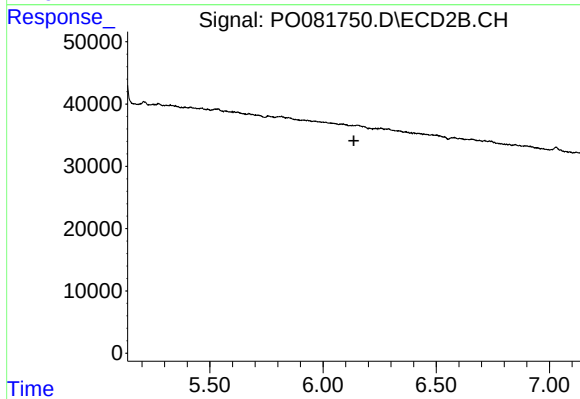

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

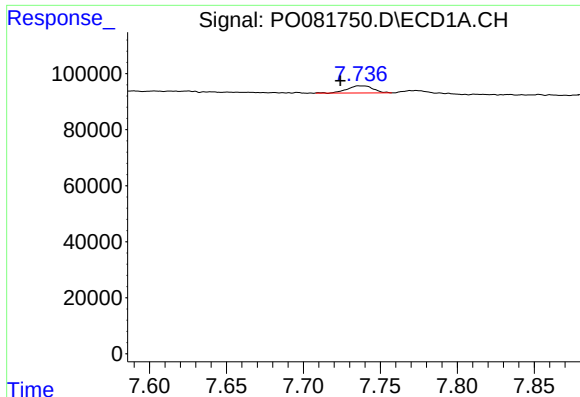

#28 AR-1254-3


R.T.: 7.736 min
Delta R.T.: 0.012 min
Response: 30704
Conc: 5.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

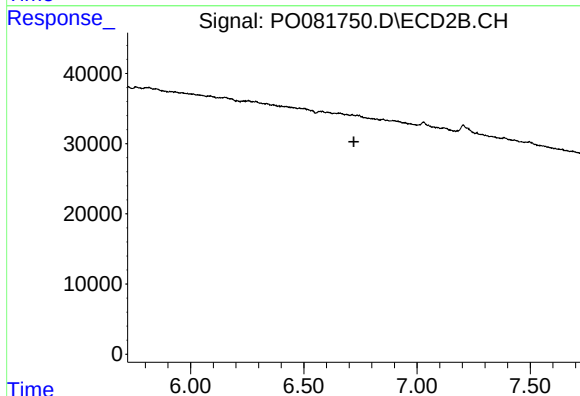


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.721 min
Response: 0
Conc: N.D.

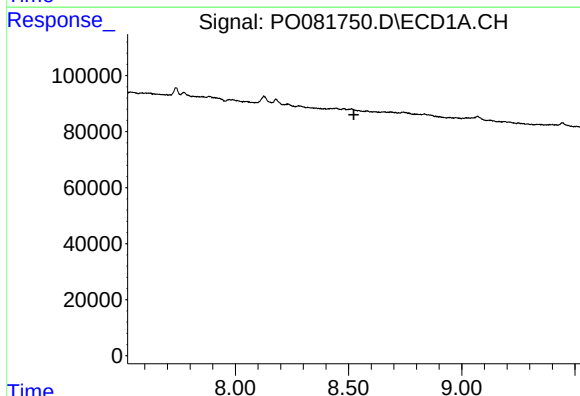

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.523 min
Response: 0
Conc: N.D.

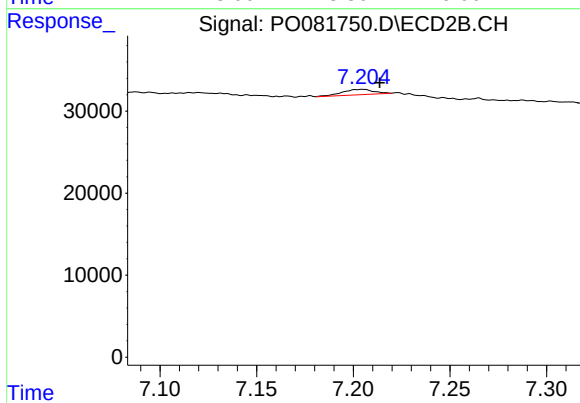

#33 AR-1260-3

R.T.: 7.205 min
Delta R.T.: -0.009 min
Response: 7268
Conc: 4.37 ng/ml