

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100421\
 Data File : P0081725.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 11:24
 Operator : AJ\MA
 Sample : M4040-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P287-DITCH

Manual Integrations
 APPROVED

mohammad
 10/5/2021 12:18:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.869	3.985	1271087	390645	14.254	14.663
2) SA Decachlor...	10.876	9.329	1106949	342323	14.861m	14.741

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100421\
Data File : P0081725.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 11:24
Operator : AJ\MA
Sample : M4040-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P287-DITCH


Manual Integrations
APPROVED

mohammad
10/5/2021 12:18:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

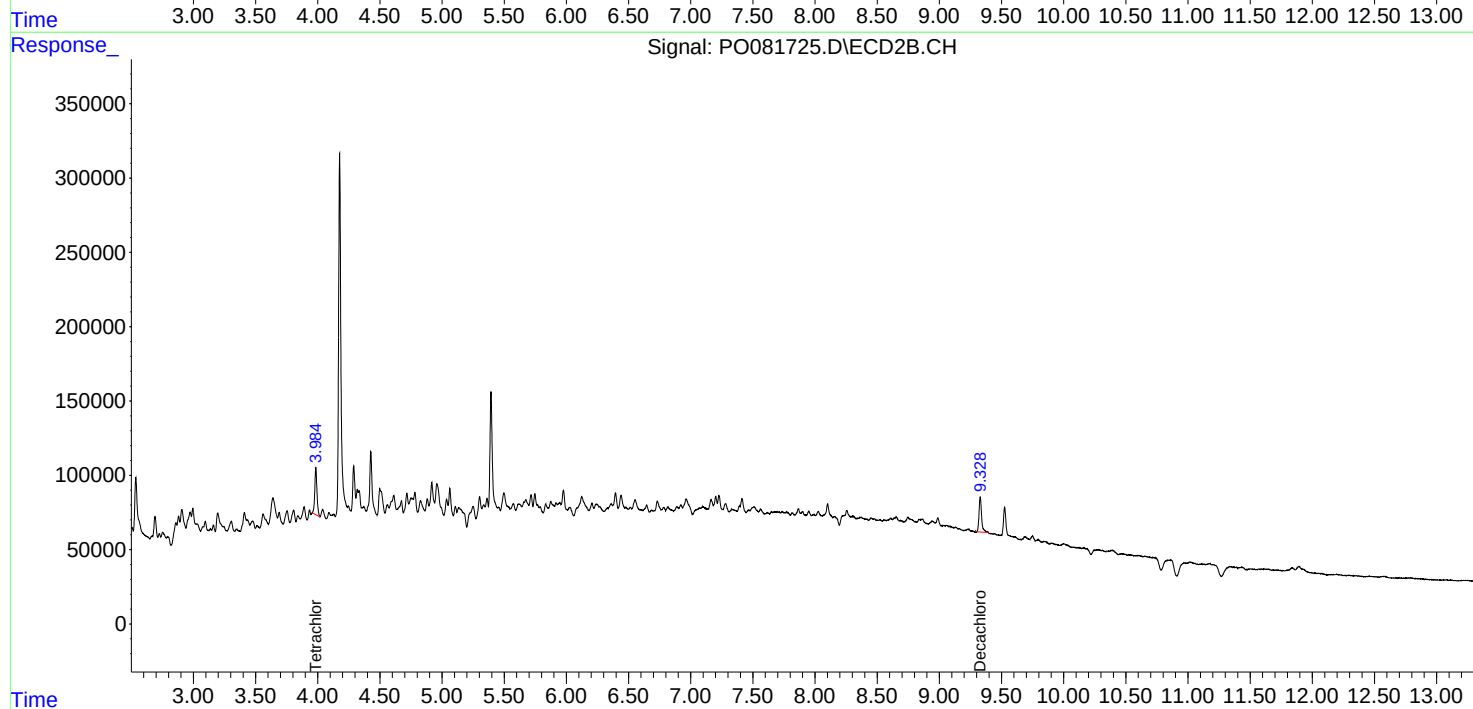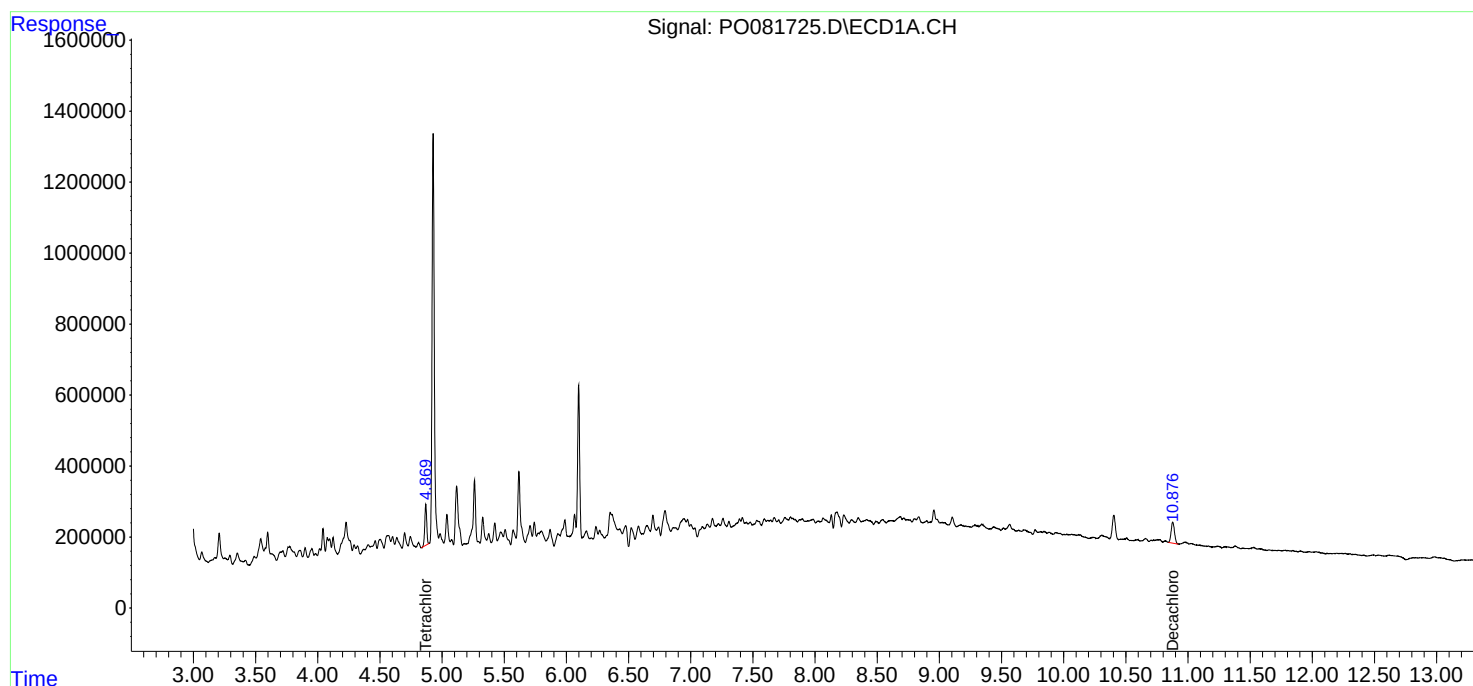

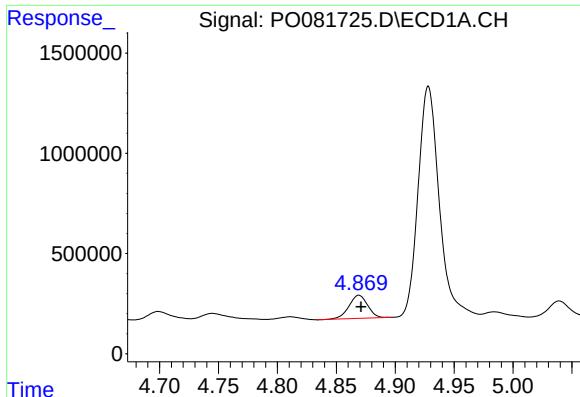


#1 Tetrachloro-m-xylene

R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 1271087
Conc: 14.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
P287-DITCH


Manual Integrations
APPROVED

mohammad
10/5/2021 12:18:07 PM

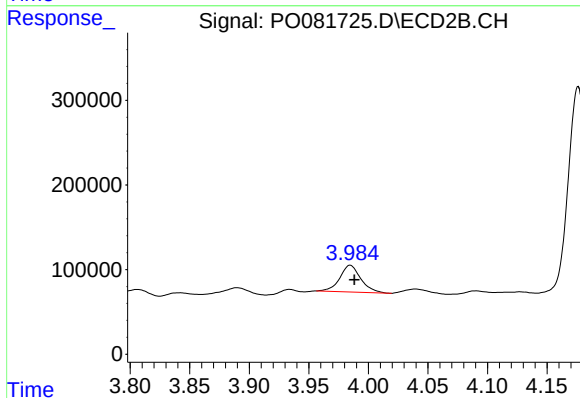


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: -0.004 min
Response: 390645
Conc: 14.66 ng/ml

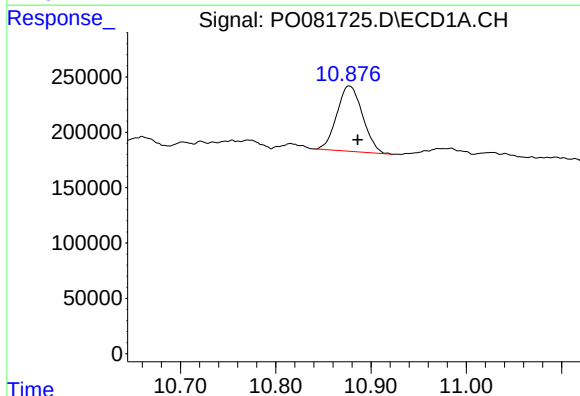

#2 Decachlorobiphenyl

R.T.: 10.876 min
Delta R.T.: -0.010 min
Response: 1106949
Conc: 14.86 ng/ml m

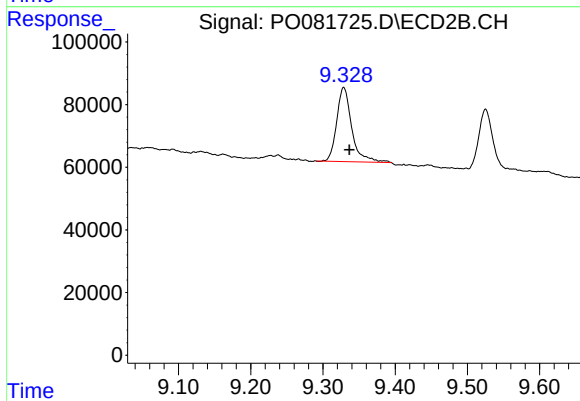

#2 Decachlorobiphenyl

R.T.: 9.329 min
Delta R.T.: -0.008 min
Response: 342323
Conc: 14.74 ng/ml