

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0100421\
 Data File : P0081728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Oct 2021 12:16
 Operator : AJ\MA
 Sample : M4020-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S-819-N-SO-2-2.5-093021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:05:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	3.984	2273001	655672	25.489	24.611
2) SA Decachlor...	10.878	9.328	1718740	540886	23.074	23.291

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO100421\
Data File : PO081728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Oct 2021 12:16
Operator : AJ\MA
Sample : M4020-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S-819-N-SO-2-2.5-093021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:05:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

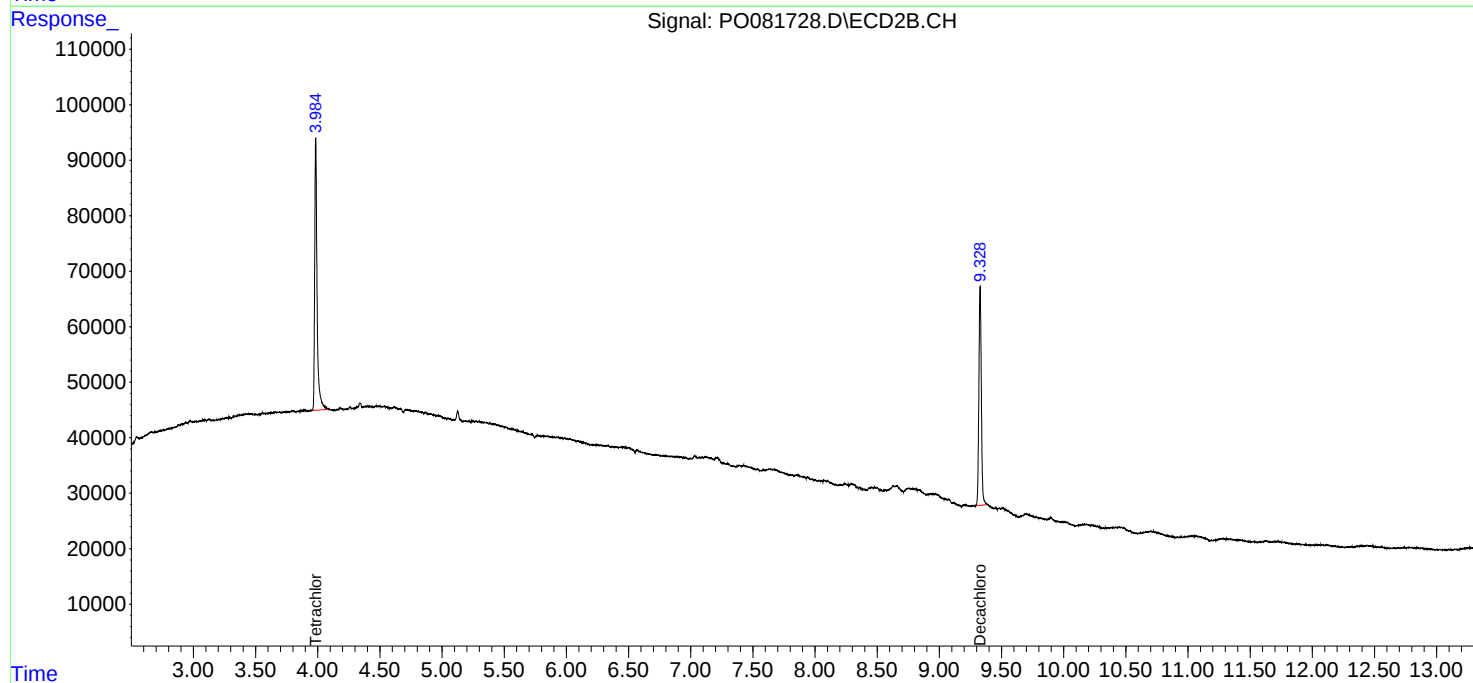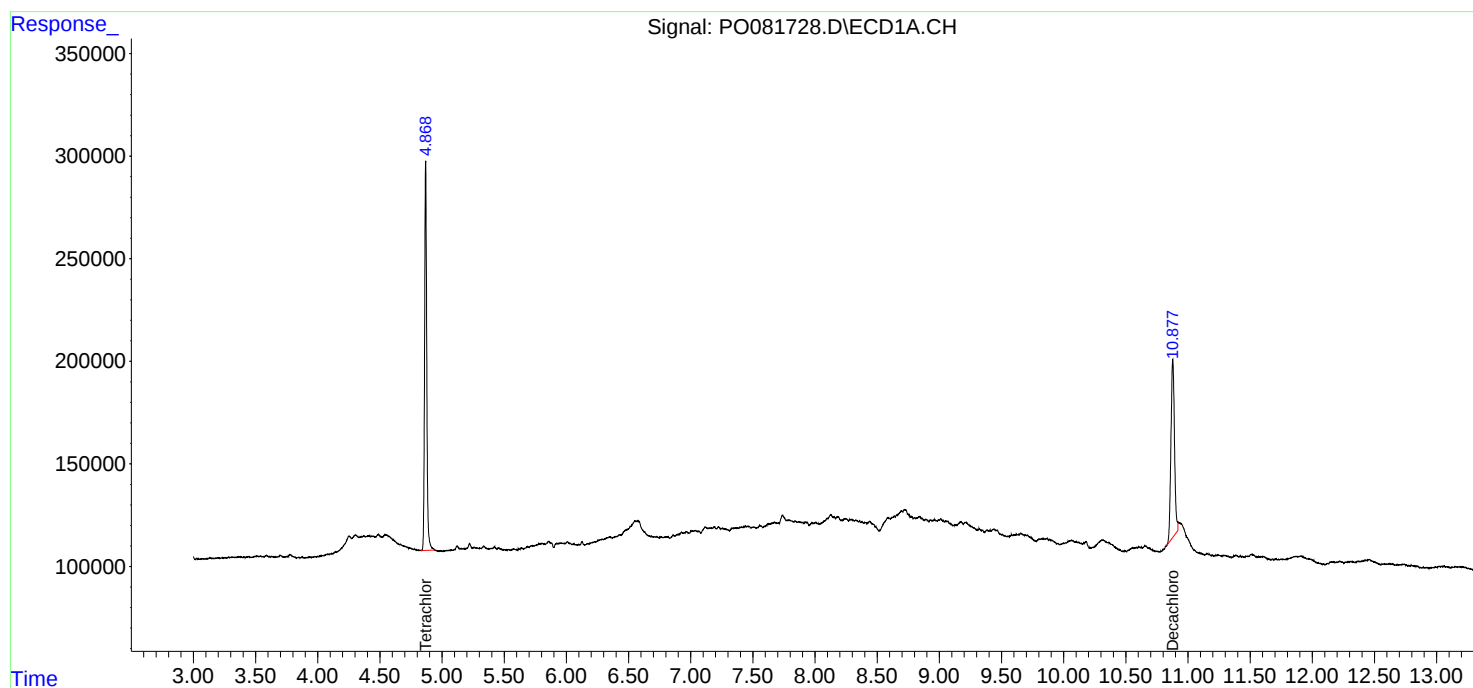


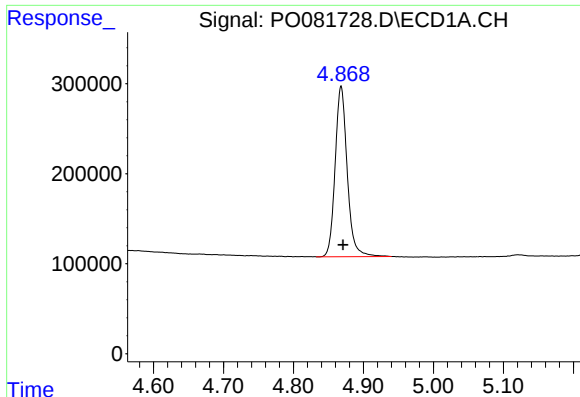

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.003 min
Response: 2273001
Conc: 25.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S-819-N-SO-2-2.5-093021

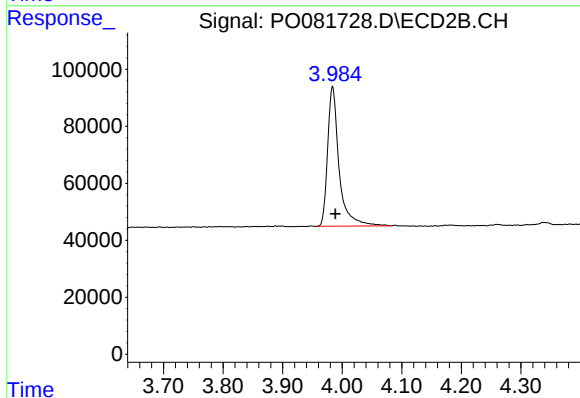


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.004 min
Response: 655672
Conc: 24.61 ng/ml

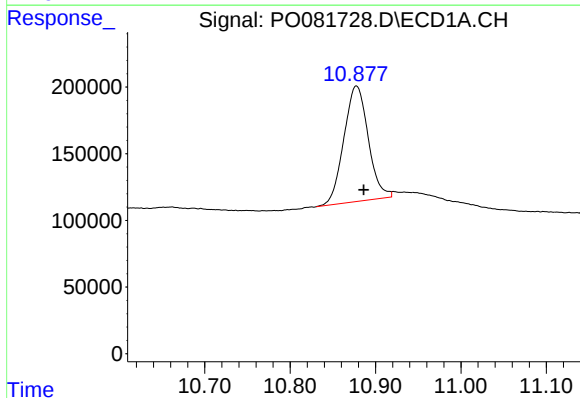

#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.009 min
Response: 1718740
Conc: 23.07 ng/ml

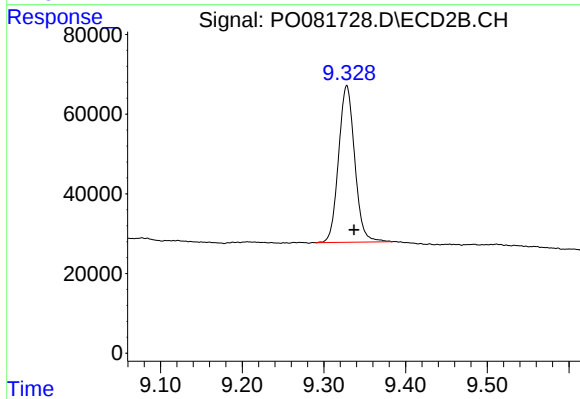

#2 Decachlorobiphenyl

R.T.: 9.328 min
Delta R.T.: -0.009 min
Response: 540886
Conc: 23.29 ng/ml